




Product Catalog
CONOLOG[®] Implant System

Valid from August 2023

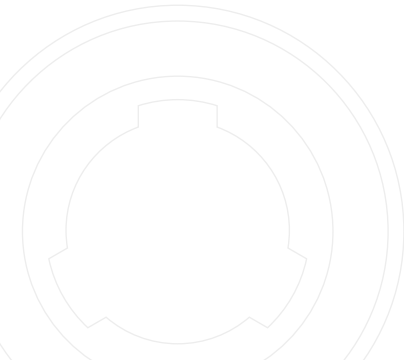

Content

Service

Clinical evidence and Science	2
-------------------------------	---

System information

The CONELOG® Implant System	3
-----------------------------	---

Surgery

Planning	18
PROGRESSIVE-LINE Implants and Instruments	20
PROGRESSIVE-LINE Guide System Instruments	26
PROGRESSIVE-LINE Flex Instruments	33
SCREW-LINE Implants and Instruments	37
SCREW-LINE Guide System Instruments	45
General Surgical Instruments	48
SCREW-LINE Osteotomy Sets	57
Cover Screws	62
Healing Caps	62

Prosthetics

Scanbody	64
Impression Taking	65
Bite Registration	66
Cast Fabrication	66
Temporary Abutments	67
CAD/CAM Prosthetics	68
CAM Blanks	70
Esthomic® Abutments	72
Universal Abutments	74
Gold-plastic Abutment	74
COMFOUR® System	76
Ball Abutment Anchoring System	81
Locator® Anchoring System	82
Double Crown Restoration	87
Accessories for Abutments	87
Prosthetic Instruments	88
Instruments for Dental Technicians	92
Selection Abutments	93

Auxiliary Articles

Implants for Practice	96
Insertion Posts	96
Demonstration Models	97
Macro Models	97
Literature	98

Additional Information

Indication Overview	102
Implant Overview	104
Prosthetic Overview	106
Screw Overview	112, 114
Overview Auxiliary Screws	113
Overview Tightening Torques	116
Materials	118

Index

Alphabetical	120
Article Number	124

Further Information

Further Documentation	136
Legal	136

Clinical evidence and Science

From the beginning on, the Camlog company has set high standards in scientific documentation of all essential properties of their implant systems.

In **Clinical evidence and Science**, we have summarized the current state of research on Camlog Implant Systems.

We are happy to pass on this concentrated knowledge to you. You are also welcome to request printed version.



www.biohorizonscamlog.com/clinical-evidence-and-science



The CONELOG® Implant System



The CONELOG® Implant System is based on years of clinical and laboratory experience and is a user-friendly, prosthetically oriented implant system.

All CONELOG® Products are manufactured with the latest state-of-the-art technology. The CONELOG® Implant System is continuously developed by the company's research and development team in collaboration with clinics, universities and dental technicians and therefore stays abreast of the latest technology.

The CAMLOG® and CONELOG® Implant Systems are very well documented scientifically. Studies* support this with respect to many parameters including the implant surface, time of implantation and/or implant loading, primary stability, and the connection design.

* See "Further documentation" on page 136

CONELOG® PROGRESSIVE-LINE Implants

The CONELOG® PROGRESSIVE-LINE Implants make it easier to implement modern treatment concepts such as immediate restorations or immediate loading, which require high primary stability [1, 2]*.

The geometry of the implant is consistently designed to develop high initial stability:

- The self-tapping screw implant has a conically shaped apical area that enables pronounced primary stability even in soft bone [1, 2]*.
- Thread extending to the apex for good anchorage in immediate implantations [1, 2]*.
- Crestal thread for improved hold with limited bone height [2]*.

CONELOG® PROGRESSIVE-LINE Implants are available with the Promote® plus Surface which extends over the entire implant body up to the acid-etched conical 45° implant shoulder. Depending on the clinical situation, this surface design thus permits slightly subcrestal implant positioning in the sense of a classic bone level implant.

CONELOG® PROGRESSIVE-LINE Implants with screw-mounted insertion post can be used for template-guided implant dentistry.


CONELOG® PROGRESSIVE-LINE Implants feature the high-precision, conical CONELOG® Implant-abutment connection with integrated Platform Switching. Prosthetic restoration is performed with CONELOG® Abutments.

* See "Further documentation" on page 136



CONELOG® PROGRESSIVE-LINE Implant, Promote® plus

Implant diameter

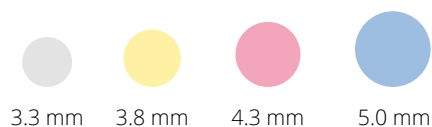

3.3 mm

3.8 mm

4.3 mm

5.0 mm

Implant lengths



7 mm

9 mm

11 mm

13 mm

16 mm

Promote® Surface

CONELOG® Implants are available with the abrasive-blasted, acid-etched Promote® Surface. The surface is based on current scientific knowledge and supports rapid osseointegration. Scientific results from studies with cell cultures, osteohistology and in pull-out trials illustrate this impressively.

CONELOG® SCREW-LINE Implants

CONELOG® SCREW-LINE Implants are slightly conical, self-tapping screw implants. They enable easy insertion by self-centering with continuous bone contact and thus achieve solid primary stability.

CONELOG® Implants are available with the abrasive-blasted, acid-etched Promote® Surface up to the acid-etched conical 45° implant shoulder and thus allow for maximum flexibility when determining the vertical implant position. Rounding of the apical geometry ensures gentle insertion of the CONELOG® SCREW-LINE Implants into the bone, also near the maxillary sinus.


CONELOG® SCREW-LINE Implants with screw-mounted insertion post can be used for template-guided implant dentistry.

CONELOG® PROGRESSIVE-LINE Implants feature the high-precision, conical CONELOG® Implant-abutment connection with integrated Platform Switching. Prosthetic restoration is performed with CONELOG® Abutments.



**CONELOG® SCREW-LINE
Implant, Promote® plus**

Implant diameter

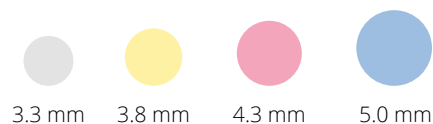

3.3 mm 3.8 mm 4.3 mm 5.0 mm

Implant lengths




All CONELOG® Implants are delivered pre-assembled in sterile packaging on a color-coded insertion post corresponding to the diameter.



The insertion posts of the CONELOG® Implants

The PROGRESSIVE-LINE and SCREW-LINE Implants are each offered with two different versions of the insertion post. Regardless of which option you choose, the instruments used to insert the implant are identical. A separate set of instruments for guided surgery is not required.

- Pre-assembled transfer part – simplified application and transfer to the patient's mouth
- Small diameter – easy access to the interdental spaces and posterior region
- Color-coded insertion post according to diameter – provides easy orientation during surgery
- Can be used as a paralleling pin – for aligning the position of multiple implants

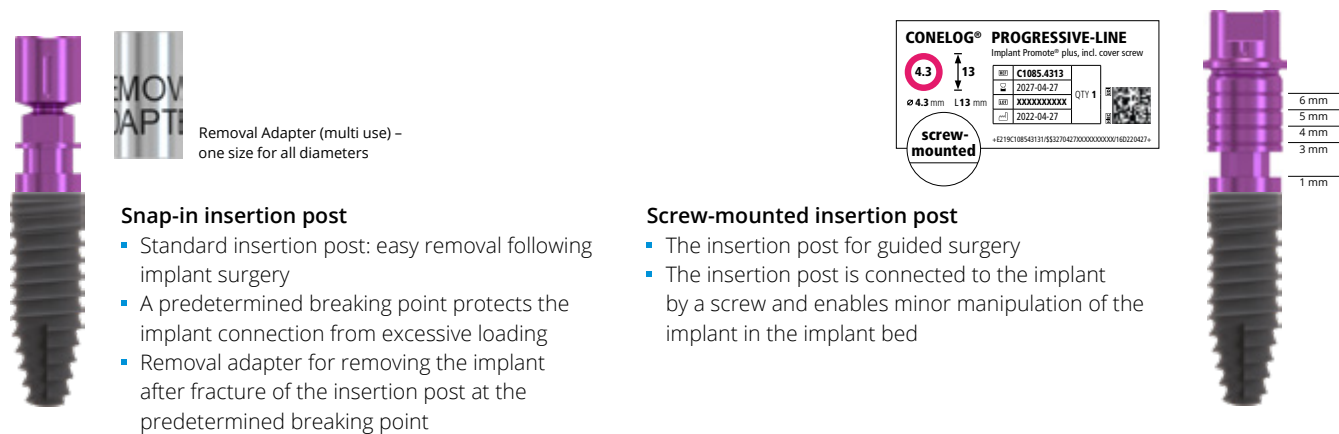

Snap-in insertion post

- Standard insertion post: easy removal following implant surgery
- A predetermined breaking point protects the implant connection from excessive loading
- Removal adapter for removing the implant after fracture of the insertion post at the predetermined breaking point

Screw-mounted insertion post

- The insertion post for guided surgery
- The insertion post is connected to the implant by a screw and enables minor manipulation of the implant in the implant bed

CONELOG® Implant-abutment connection

The geometry of the CONELOG® Implant-abutment connection enables integrated Platform Switching and provides excellent tactile feedback when inserting the abutments.

Indexing via the three grooves/cams allows the cams to slide noticeably into the grooves of the implant and thus into the final position when the abutment is rotated slightly. Simple, easy and safe orientation in the longitudinal axis of the implant is thus ensured. The precise conical connection minimizes micro-movements and demonstrates superior stability compared to other conical connections [3, 4]*.


* See "Further documentation" on page 136.

Advantages and benefits of the CONELOG® Connection

- Simple, fast and precise abutment positioning with clearly noticeable tactile feedback
- Precise, conical implant-abutment connection with superior stability compared to other conical connections^{1,2*}
- Integrated Platform Switching

For optimal positioning of the abutments, the implant should be aligned in the bone so that one of the three grooves points in vestibular direction. With the CONELOG® Implants, the insertion tools include markings that correspond to the three grooves of the implant inner configuration.

* See "Further documentation" on page 136.

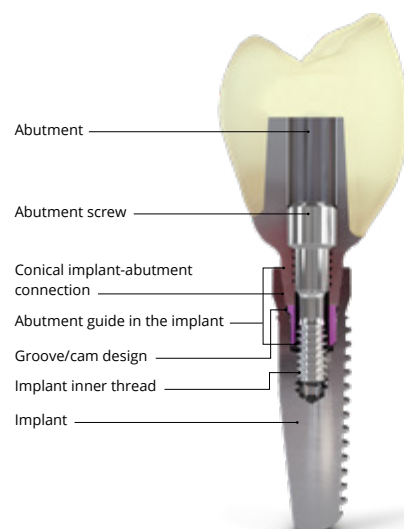

CONELOG® Prosthetic components

The CONELOG® Implants can be provided with a wide range of flexible, anatomically adapted prosthetic components. CONELOG® Abutments are color-coded according to the implant diameters.

Effect of the Platform Switching design

The CONELOG® Implant System offers integrated Platform Switching as the implant shoulder is not covered by the healing caps and abutments. Platform Switching is used to support the hard and soft tissue in the peri-implant esthetic region. The distance between the implant-abutment interface and the alveolar crest is increased and thereby reduces the effect of inflammatory cell infiltration with concomitant bone resorption.



CONELOG® Healing caps

CONELOG® Healing caps sit on the machined implant shoulder, but do not cover it completely. As a result, the soft tissue over the shoulder can be adapted. The conical surfaces do not come into contact.

The healing caps are used according to their indication for single and two-stage procedures. The healing caps are available in three geometries (cylindrical, wide body and bottleneck) and are screwed directly into the implant.

CONELOG® Impression taking

Impression-taking of the CONELOG® Implants is possible with impression posts, open or closed tray. All impression-taking components are color-coded based on the implant diameter. High-precision components ensure correct transfer of the intraoral situation.

The CONELOG® Impression posts do not lock into the cone of the implant, but lie on the implant shoulder. Thus, a vertical offset is prevented when taking the impression. The antirotational mechanism is ensured by the CONELOG® groove/cam geometry.





CONELOG® Temporary abutments


CONELOG® Temporary abutments made of titanium alloy are available for temporary restorations in crown and bridge versions. The abutments can be used in immediate implantations or after exposing the gingiva.

CONELOG® Esthomic® Abutments

Anatomically preformed abutments allow for optimal stump design. The CONELOG® Esthomic® Abutments are available both straight and angled with various gingival heights and with an oval anatomically pre-shaped shoulder profile. The angled Esthomic® Abutments are available in A and B versions differentiated by a cam offset of 60°. This results in six prosthetic-oriented rotating positions and allows perfect prosthetic alignment of the axes.




CONELOG® Esthomic® Abutment cam alignment

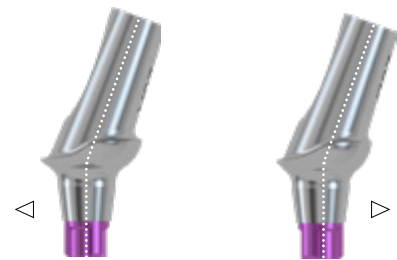

Type A
Cam alignment against the angle

Type B
Cam alignment in direction of the angle

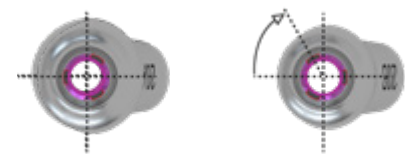

Type A

Type B
Cams with 60° offset

CONELOG® Disconnecter for CONELOG® Abutments

The CONELOG® Implant-abutment connection is characterized by a self-locking taper. A special CONELOG® Disconnecter is available for the easy removal of CONELOG® Abutments from CONELOG® Implants or lab analogs. First, the CONELOG® Abutment screw or the lab screw is removed and the disconnecter is screwed into the screw canal until the abutment releases from the internal taper of the CONELOG® Implant or lab analog.



CONELOG® Universal and telescope abutments

CONELOG® Universal and telescope abutments can be used for individually fabricated cementable crown and bridge restorations and for double crown restorations. The abutments are made of titanium alloy and can be custom trimmed.


CONELOG® Titanium bases CAD/CAM

CONELOG® Titanium bases CAD/CAM act as a bonding basis for customized, implant-supported dental restorations made of suitable materials. Reconstructions are fabricated with the aid of CAD/CAM techniques. CONELOG® Titanium bases CAD/CAM are available in crown and bridge versions, each with gingival heights of 1.0 and 2.0 mm.



CONELOG® Ball, Locator® and straight bar abutments

Ball, Locator® and straight bar abutments are available for the CONELOG® Implant System. These differ from the abutments in the apical area through different connection designs. Ball, Locator® and straight bar abutments are manufactured as single units with a thread in the apical region which engages with the inner thread of the CONELOG® Implant. These abutments are screwed into the CONELOG® Implant using the corresponding insertion tools.

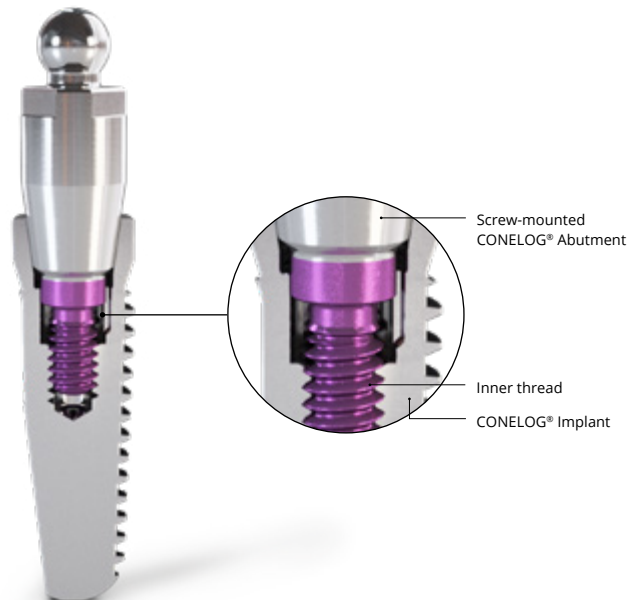


**Example: CONELOG® Ball abutment (Ø 4.3 m)
in a CONELOG® SCREW-LINE Implant**

COMFOUR® System

Occlusal screw-mounted restorations are state-of-the-art. With the COMFOUR® System, edentulous patients are given the option of immediate, comfortable, and fixed dentures based on four or six implants as a rule, with a huge gain in their quality of life. Clinicians too can look forward to considerably greater comfort and freedom. COMFOUR® provides several treatment options. In addition to occlusal screw-mounted crowns and bridges for immediate and delayed restorations, the multi-option system also permits bar restorations on straight and angled bar abutments. COMFOUR® offers a range of options to master the challenges faced in routine practice with greater ease and in less time.

Next to its versatility, the COMFOUR® Prosthetic System is particularly impressive thanks to its slim design.

All components are of a delicate and low design, which simplifies prosthetic restorations considerably for dentists and dental technicians. In addition, a number of technical highlights ensure that COMFOUR® is not simply just a name but also a program—for users and patients alike.

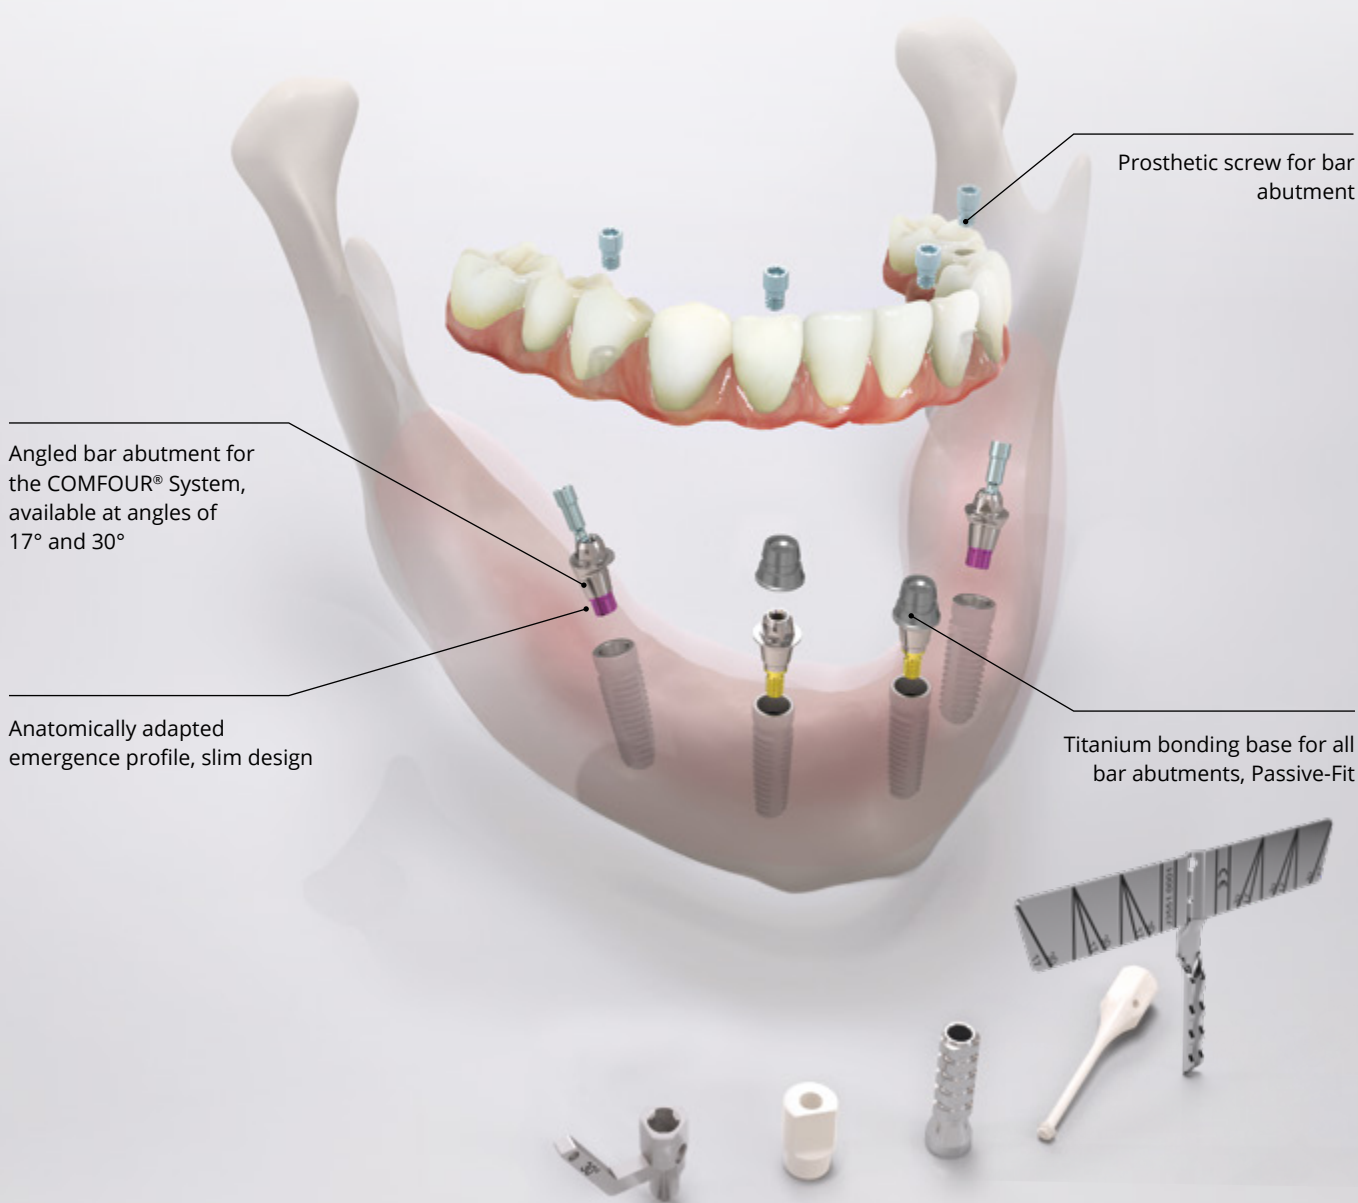

COMFOUR® offers a large selection of options to manage the requirements of your practice.

CAD/CAM services

Individually CAD/CAM fabricated prosthetics, healing caps and impression posts, scanning and design services, 3D implant planning, printed drilling templates and jaw models are available from Camlog through our DEDICAM® Service Division.

Personal support with the accustomed competence of our employees as well as processes optimized right down to the finest detail ensure a high degree of certainty of results with the greatest possible individual freedom.
























Extensive libraries for the open CAD systems from 3Shape, exocad and Dental Wings are available for implant-supported restorations.



DEDICAM® DIGITAL CONCEPTS

Discover your options and start your digital future with DEDICAM®.
DEDICAM® Services are not available in all countries. Please ask your local Camlog representative for details.


Explanation of symbols

	CE marking
	CE marking with number of the Notified Body
	Consult Instructions for Use
	Caution, observe the warning notices
	Medical Device
	Article number
	Lot number
	Serial number
	Sterilized using irradiation
	Single sterile barrier system with protective packaging outside
	Single sterile barrier
	Non-sterile
	Date of manufacture
	Use-by date
	Do not resterilize
	Do not reuse
	Do not use if package is damaged
	Protect against sunlight
	Temperature limit
	Manufacturer
	MR Conditional
	Contains hazardous substances
	Caution: US Federal law restricts this device to sale by or on the order of a dentist or physician.

Explanation of abbreviations

\varnothing	Diameter
A \varnothing	Apical diameter
G \varnothing	Gingival diameter
PP \varnothing	Prosthetic platform diameter
L	Length
GH	Gingival height
PEEK	Poly ether ether ketone
POM	Polyoxymethylene
PPSU	Polyphenylsulfone

Color coding of the surgical and prosthetic CONELOG® Products

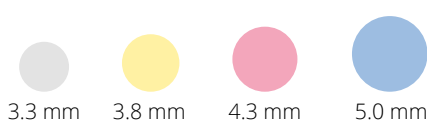

General safety instructions and warnings

- The descriptions in this product catalog are not sufficient to allow immediate use of the CONELOG® Implant System.
- Instruction by a surgeon experienced in using the CONELOG® Implant System is strongly recommended. CONELOG® Products may only be applied by dentists, physicians, surgeons and dental technicians trained on the system. Appropriate courses and training sessions are offered by Camlog.
- Methodical errors made during the treatment can result in loss of the implant and significant loss of the peri-implant bone.
- The images in this document are for reference purposes only and may differ from the actual product.

Packaging of PROGRESSIVE-LINE Implants

Secondary packaging


Sealed, folding box with color-coded product label

Inner implant packaging (primary packaging)

Sealed, color-coded



Example of product label for outer packaging of the implant

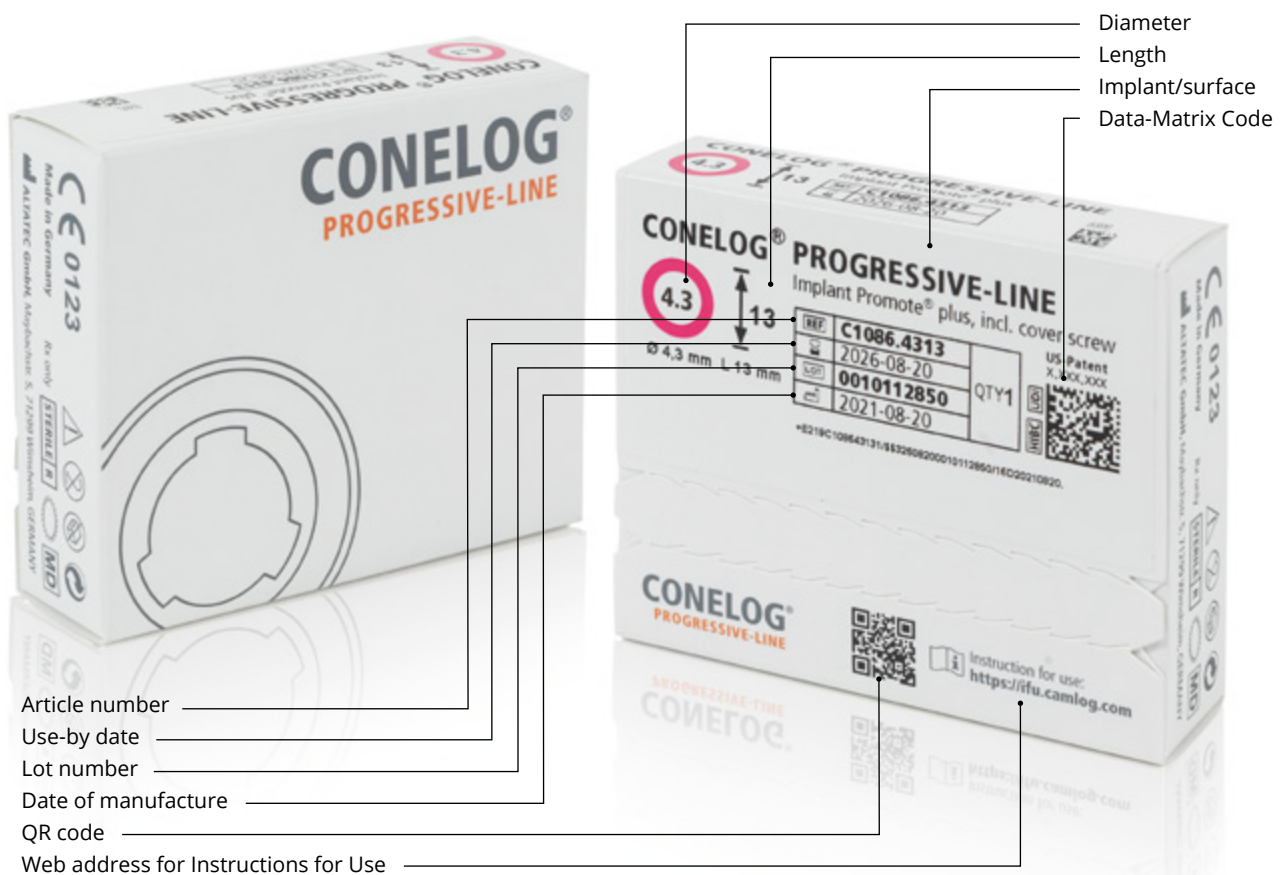



New

Direct part marking – better identification and traceability






In future, all Camlog instruments will feature a label with the lot number and/or UDI code in addition to the article number. This makes it easier for the entire practice team to identify and assign the products. The product images contained in the catalog do not yet always reflect this specification.

Surgery





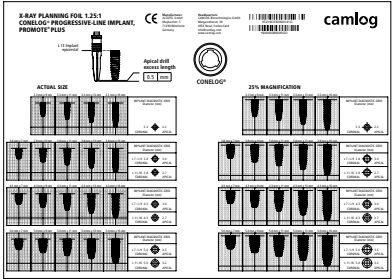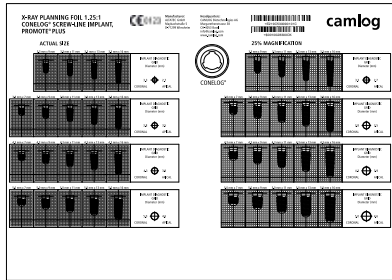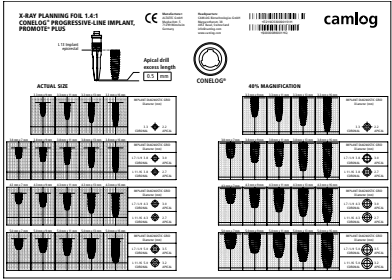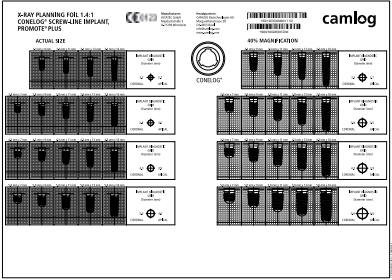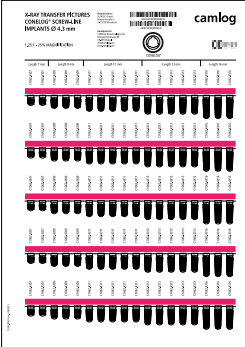

Planning

X-Ray Planning foils and X-Ray Transfer pictures

	Article	Art. No.	Ø
	<p>X-Ray Planning foil 1.25:1 CONELOG® PROGRESSIVE-LINE Implants Magnification 25 %</p>	C5300.9014	-
	<p>X-Ray Planning foil 1.25:1 CONELOG® SCREW-LINE Implants Magnification 25 %</p>	C5300.9010	-
	<p>X-Ray Planning foil 1.4:1 CONELOG® PROGRESSIVE-LINE Implants Magnification 40 %</p>	C5300.9015	-
	<p>X-Ray Planning foil 1.4:1 CONELOG® SCREW-LINE Implants Magnification 40 %</p>	C5300.9011	-
	<p>X-Ray Transfer pictures 1.25:1 CONELOG® SCREW-LINE Implants Planning foils, self-adhesive Magnification 25 %</p>	C5300.9080	3.3 mm
		C5300.9081	3.8 mm
		C5300.9082	4.3 mm
		C5300.9083	5.0 mm


CT-Planning

for 3D X-ray and drilling templates

	Article	Art. No.	L
	Tubing for CT planning for drill Ø 2.0 mm*, corrugated tubing (10 units) internal diameter 2.1 mm external diameter 2.5 mm Material Titanium alloy	A2002.2000	4.0 mm 10.0 mm
	Tubing for CT planning for drill Ø 2.2 mm, corrugated tubing (10 units) internal diameter 2.3 mm external diameter 2.7 mm Material Titanium alloy	A2222.2200	4.0 mm 10.0 mm
	Drill for placement of corrugated CT-tubes (for A2002.2000) Ø 2.6 mm Material Stainless steel	A2050.2600	-
	Drill for placement of corrugated CT-tubes (for A2222.2200) Ø 2.8 mm Material Stainless steel	A2050.2800	-


* for pilot drills J5051.2003 and pilot drills SCREW-LINE J5051.2000

PROGRESSIVE-LINE

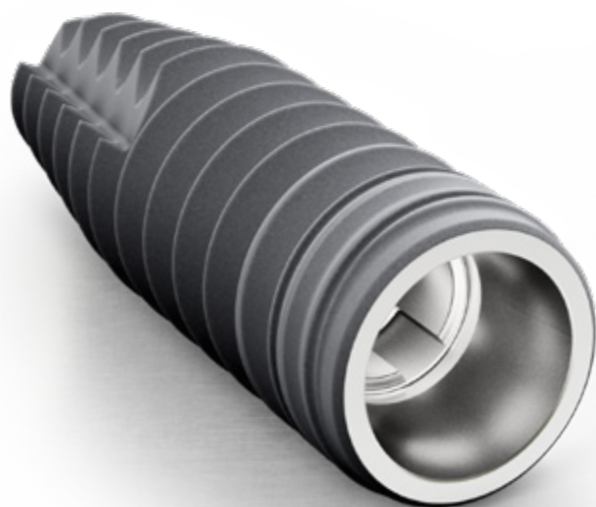


PROGRESSIVE-LINE

Implants with snap-in insertion posts

	Article	Art. No.	Ø	L	A Ø	
	CONELOG® PROGRESSIVE-LINE Implant, Promote® plus incl. snap-in insertion post and cover screw, sterile Material Titanium Grade 4	C1086.3309	3.3 mm	9 mm	2.2 mm	
		C1086.3311		11 mm		
		C1086.3313		13 mm		
		C1086.3316		16 mm		
		C1086.3807	3.8 mm	7 mm	3.0 mm	
		C1086.3809		9 mm		
		C1086.3811		11 mm		
		C1086.3813		13 mm		
		C1086.3816	16 mm	2.7 mm		
		C1086.4307	4.3 mm		7 mm	3.0 mm
		C1086.4309			9 mm	
		C1086.4311			11 mm	
		C1086.4313		13 mm		
		C1086.4316	16 mm	2.7 mm		
		C1086.5007	5.0 mm		7 mm	3.5 mm
		C1086.5009			9 mm	
		C1086.5011			11 mm	
		C1086.5013		13 mm		
C1086.5016	16 mm	3.2 mm				

Surgery


Implants with screw-mounted insertion posts

	Article	Art. No.	Ø	L	A Ø	
	CONELOG® PROGRESSIVE-LINE Implant, Promote® plus incl. screw-mounted insertion post and cover screw, sterile Material Titanium Grade 4	C1085.3309	3.3 mm	9 mm	2.2 mm	
		C1085.3311		11 mm		
		C1085.3313		13 mm		
		C1085.3316		16 mm		
		C1085.3807	3.8 mm	7 mm	3.0 mm	
		C1085.3809		9 mm		
		C1085.3811		11 mm		
		C1085.3813		13 mm		
		C1085.3816	16 mm	2.7 mm		
		C1085.4307	4.3 mm		7 mm	3.0 mm
		C1085.4309			9 mm	
		C1085.4311			11 mm	
		C1085.4313		13 mm		
		C1085.4316	16 mm	2.7 mm		
		C1085.5007	5.0 mm		7 mm	3.5 mm
		C1085.5009			9 mm	
		C1085.5011			11 mm	
		C1085.5013		13 mm		
C1085.5016	16 mm	3.2 mm				

Note
 Implants with the screw-mounted insertion post (Art. No. C1085.xxxx) are to be used for template-guided implant insertion with the PROGRESSIVE-LINE Guide System.

PROGRESSIVE-LINE

Surgery Set CAMLOG®/CONELOG®

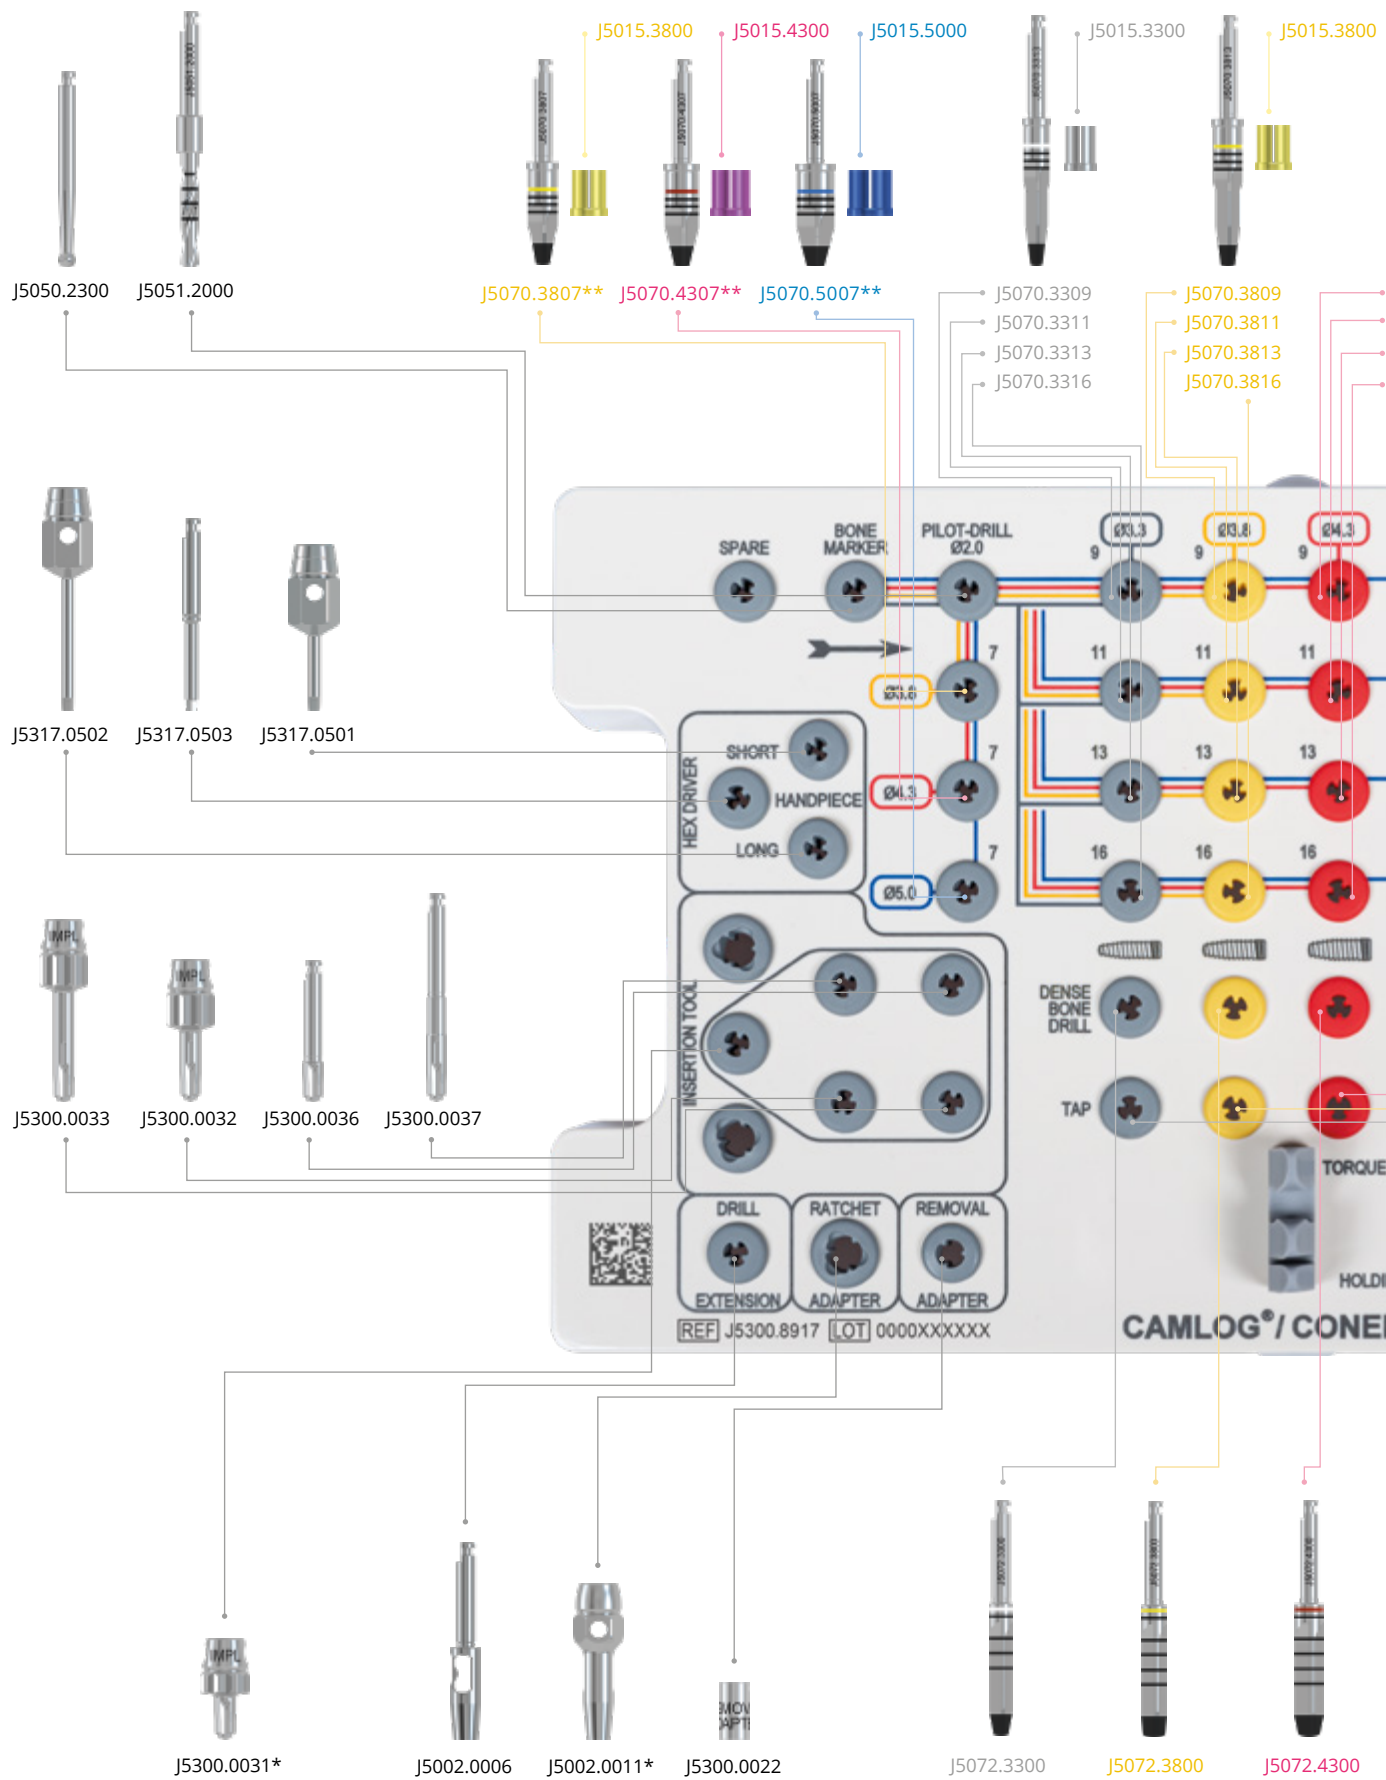

* These articles are not included in the surgery set and must be ordered separately.



Note

- The drills are arranged and sorted in the set according to the treatment sequence.
- Colored lines indicate the exact drilling sequence.

- J5070.4309
- J5070.4311
- J5070.4313
- J5070.4316
- J5070.5009
- J5070.5011
- J5070.5013
- J5070.5016



J5300.2000



J5015.0013



J5015.0011



J5015.0009




J5015.0007



J5320.1030




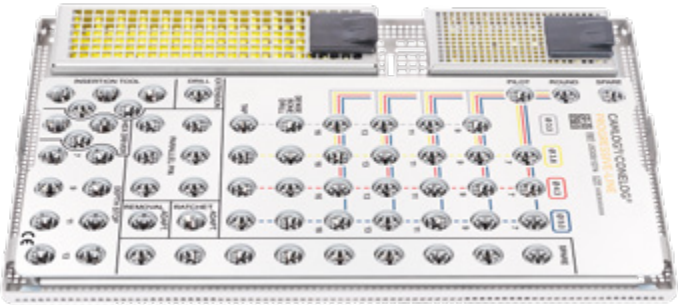
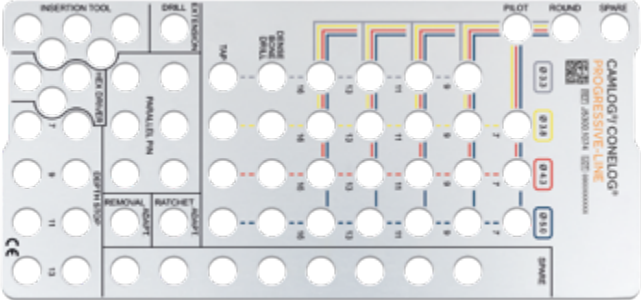
J5302.0010

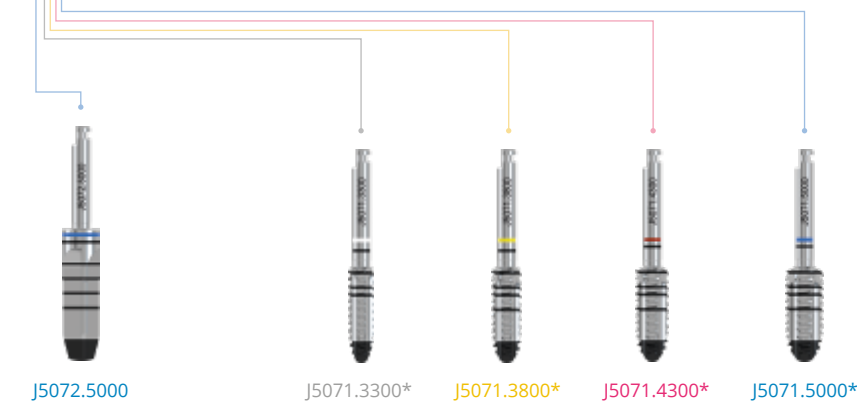

J5072.5000 J5071.3300* J5071.3800* J5071.4300* J5071.5000*






PROGRESSIVE-LINE

Surgery set and wash tray

	Article	Art. No.
 <p>A white plastic surgery set tray containing various surgical instruments organized by color-coded handles (blue, yellow, red, blue). The tray has a handle on the right side and the text 'CAMLOG® CONELOG® PROGRESSIVE-LINE' printed on the bottom.</p>	<p>Surgery Set CAMLOG®/CONELOG® PROGRESSIVE-LINE contains all necessary color-code ordered surgical instruments, incl. torque wrench and universal holding key (taps are not included)</p>	<p>J5300.0065</p>
 <p>A rectangular stainless steel wash tray with a grid of circular holes for instruments. It features a color-coded layout with labels for different instrument types and sizes. The text 'CAMLOG®/CONELOG® PROGRESSIVE-LINE' is visible on the right side.</p>	<p>Surgery wash tray CAMLOG®/CONELOG® PROGRESSIVE-LINE incl. pattern, without content</p>	<p>J5300.8970</p>
 <p>A stainless steel pattern for the surgery wash tray, showing the layout of circular holes and their dimensions. It includes labels for different instrument types such as 'INSERTION TOOL', 'DRILL', 'PILOT', 'ROUND', and 'SPHERE'. The text 'CAMLOG®/CONELOG® PROGRESSIVE-LINE' is printed on the right side.</p>	<p>Pattern for surgery wash tray CAMLOG®/CONELOG® PROGRESSIVE-LINE Material Stainless steel</p>	<p>J5300.1074</p>

Preparation of the implant bed for CAMLOG® PROGRESSIVE-LINE Implants and for CONELOG® PROGRESSIVE-LINE Implants is performed with identical instruments.

Surgical instruments

	Article	Art. No.	Ø	L
	Form drills PROGRESSIVE-LINE resterilizable Material Stainless steel	J5070.3309	3.3 mm	9 mm
		J5070.3311		11 mm
		J5070.3313		13 mm
		J5070.3316		16 mm
		J5070.3807	3.8 mm	7 mm
		J5070.3809		9 mm
		J5070.3811		11 mm
		J5070.3813		13 mm
		J5070.3816	4.3 mm	16 mm
		J5070.4307		7 mm
		J5070.4309		9 mm
		J5070.4311		11 mm
		J5070.4313	5.0 mm	13 mm
		J5070.4316		16 mm
		J5070.5007		7 mm
		J5070.5009		9 mm
J5070.5011	5.0 mm	11 mm		
J5070.5013		13 mm		
J5070.5016		16 mm		
	Depth stop, for form drills PROGRESSIVE-LINE and SCREW-LINE resterilizable Material Titanium alloy	J5015.3300	3.3 mm	-
		J5015.3800	3.8 mm	
		J5015.4300	4.3 mm	
		J5015.5000	5.0 mm	
	Dense bone drill PROGRESSIVE-LINE resterilizable Material Stainless steel	J5072.3300	3.3 mm	-
		J5072.3800	3.8 mm	
		J5072.4300	4.3 mm	
		J5072.5000	5.0 mm	
	Tap PROGRESSIVE-LINE resterilizable Material Stainless steel	J5071.3300	3.3 mm	-
		J5071.3800	3.8 mm	
		J5071.4300	4.3 mm	
		J5071.5000	5.0 mm	
	Paralleling pin PROGRESSIVE-LINE with depth marks (for pilot drilling Ø 2.0 mm) Material Titanium alloy	J5300.2000	-	-


PROGRESSIVE-LINE Guide System






PROGRESSIVE-LINE Guide System



Surgery tray CAMLOG®/CONELOG®

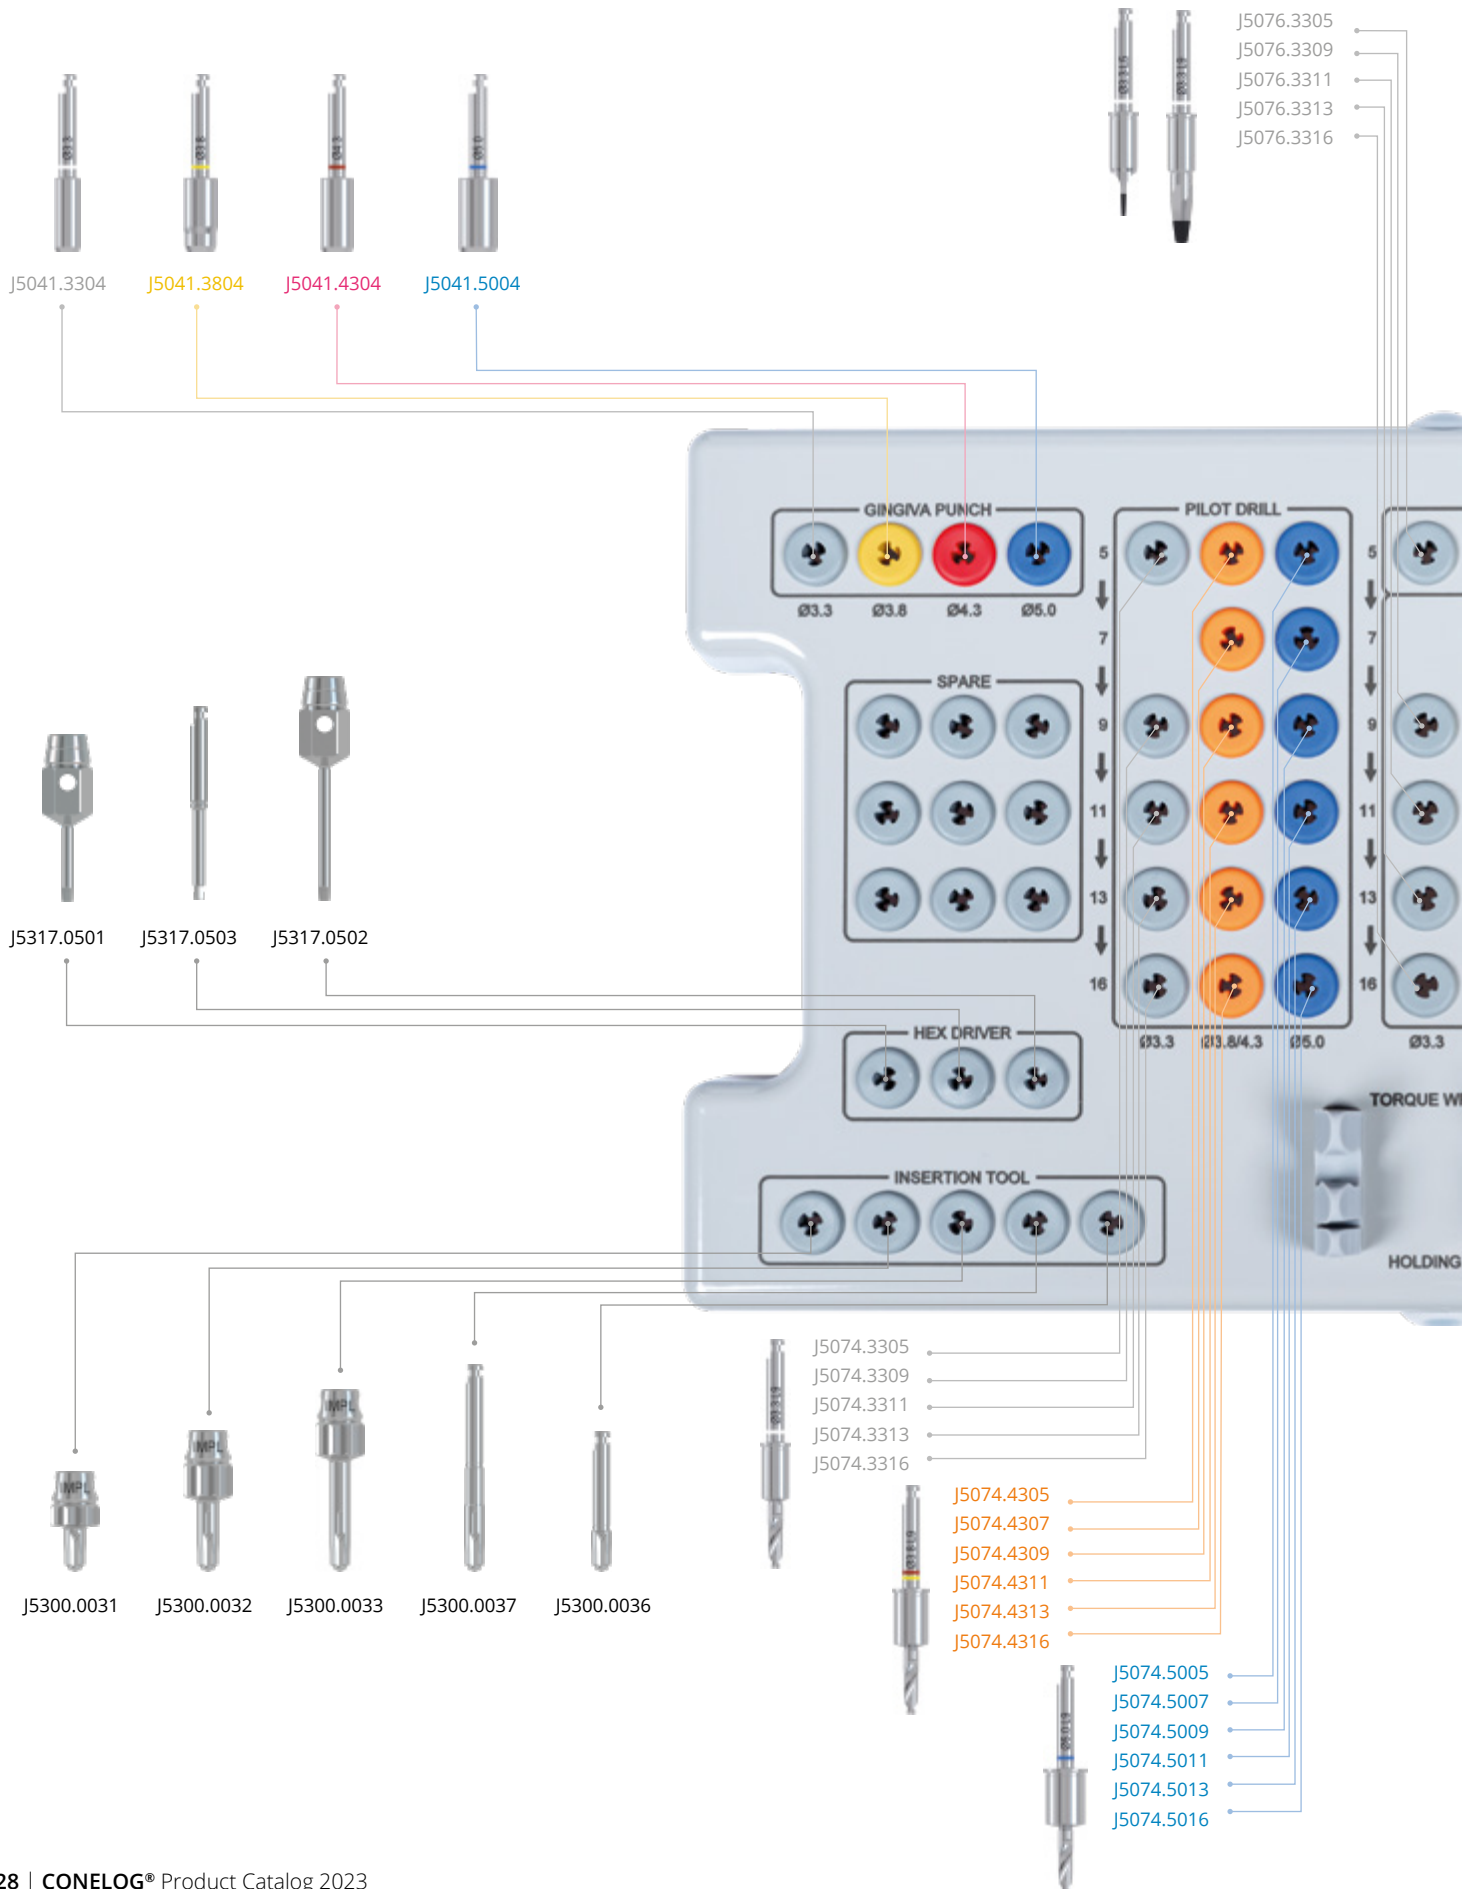

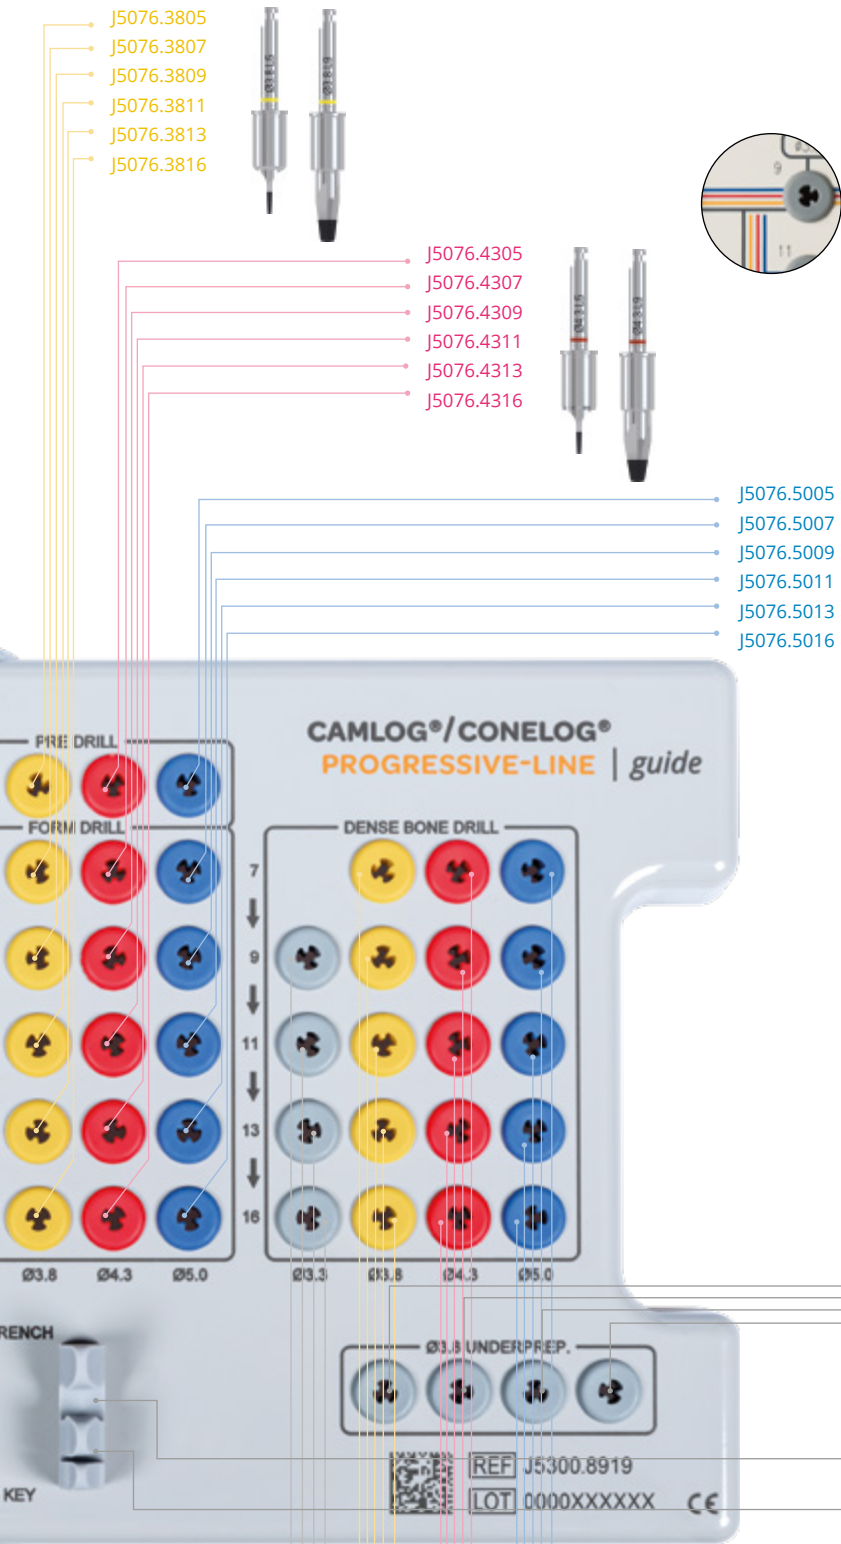

Note

- The drills are arranged and sorted in the set according to the treatment sequence.
- Colored lines indicate the exact drilling sequence.

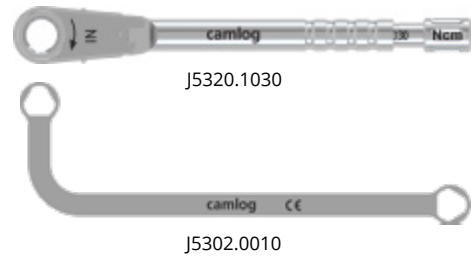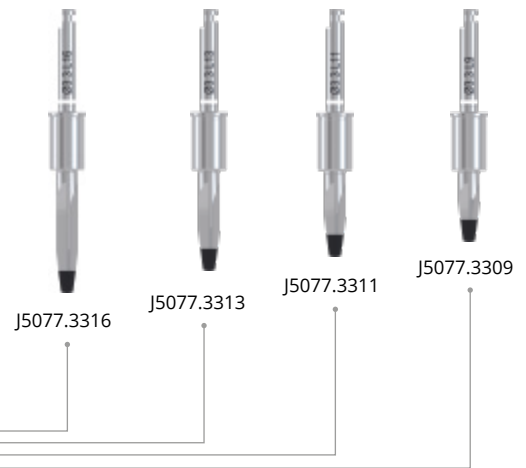

- J5078.3309**
J5078.3311
J5078.3313
J5078.3316
- J5078.3807**
J5078.3809
J5078.3811
J5078.3813
J5078.3816
- J5078.4307**
J5078.4309
J5078.4311
J5078.4313
J5078.4316
- J5078.5007**
J5078.5009
J5078.5011
J5078.5013
J5078.5016



PROGRESSIVE-LINE Guide System





Surgery and wash tray

	Article	Art. No.
	<p>Guide System surgery tray CAMLOG®/CONELOG® PROGRESSIVE-LINE without content</p>	<p>J5300.8919</p>
	<p>Guide System surgery wash tray CAMLOG®/CONELOG® PROGRESSIVE-LINE incl. pattern, without content</p> <p>Material Stainless steel</p>	<p>J5300.8971</p>
	<p>Guide System pattern for surgery wash tray CAMLOG®/CONELOG® PROGRESSIVE-LINE</p> <p>Material Stainless steel</p>	<p>J5300.1072</p>

Note




Implants with the screw-mounted insertion post (Art. No. C1085.xxxx) are to be used for template-guided implant insertion with the PROGRESSIVE-LINE Guide System.

Surgical instruments

	Article	Art. No.	Ø	L	
	Guide System gingiva punch PROGRESSIVE-LINE resterilizable Material Stainless steel	J5041.3304	3.3 mm	-	
		J5041.3804	3.8 mm		
		J5041.4304	4.3 mm		
		J5041.5004	5.0 mm		
	Guide System pilot drills PROGRESSIVE-LINE resterilizable Material Stainless steel	J5074.3305	3.3 mm	5 mm	
		J5074.3309		9 mm	
		J5074.3311		11 mm	
		J5074.3313		13 mm	
		J5074.3316		16 mm	
		J5074.4305	3.8 mm	4.3 mm	5 mm
		J5074.4307			7 mm
		J5074.4309	5.0 mm		9 mm
		J5074.4311			11 mm
		J5074.4313			13 mm
		J5074.4316			16 mm
		J5074.5005	5.0 mm		5 mm
		J5074.5007			7 mm
		J5074.5009			9 mm
		J5074.5011			11 mm
		J5074.5013			13 mm
J5074.5016	16 mm				
	Guide System pre-drill PROGRESSIVE-LINE resterilizable Material Stainless steel	J5076.3305	3.3 mm	5 mm	
		J5076.3805	3.8 mm		
		J5076.4305	4.3 mm		
		J5076.5005	5.0 mm		
	Guide System form drills PROGRESSIVE-LINE resterilizable Material Stainless steel	J5076.3309	3.3 mm	9 mm	
		J5076.3311		11 mm	
		J5076.3313		13 mm	
		J5076.3316		16 mm	
		J5076.3807	3.8 mm		7 mm
		J5076.3809			9 mm
		J5076.3811			11 mm
		J5076.3813			13 mm
		J5076.3816			16 mm
		J5076.4307	4.3 mm		7 mm
		J5076.4309			9 mm
		J5076.4311			11 mm
		J5076.4313			13 mm
		J5076.4316	5.0 mm		16 mm
		J5076.5007			7 mm
		J5076.5009			9 mm
		J5076.5011			11 mm
		J5076.5013			13 mm
J5076.5016	16 mm				

PROGRESSIVE-LINE Guide System

Surgical instruments

	Article	Art. No.	Ø	L
	Guide System dense bone drill PROGRESSIVE-LINE resterilizable Material Stainless steel	J5078.3309	3.3 mm	9 mm
		J5078.3311		11 mm
		J5078.3313		13 mm
		J5078.3316		16 mm
		J5078.3807	3.8 mm	7 mm
		J5078.3809		9 mm
		J5078.3811		11 mm
		J5078.3813		13 mm
		J5078.3816	16 mm	
		J5078.4307	4.3 mm	7 mm
		J5078.4309		9 mm
		J5078.4311		11 mm
		J5078.4313		13 mm
		J5078.4316	16 mm	
		J5078.5007	5.0 mm	7 mm
		J5078.5009		9 mm
		J5078.5011		11 mm
		J5078.5013		13 mm
J5078.5016	16 mm			
	Guide System form drill for Ø 3.8 mm underpreparation PROGRESSIVE-LINE resterilizable Material Stainless steel	J5077.3309	3.3 mm	9 mm
		J5077.3311		11 mm
		J5077.3313		13 mm
		J5077.3316		16 mm
	Guide System guiding sleeve PROGRESSIVE-LINE (2 units) Material Titanium alloy	J3754.3301*	3.3 mm	-
		J3754.3801*	3.8 mm	
		J3754.4301*	4.3 mm	
		J3754.5001*	5.0 mm	


* The sleeves are not compatible with the SCREW-LINE Guide System.

PROGRESSIVE-LINE Flex



PROGRESSIVE-LINE Flex

Surgery Set CAMLOG®/CONELOG®

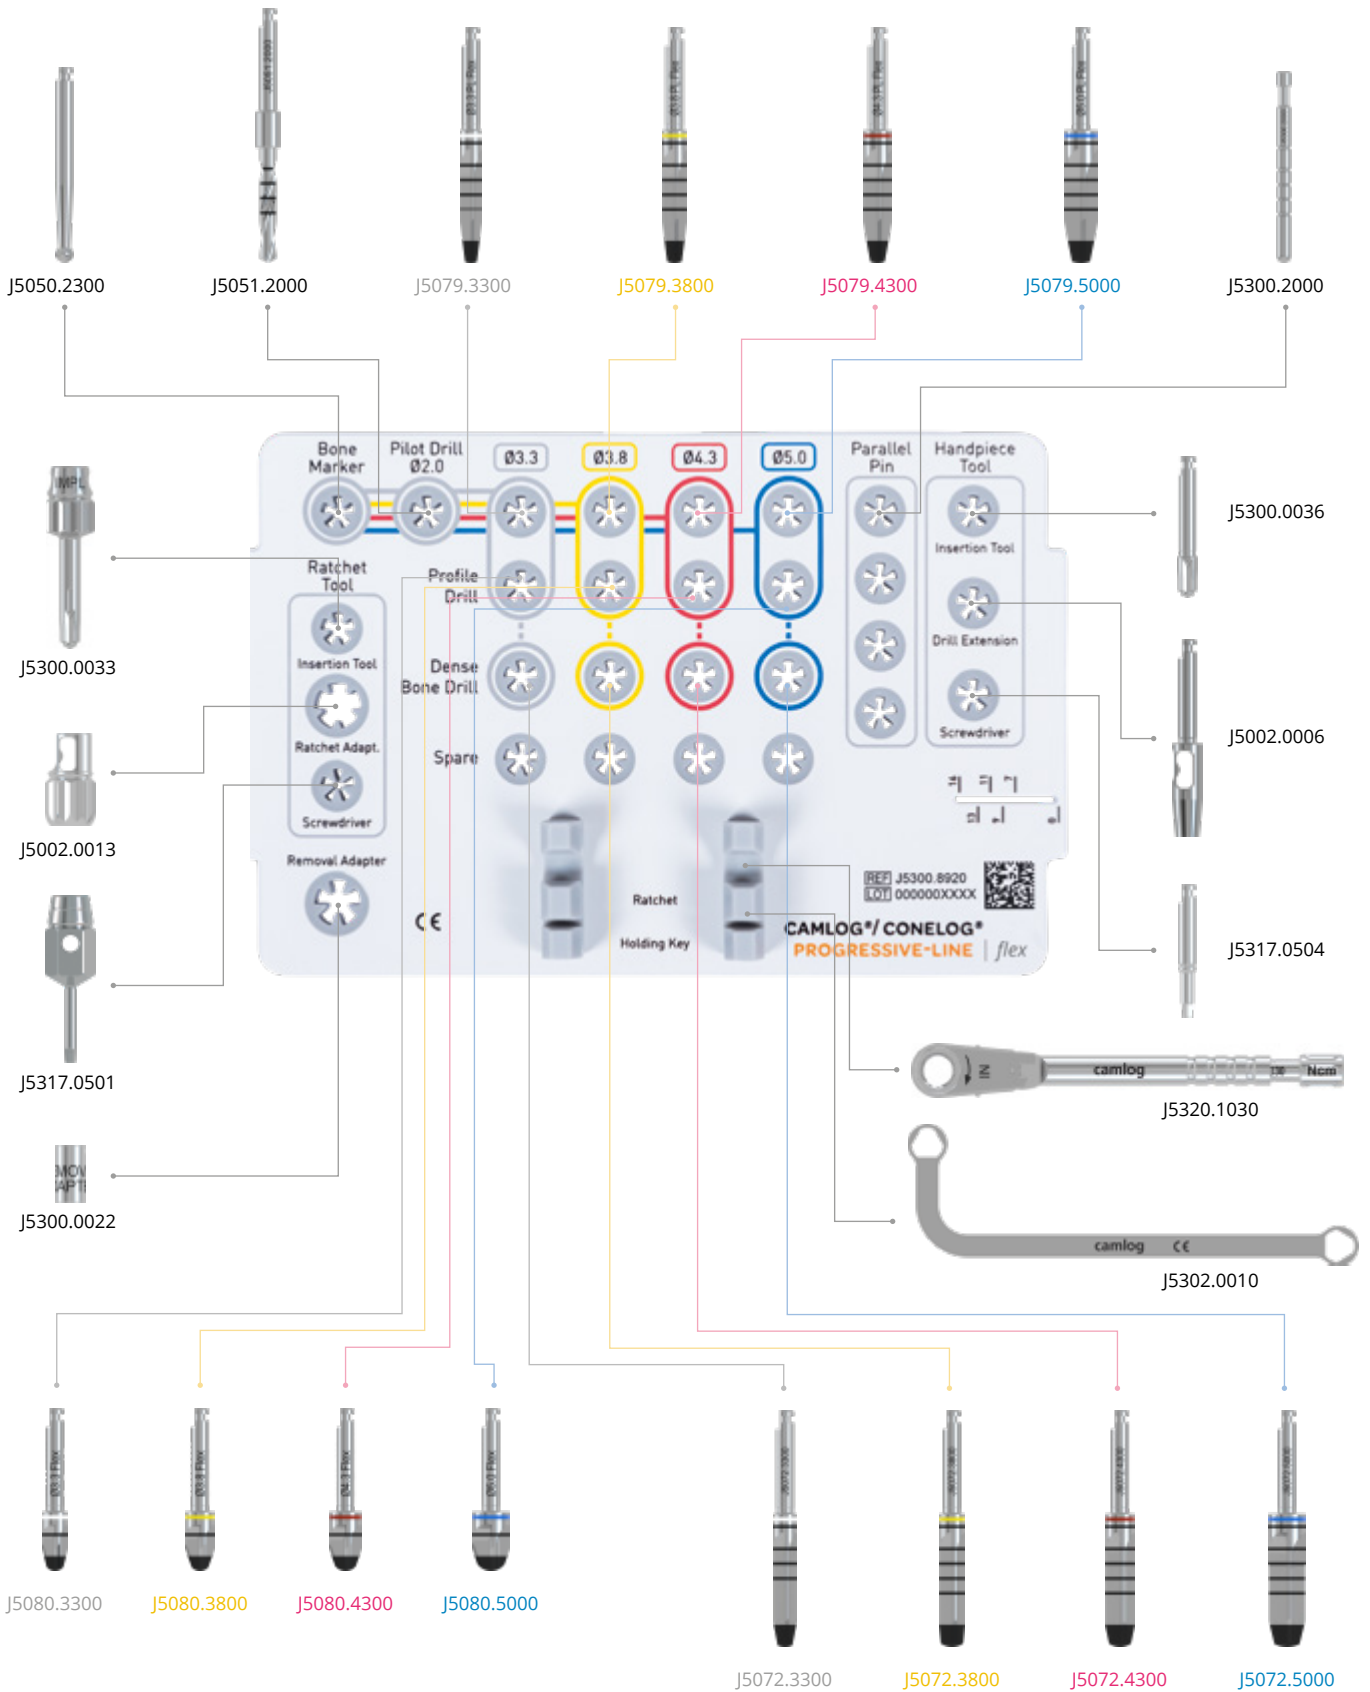

Note






- The drills are arranged and sorted in the set according to the treatment sequence.
- Colored lines indicate the exact drilling sequence.

Surgery Set



	Article	Art. No.
	<p>Surgery Set CAMLOG®/CONELOG® PROGRESSIVE-LINE Flex contains all necessary color-code ordered surgical instruments, incl. torque wrench and universal holding key</p>	<p>J5300.0071</p>

PROGRESSIVE-LINE Flex

Surgical instruments


	Article	Art. No.	Ø	L
	Drill PROGRESSIVE-LINE Flex resterilizable Material Stainless steel	J5079.3300	3.3 mm	-
		J5079.3800	3.8 mm	
		J5079.4300	4.3 mm	
		J5079.5000	5.0 mm	
	Profile drill PROGRESSIVE-LINE Flex resterilizable Material Stainless steel	J5080.3300	3.3 mm	-
		J5080.3800	3.8 mm	
		J5080.4300	4.3 mm	
		J5080.5000	5.0 mm	
	Dense bone drill PROGRESSIVE-LINE resterilizable Material Stainless steel	J5072.3300	3.3 mm	-
		J5072.3800	3.8 mm	
		J5072.4300	4.3 mm	
		J5072.5000	5.0 mm	
	Tap PROGRESSIVE-LINE resterilizable Material Stainless steel	J5071.3300	3.3 mm	-
		J5071.3800	3.8 mm	
		J5071.4300	4.3 mm	
		J5071.5000	5.0 mm	
	Wrench adapter Material Stainless steel	J5002.0013	-	11 mm

SCREW-LINE

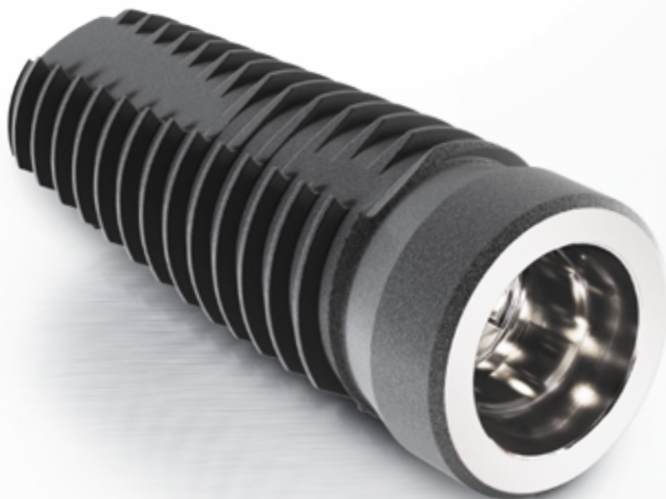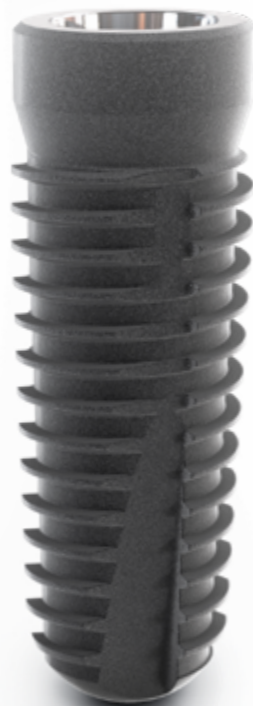

SCREW-LINE


Implants with snap-in insertion posts

	Article	Art. No.	Ø	L	A Ø
	CONELOG® SCREW-LINE Implant, Promote® plus incl. snap-in insertion post and cover screw, sterile Material Titanium Grade 4	C1066.3309	3.3 mm	9 mm	2.7 mm
		C1066.3311		11 mm	
		C1066.3313		13 mm	
		C1066.3316		16 mm	
		C1066.3807	3.8 mm	7 mm	3.5 mm
		C1066.3809		9 mm	
		C1066.3811		11 mm	
		C1066.3813		13 mm	
		C1066.3816	16 mm		
		C1066.4307	4.3 mm	7 mm	3.9 mm
		C1066.4309		9 mm	
		C1066.4311		11 mm	
		C1066.4313		13 mm	
		C1066.4316	16 mm		
		C1066.5007	5.0 mm	7 mm	4.6 mm
		C1066.5009		9 mm	
		C1066.5011		11 mm	
		C1066.5013		13 mm	
		C1066.5016		16 mm	

Note

CONELOG® SCREW-LINE implants, Promote® plus, with Art. No. C1066.xxxx and C1065-xxxx can be used exclusively with the insertion tools (Art. No. J5300.0031, J5300.0032, J5300.0033, J5300.0034 or J5300.0035, J5300.0036 and J5300.0037).

Implants with screw-mounted insertion posts

	Article	Art. No.	Ø	L	A Ø
	CONELOG® SCREW-LINE Implant, Promote® plus incl. screw-mounted insertion post and cover screw, sterile Material Titanium Grade 4	C1065.3309	3.3 mm	9 mm	2.7 mm
		C1065.3311		11 mm	
		C1065.3313		13 mm	
		C1065.3316		16 mm	
		C1065.3807	3.8 mm	7 mm	3.5 mm
		C1065.3809		9 mm	
		C1065.3811		11 mm	
		C1065.3813		13 mm	
		C1065.3816		16 mm	
		C1065.4307	4.3 mm	7 mm	3.9 mm
		C1065.4309		9 mm	
		C1065.4311		11 mm	
		C1065.4313		13 mm	
		C1065.4316	16 mm	5.0 mm	4.6 mm
		C1065.5007	7 mm		
		C1065.5009	9 mm		
		C1065.5011	11 mm		
		C1065.5013	13 mm		
		C1065.5016	16 mm		

Note


Implants with the screw-mounted insertion post (Art. No. C10655.xxxx) are to be used for template-guided implant insertion with the SCREW-LINE Guide System.

Note

CONELOG® SCREW-LINE implants, Promote® plus, with Art. No. C1066.xxxx and C1065-xxxx can be used exclusively with the insertion tools (Art. No. J5300.0031, J5300.0032, J5300.0033, J5300.0034 or J5300.0035, J5300.0036 and J5300.0037).

SCREW-LINE

Surgery Set CAMLOG®/CONELOG®

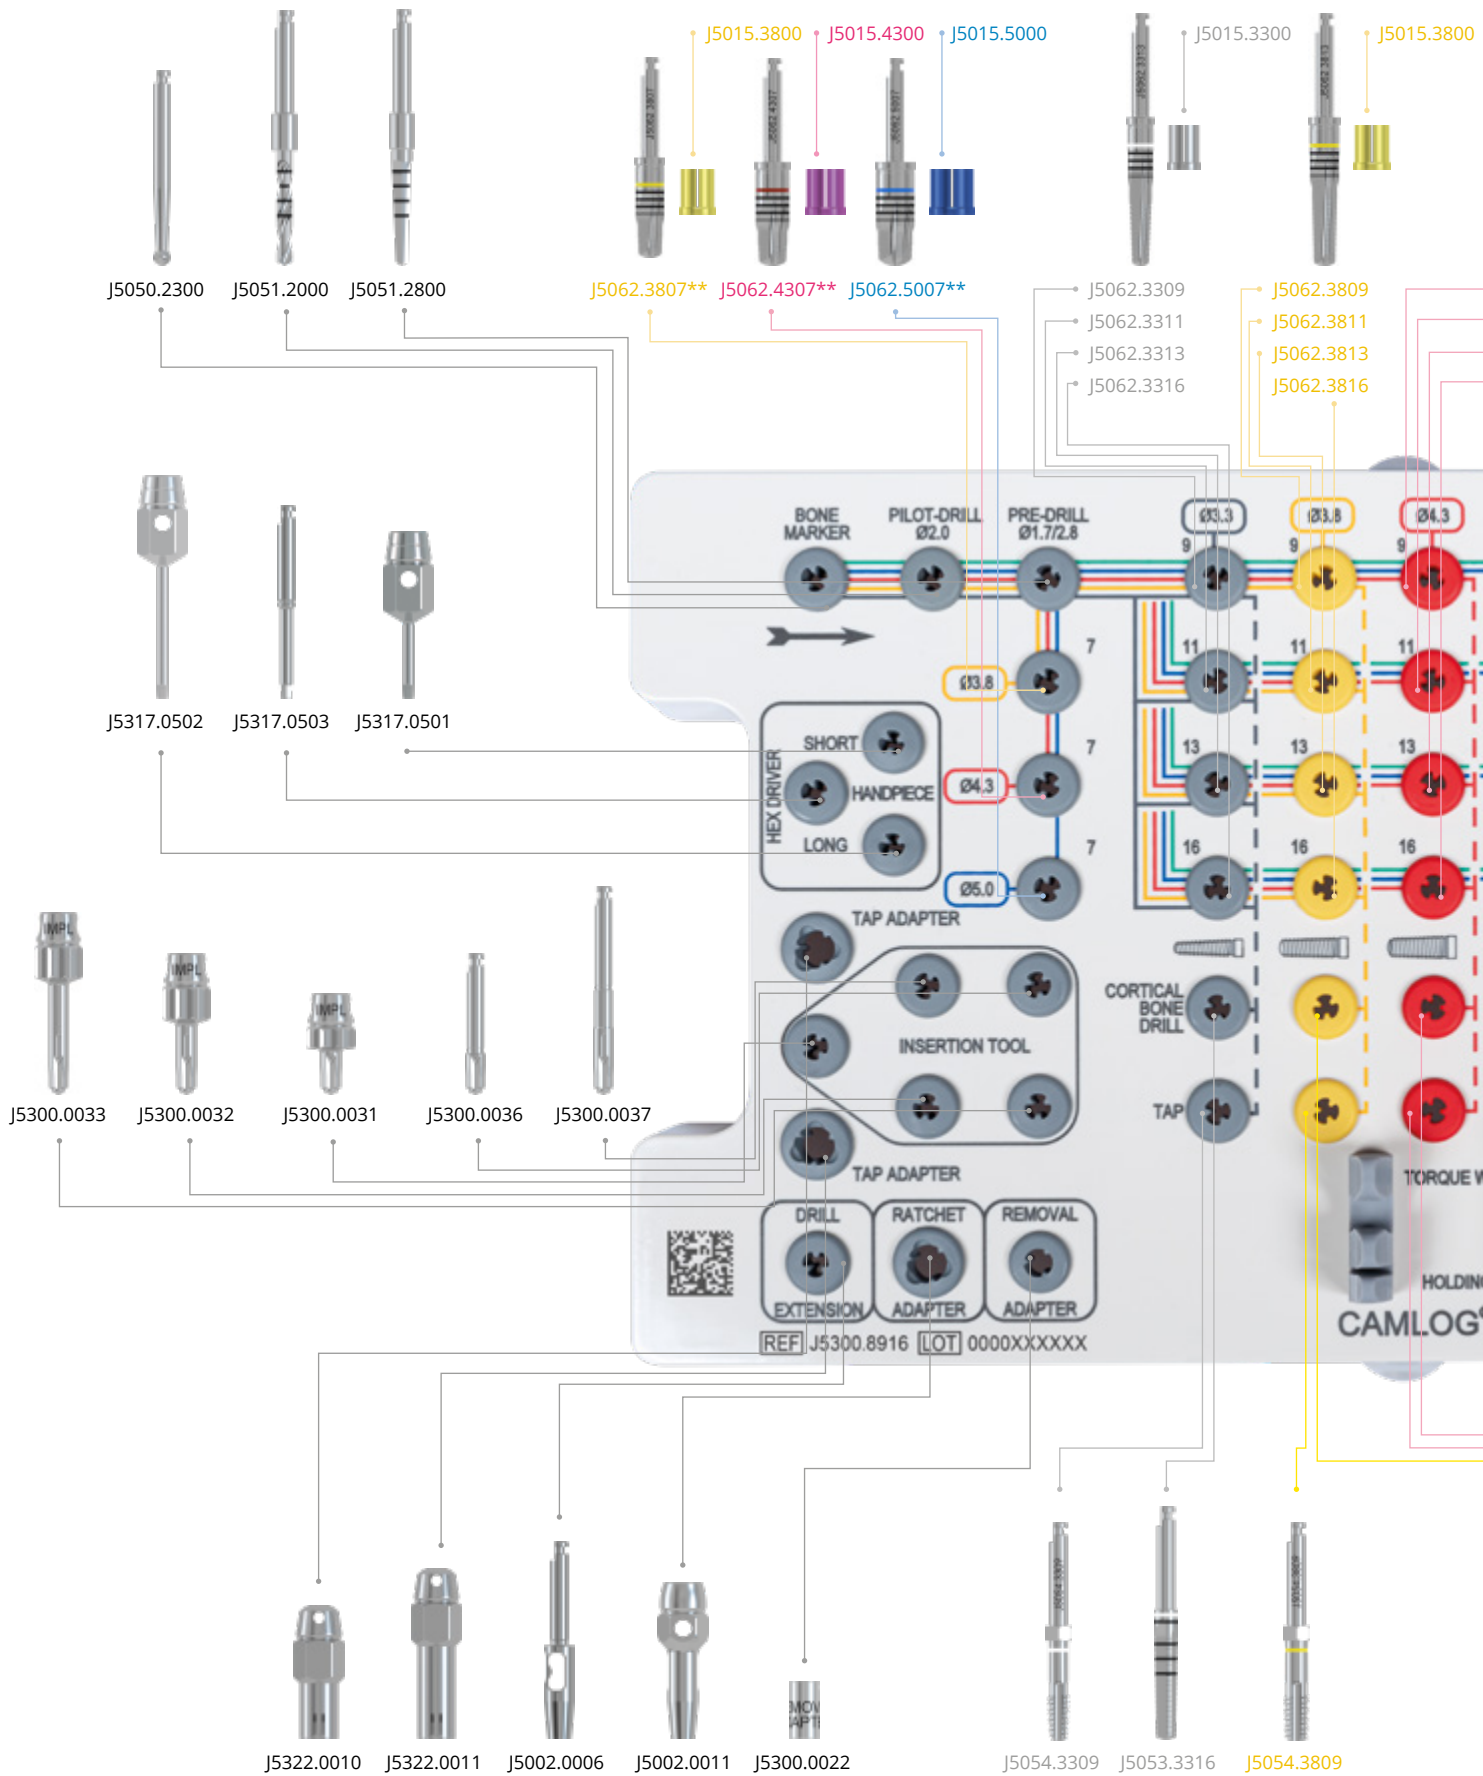

* This article is not included in the surgery set and must be ordered separately.

Note

- The drills are arranged and sorted in the set according to the treatment sequence.
- Colored lines indicate the exact drilling sequence.

J5015.4300 J5015.5000 J5015.6000*

J5062.4309 J5062.4311 J5062.4313 J5062.4316 J5062.5009 J5062.5011 J5062.5013 J5062.5016 J5062.6009* J5062.6011* J5062.6013* J5062.6016*

J5300.2028

J5015.0013 J5015.0011 J5015.0009 J5015.0007

J5320.1030

J5302.0010

J5053.3816 J5054.4309 J5053.4316 J5054.5009 J5053.5016 J5054.6009* J5053.6016*





SCREW-LINE

Surgery set and wash tray

	Article	Art. No.
 <p>A white plastic surgery set containing various color-coded surgical instruments, including a torque wrench and a universal holding key. The set is organized into compartments and labeled with 'CAMLOG®/CONELOG® SCREW-LINE'.</p>	<p>Surgery Set CAMLOG®/CONELOG® SCREW-LINE contains all necessary color-code ordered surgical instruments, incl. torque wrench and universal holding key (drills and taps for Ø 6.0 mm are not included)</p>	<p>J5300.0063</p>
 <p>A rectangular metal wash tray with a grid of circular holes for instruments. It features color-coded markings and labels for different instrument types. The tray is labeled 'CAMLOG®/CONELOG® SCREW-LINE'.</p>	<p>Surgery wash tray CAMLOG®/CONELOG® SCREW-LINE incl. pattern, without content</p>	<p>J5300.8968</p>
 <p>A stainless steel pattern for the surgery wash tray, showing the layout of circular holes and color-coded markings. It is labeled 'CAMLOG®/CONELOG® SCREW-LINE' and includes various tool labels like 'INSERTION TOOL', 'DRILL', 'RATCHET', 'TAP', 'PIB', 'PILOT', and 'ROUND'.</p>	<p>Pattern for surgery wash tray CAMLOG®/CONELOG® SCREW-LINE Material Stainless steel</p>	<p>J5300.1073</p>




Preparation of the implant bed for CAMLOG® SCREW-LINE Implants and for CONELOG® SCREW-LINE Implants is performed with identical instruments.

Surgical instruments

	Article	Art. No.	Ø	L
	Form drills SCREW-LINE resterilizable Material Stainless steel	J5062.3309	3.3 mm	9 mm
		J5062.3311		11 mm
		J5062.3313		13 mm
		J5062.3316		16 mm
		J5062.3807	3.8 mm	7 mm
		J5062.3809		9 mm
		J5062.3811		11 mm
		J5062.3813		13 mm
		J5062.3816		16 mm
		J5062.4307	4.3 mm	7 mm
		J5062.4309		9 mm
		J5062.4311		11 mm
		J5062.4313		13 mm
		J5062.4316	16 mm	
		J5062.5007	5.0 mm	7 mm
		J5062.5009		9 mm
		J5062.5011		11 mm
		J5062.5013		13 mm
J5062.5016	16 mm			
	Depth stop, for form drills PROGRESSIVE-LINE and SCREW-LINE resterilizable Material Titanium alloy	J5015.3300	3.3 mm	-
		J5015.3800	3.8 mm	
		J5015.4300	4.3 mm	
		J5015.5000	5.0 mm	
	Form drills SCREW-LINE cortical bone, resterilizable Material Stainless steel	J5053.3316	3.3 mm	-
		J5053.3816	3.8 mm	
		J5053.4316	4.3 mm	
		J5053.5016	5.0 mm	
	Tap SCREW-LINE with hexagon, resterilizable Material Stainless steel	J5054.3309	3.3 mm	-
		J5054.3809	3.8 mm	
		J5054.4309	4.3 mm	
		J5054.5009	5.0 mm	

SCREW-LINE

Surgical instruments

	Article	Art. No.	Ø	L
	EP pilot drill set sterile Content: EP round bur (Ø 3.0 mm) EP pilot drill (Ø 2.0 mm) Material Stainless steel / plastic	J5060.0001	-	-
	SCREW-LINE EP pre-drill sterile Material Stainless steel / plastic	J5060.2800	1.7– 2.8 mm	-
	SCREW-LINE EP form drill sterile Material Stainless steel / plastic	J5060.3309	3.3 mm	9 mm
		J5060.3311		11 mm
		J5060.3313		13 mm
		J5060.3807	3.8 mm	7 mm
		J5060.3809		9 mm
		J5060.3811		11 mm
		J5060.3813		13 mm
		J5060.4307	4.3 mm	7 mm
		J5060.4309		9 mm
		J5060.4311		11 mm
		J5060.4313		13 mm
		J5060.5007	5.0 mm	7 mm
		J5060.5009		9 mm
		J5060.5011		11 mm
J5060.5013	13 mm			

EP: Single-patient drill



The EP drills are for single use only and must not be resterilized.

SCREW-LINE Guide System



SCREW-LINE Guide System

Surgical instruments

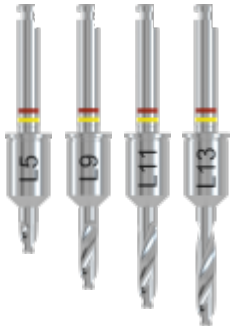	Article	Art. No.	Ø	L
	Guide System Pilot drill set internal irrigation, sterile (for pilot drilling Ø 2.0 mm) Material Stainless steel	J5063.3309	3.3 mm	9 mm (incl. 5 mm)**
		J5063.3311		11 mm (incl. 5 and 9 mm)**
		J5063.3313		13 mm (incl. 5, 9 and 11 mm)**
		J5064.3316*		16 mm
		J5063.4307	3.8 mm	7 mm (incl. 5 mm)**
			4.3 mm	
		J5063.4309	3.8 mm	9 mm (incl. 5 mm)**
			4.3 mm	
		J5063.4311	3.8 mm	11 mm (incl. 5 and 9 mm)**
			4.3 mm	
J5063.4313	3.8 mm	13 mm (incl. 5, 9 and 11 mm)**		
	4.3 mm			
J5064.4316*	3.8 mm	16 mm		
	4.3 mm			
	Guide System Surgery Set SCREW-LINE internal irrigation, sterile Material Stainless steel	J5065.3309	3.3 mm	9 mm (incl. 5 mm)****
		J5065.3311		11 mm (incl. 5 and 9 mm)****
		J5065.3313		13 mm (incl. 5, 9 and 11 mm)****
		J5066.3316****		16 mm
		J5065.3807	3.8 mm	7 mm (incl. 5 mm)****
		J5065.3809		9 mm (incl. 5 mm)****
		J5065.3811		11 mm (incl. 5 and 9 mm)****
		J5065.3813		13 mm (incl. 5, 9 and 11 mm)****
		J5066.3816****	16 mm	
		J5065.4307	4.3 mm	7 mm (incl. 5 mm)****
		J5065.4309		9 mm (incl. 5 mm)****
		J5065.4311		11 mm (incl. 5 and 9 mm)****
		J5065.4313		13 mm (incl. 5, 9 and 11 mm)****
		J5066.4316****		16 mm

* Necessary Guide System pilot drill for implant length 16 mm, following obligatory prior use of the pilot drill set length 13 mm.

** All Guide System pilot drill sets include a 5 mm long pilot drill, as well as all pilot drills necessary for the selected implant length.



*** Necessary Guide System form drill for implant length 16 mm, following obligatory prior use of the Guide System surgery set length 13 mm.

**** All Guide System surgery sets include a 5 mm long pre-drill, as well as all form drills necessary for the selected implant length.

All Guide System drills and gingiva punches for SCREW-LINE are intended for single use only.

Note

Implants with the screw-mounted insertion post (Art. No. C10655.xxxx) are to be used for template-guided implant insertion with the SCREW-LINE Guide System. The SCREW-LINE Guide System can only be used for implant diameters 3.3/3.8/4.3 mm.

	Article	Art. No.	Ø	L
	Guide System Form drill SCREW-LINE cortical bone internal irrigation, sterile Material Stainless steel	J5068.3309	3.3 mm	9 mm
		J5068.3311		11 mm
		J5068.3313		13 mm
		J5068.3316		16 mm
		J5068.3807	3.8 mm	7 mm
		J5068.3809		9 mm
		J5068.3811		11 mm
		J5068.3813		13 mm
		J5068.3816		16 mm
		J5068.4307		4.3 mm
		J5068.4309	9 mm	
		J5068.4311	11 mm	
		J5068.4313	13 mm	
		J5068.4316	16 mm	
	Guide System Gingiva punch sterile Material Stainless steel	J5041.3303	3.3 mm	-
		J5041.3803	3.8 mm	
		J5041.4303	4.3 mm	
	Guide System guiding sleeve Height 3.0 mm (2 units) Material Titanium alloy	J3734.3303*	3.3 mm	-
		J3734.3803*	3.8 mm	
		J3734.4303*	4.3 mm	
	Drill extension ISO shaft, for instruments with internal irrigation Material Stainless steel	J5002.0005	-	26.6 mm






* The sleeves are not compatible with the PROGRESSIVE-LINE Guide System.

All Guide System drills and gingiva punches for SCREW-LINE are intended for single use only.






General surgical instruments



General surgical instruments

	Article	Art. No.	Ø	L
	<p>Round bur resterilizable</p> <p>Material Stainless steel</p>	J5050.2300	2.3 mm	-
	<p>Point drill resterilizable</p> <p>Material Stainless steel</p>	J5051.1500	1.5 mm	-
	<p>Pilot drill without coil, resterilizable</p> <p>Material Stainless steel</p>	J5051.2003	2.0 mm	-
	<p>Pilot drill SCREW-LINE resterilizable</p> <p>Material Stainless steel</p>	J5051.2000	2.0 mm	-
	<p>Pre-drill SCREW-LINE resterilizable</p> <p>Material Stainless steel</p>	J5051.2800	1.7–2.8 mm	-

General surgical instruments

	Article		Art. No.	Ø	L
	Depth stop SCREW-LINE for pilot drill (J5051.2000) and pre-drill (J5051.2800), resterilizable Material Stainless steel		J5015.0009	-	9 mm
			J5015.0011		11 mm
			J5015.0013		13 mm
	Bone profiler Material Stainless steel	Ø 5.0 mm	J5003.3350*	3.3 mm	-
		Ø 6.0 mm	J5003.4360*	3.8 mm	
				4.3 mm	
		Ø 7.0 mm	J5003.5070*	5.0 mm	
	CONELOG® Guiding pin for bone profiler Material Titanium alloy		C5002.3300	3.3 mm	-
			C5002.3800	3.8 mm	
			C5002.4300	4.3 mm	
			C5002.5000	5.0 mm	
	Countersink Material Stainless steel	Ø 4.6 mm	J5006.3346	3.3 mm	-
		Ø 5.2 mm	J5006.3852	3.8 mm	
		Ø 5.6 mm	J5006.4356	4.3 mm	
		Ø 6.3 mm	J5006.5063	5.0 mm	
	Baring drill for cover screw Material Stainless steel		J5004.3300	3.3 mm	-
			J5004.3800	3.8 mm	
			J5004.4300	4.3 mm	
			J5004.5000	5.0 mm	

* Always to be used in conjunction with the matching guiding pin!

	Article	Art. No.	∅	Dimension
	Paralleling pin SCREW-LINE with depth marks Material Titanium alloy	J5300.2028	-	∅ 1.7-2.8 mm/ 2.0 mm
	Drill extension ISO shaft (not for drills with internal irrigation) Material Stainless steel	J5002.0006	-	26.5 mm
	Tap adapter, short for tap SCREW-LINE Material Stainless steel	J5322.0010	-	18.0 mm
	Tap adapter, long for tap SCREW-LINE Material Stainless steel	J5322.0011	-	23.0 mm
	Removal adapter for CAMLOG® and CONELOG® suitable for all implant diameters Material Stainless steel	J5300.0022*	3.3 mm 3.8 mm 4.3 mm 5.0 mm	6.2 mm

* only for use with CONELOG® PROGRESSIVE-LINE Implants with Art. No. C1086.xxxx as well as CONELOG® SCREW-LINE Implants with Art. No. C1066.xxxx








General surgical instruments






	Article	Art. No.	Dimension
	Insertion tool, extra short for screw implants, manual/wrench Material Stainless steel	J5300.0031*	13.7 mm
	Insertion tool, short for screw implants, manual/wrench Material Stainless steel	J5300.0032*	19.2 mm
	Insertion tool, long for screw implants, manual/wrench Material Stainless steel	J5300.0033*	24.8 mm
	Insertion tool, short for screw implants, with ISO-shaft for angled hand piece (without hexagon at the shaft) Material Stainless steel	J5300.0036*	19.1 mm
	Insertion tool, long for screw implants, with ISO-shaft for angled hand piece (without hexagon at the shaft) Material Stainless steel	J5300.0037*	28.2 mm
	Insertion tool, short for screw implants, with ISO-shaft for angled hand piece, for hex clamping system Material Stainless steel	J5300.0034*	19.1 mm
	Insertion tool, long for screw implants, with ISO-shaft for angled hand piece, for hex clamping system Material Stainless steel	J5300.0035*	28.2 mm

* only for use with CONELOG® PROGRESSIVE-LINE Implants with Art. No. C1085.xxxx and C1086.xxxx as well as CONELOG® SCREW-LINE Implants with Art. No. C1065.xxxx and C1066.xxxx

	Article	Art. No.	Dimension
	<p>Torque wrench with continuous torque adjustment until maximal 30 Ncm</p> <p>Material Stainless steel</p>	J5320.1030	-
	<p>PickUp instrument holder for carrying implants</p> <p>Material Stainless steel</p>	J5300.0030	-
	<p>Adapter ISO shaft for angled hand piece/wrench</p> <p>Material Stainless steel</p>	J5002.0011	21.0 mm

General surgical instruments

	Article	Art. No.	Ø	Dimension
	Universal holding key Material Stainless steel	J5302.0010	-	-
	CONELOG® Insertion aid, short for CONELOG® Implants Material Stainless steel	C5302.3311	3.3 mm	28.1 mm
		C5302.4311	3.8 mm	
		C5302.5011	4.3 mm	
	CONELOG® Insertion aid, long for CONELOG® Implants Material Stainless steel	C5302.3310	3.3 mm	33.1 mm
		C5302.4310	3.8 mm	
		C5302.5010	4.3 mm	
	Sleeve for inserting the insertion aid into the implant color-coded Material Titanium alloy	J5302.3300	3.3 mm	-
		J5302.3800	3.8 mm	
		J5302.4300	4.3 mm	
		J5302.5000	5.0 mm	
	Screwdriver hex, extra short, manual/wrench Material Stainless steel	J5317.0510	-	14.5 mm
	Screwdriver hex, short, manual/wrench Material Stainless steel	J5317.0501	-	22.5 mm
	Screwdriver hex, long, manual/wrench Material Stainless steel	J5317.0502	-	30.3 mm


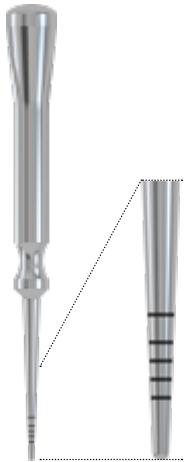
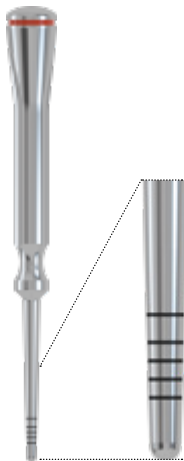
	Article	Art. No.	Dimension
	Screwdriver hex, short, ISO shaft Material Stainless steel	J5317.0504	18.0 mm
	Screwdriver hex, long, ISO shaft Material Stainless steel	J5317.0503	26.0 mm
	Manual screwdriver, hex without wrench head connection Material Stainless steel	J5317.0511	23.0 mm
	Cleaning needle for instruments with internal irrigation Material Stainless steel	J5002.0012	-
	Cleaning cannula for instruments with internal irrigation Material Stainless steel	J5002.0020	-

SCREW-LINE Osteotomy Set



SCREW-LINE Osteotomy Set

straight convex


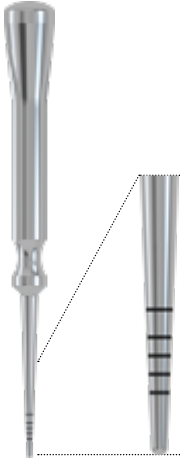
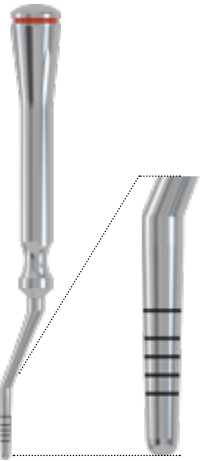
	Article	Art. No.	Ø
	<p>Osteotomy Set CAMLOG®/CONELOG® SCREW-LINE straight convex</p> <p>Material Stainless steel</p>	<p>J5418.0020</p>	<p>-</p>
	<p>Pre-Osteotome SCREW-LINE straight convex</p> <p>Material Stainless steel</p>	<p>J5417.2800*</p>	<p>1.7– 2.8 mm</p>
	<p>Osteotome SCREW-LINE straight convex</p> <p>Material Stainless steel</p>	<p>J5418.3300*</p> <p>J5418.3800*</p> <p>J5418.4300*</p> <p>J5418.5000*</p>	<p>3.3 mm</p> <p>3.8 mm</p> <p>4.3 mm</p> <p>5.0 mm</p>

* These products are included in the CAMLOG®/CONELOG® SCREW-LINE straight-convex osteotomy set.

Surgery




SCREW-LINE Osteotomy Set

angled convex

	Article	Art. No.	Ø
	<p>Osteotomy Set CAMLOG®/CONOLOG® SCREW-LINE angled convex</p> <p>Material Stainless steel</p>	<p>J5418.0030</p>	<p>-</p>
	<p>Pre-Osteotome SCREW-LINE straight convex</p> <p>Material Stainless steel</p>	<p>J5417.2800*</p>	<p>1.7– 2.8 mm</p>
	<p>Osteotome SCREW-LINE angled convex</p> <p>Material Stainless steel</p>	<p>J5418.3310*</p> <p>J5418.3810*</p> <p>J5418.4310*</p> <p>J5418.5010*</p>	<p>3.3 mm</p> <p>3.8 mm</p> <p>4.3 mm</p> <p>5.0 mm</p>

* These products are included in the CAMLOG®/CONOLOG® SCREW-LINE angled-convex osteotomy set.




straight concave

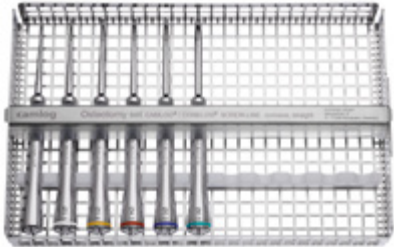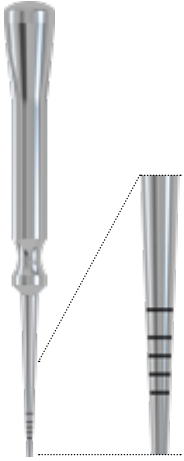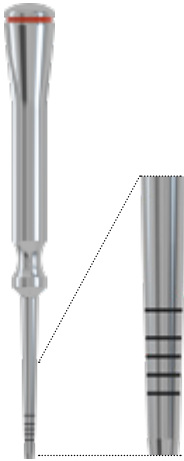	Article	Art. No.	∅
	Osteotomy Set CAMLOG®/CONELOG® SCREW-LINE straight concave Material Stainless steel	J5420.0020	-
	Pre-Osteotome SCREW-LINE straight concave Material Stainless steel	J5419.2800*	1.7– 2.8 mm
	Osteotome SCREW-LINE straight concave Material Stainless steel	J5420.3300*	3.3 mm
		J5420.3800*	3.8 mm
		J5420.4300*	4.3 mm
		J5420.5000*	5.0 mm

* These products are included in the CAMLOG®/CONELOG® SCREW-LINE straight-concave osteotomy set.

SCREW-LINE Osteotomy Set

angled concave

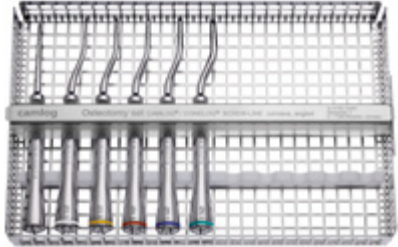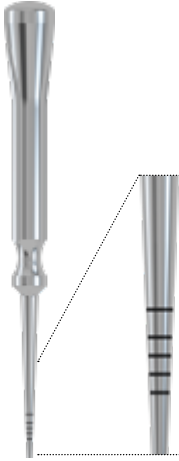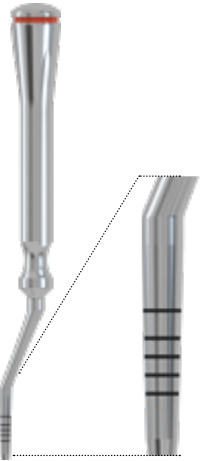
	Article	Art. No.	Ø
	Osteotomy Set CAMLOG®/CONELOG® SCREW-LINE angled concave Material Stainless steel	J5420.0030	-
	Pre-Osteotome SCREW-LINE straight concave Material Stainless steel	J5419.2800*	1.7– 2.8 mm
	Osteotome SCREW-LINE angled concave Material Stainless steel	J5420.3310*	3.3 mm
		J5420.3810*	3.8 mm
		J5420.4310*	4.3 mm
		J5420.5010*	5.0 mm

* These products are included in the CAMLOG®/CONELOG® SCREW-LINE angled-concave osteotomy set.

Cover screws and healing caps






Cover screws

	Article	Art. No.	Ø
	CONELOG® Implant cover screw Material Titanium alloy	C2019.3300	3.3 mm
		C2019.3800	3.8 mm
		C2019.4300	4.3 mm
		C2019.5000	5.0 mm

The implant cover screws are for single use only and must not be resterilized.

Healing caps

	Article	Art. No.	Ø	GH	G Ø
	CONELOG® Healing cap, cylindrical sterile Material Titanium alloy	C2015.3320	3.3 mm	2.0 mm	3.0 mm
		C2015.3340		4.0 mm	3.0 mm
		C2015.3820	3.8 mm	2.0 mm	3.5 mm
		C2015.3840		4.0 mm	3.5 mm
		C2015.3860*	6.0 mm	3.5 mm	
		C2015.4320	4.3 mm	2.0 mm	3.8 mm
		C2015.4340		4.0 mm	3.8 mm
		C2015.4360*	6.0 mm	3.8 mm	
		C2015.5020	5.0 mm	2.0 mm	4.5 mm
		C2015.5040		4.0 mm	4.5 mm
C2015.5060*	6.0 mm	4.5 mm			
	CONELOG® Healing cap, wide body sterile Material Titanium alloy	C2014.3340	3.3 mm	4.0 mm	4.8 mm
		C2014.3840	3.8 mm	4.0 mm	5.3 mm
		C2014.3860		6.0 mm	5.3 mm
		C2014.4340	4.3 mm	4.0 mm	5.8 mm
		C2014.4360		6.0 mm	5.8 mm
		C2014.5040	5.0 mm	4.0 mm	6.5 mm
C2014.5060	6.0 mm	6.5 mm			
	CONELOG® Healing cap, bottleneck sterile Material Titanium alloy	C2011.3340	3.3 mm	4.0 mm	3.3 mm
		C2011.3840	3.8 mm	4.0 mm	3.8 mm
		C2011.3860		6.0 mm	3.8 mm
		C2011.4340	4.3 mm	4.0 mm	4.0 mm
		C2011.4360		6.0 mm	4.0 mm
		C2011.5040	5.0 mm	4.0 mm	4.7 mm
C2011.5060	6.0 mm	4.7 mm			



* suitable for bite registration

Healing caps are for single use only and must not be resterilized.

Prosthetics



Scanbodies

	Article	Art. No.	Ø
	<p>CONELOG® Scanbody* for optical, 3-dimensional localization of CONELOG® Implants in the mouth or CONELOG® Lab analogs in the working model, incl. abutment screw, sterile</p> <p>Not compatible with the CEREC and inLab systems from Dentsply Sirona</p> <p>Material PEEK</p>	C2600.3310	3.3 mm
		C2600.4310	3.8 mm
			4.3 mm
		C2600.5010	5.0 mm
	<p>CONELOG® ScanPost for Sirona® Scanbody for digital recording of the CONELOG® Implant or lab analog position and for further processing in the CEREC and inLab systems from Dentsply Sirona, incl. abutment screw</p> <p>Material Titanium alloy</p>	C2620.3306	3.3 mm
		C2620.3806	3.8 mm
		C2620.4306	4.3 mm
		C2620.5006	5.0 mm

* Please check whether the CONELOG® Scanbody is available in the CAD software used.
CAD libraries for selected CONELOG® Prosthetic components are available for free download here:
www.camlog.com/en/media-center/cad-libraries

Matching Sirona® Scanbodies size S for CONELOG® ScanPost and CONELOG® Titanium base CAD/CAM, crown, with Ø 3.3/3.8/4.3 mm:




For Omnicam®: Article number 6431311
For Bluecam®: Article number 6431295

Matching Sirona® Scanbodies size L for CONELOG® ScanPost and CONELOG® Titanium base CAD/CAM, crown, with Ø 5.0 mm:



For Omnicam®: Article number 6431329
For Bluecam®: Article number 6431303

Sirona® Scanbodies are available from Dentsply Sirona.






Impression taking

	Article	Art. No.	Ø
 <p>3 mm 10 mm</p>	CONELOG® Impression post, open tray incl. fixing screw (the fixing screw can be shortened extra-oral by 3 mm with a screwdriver, hex) Material Titanium alloy	C2121.3300	3.3 mm
		C2121.3800	3.8 mm
		C2121.4300	4.3 mm
		C2121.5000	5.0 mm
 <p>10.7 mm</p>	CONELOG® Impression post, closed tray incl. impression cap, bite registration cap and fixing screw Material Titanium alloy / POM	C2110.3300	3.3 mm
		C2110.3800	3.8 mm
		C2110.4300	4.3 mm
		C2110.5000	5.0 mm
	Impression cap for impression post, closed tray (5 units) Material POM	J2111.3300	3.3 mm
		J2111.3800	3.8 mm
		J2111.4300	4.3 mm
		J2111.5000	5.0 mm

Bite registration



	Article	Art. No.	Ø
	CONELOG® Bite registration post incl. fixing screw and bite registration cap Material Titanium alloy / POM	C2140.3300	3.3 mm
		C2140.3800	3.8 mm
		C2140.4300	4.3 mm
		C2140.5000	5.0 mm
	Bite registration cap (5 units) Material POM	J2112.3300	3.3 mm
		J2112.3800	3.8 mm
		J2112.4300	4.3 mm
		J2112.5000	5.0 mm

Cast fabrication

	Article	Art. No.	Ø
	CONELOG® Lab analog for cast models Material Titanium alloy	C3010.3300	3.3 mm
		C2211.3300	3.8 mm
		C3010.4300	4.3 mm
		C3010.5000	5.0 mm
	CONELOG® Lab analog (3 units) for cast models Material Titanium alloy	C3010.3303	3.3 mm
		C3010.3803	3.8 mm
		C3010.4303	4.3 mm
		C3010.5003	5.0 mm
	CONELOG® Implant analog for printed and cast models Material Titanium alloy	C3025.3300	3.3 mm
		C3025.3800	3.8 mm
		C3025.4300	4.3 mm
		C3025.5000	5.0 mm
	CONELOG® Implant analog (3 units) for printed and cast models Material Titanium alloy	C3025.3303	3.3 mm
		C3025.3803	3.8 mm
		C3025.4303	4.3 mm
		C3025.5003	5.0 mm
	DIM Analog® for the CONELOG® Implant System for printed models, incl. knurled nut Material Titanium alloy / stainless steel	C3012.3300	3.3 mm
		C3012.4300	3.8 mm
			4.3 mm
C3012.5000	5.0 mm		

Manufacturer DIM Analog®: NT-Trading GmbH & Co. KG | G.-Braun-Straße 18 | 76187 Karlsruhe | Germany
 DIM Analog® is a registered trademark of the NT-Trading GmbH & Co. KG company.





Temporary abutments

	Article	Art. No.	Ø	GH
 <p>11 mm</p>	CONELOG® Temporary abutment, crown, titanium alloy preparable, incl. abutment screw Material Titanium alloy	C2239.3300*	3.3 mm	-
		C2239.3800	3.8 mm	
		C2239.4300	4.3 mm	
		C2239.5000	5.0 mm	
 <p>11.2 mm</p>	CONELOG® Temporary abutment, bridge, titanium alloy preparable, incl. abutment screw Material Titanium alloy	C2339.3300	3.3 mm	-
		C2339.3800	3.8 mm	
		C2339.4300	4.3 mm	
		C2339.5000	5.0 mm	

* only for crown restorations in the region of the upper lateral and lower lateral and central incisors

CAD/CAM prosthetics

Crown, bridge and hybrid restoration

	Article	Art. No.	Ø	GH
	CONELOG® Titanium base CAD/CAM, crown Bonding base for individual CAD/CAM fabricated dental prostheses, incl. dark purple anodized abutment screw and bonding aid (POM) Material Titanium alloy / POM	C2242.3308*	3.3 mm	0.8 mm
		C2242.3808	3.8 mm	
		C2242.4308	4.3 mm	
		C2242.5008	5.0 mm	
	CONELOG® Titanium base CAD/CAM, crown Bonding base for individual CAD/CAM fabricated dental prostheses, incl. dark purple anodized abutment screw and bonding aid (POM) Material Titanium alloy / POM	C2242.3320*	3.3 mm	2.0 mm
		C2242.3820	3.8 mm	
		C2242.4320	4.3 mm	
		C2242.5020	5.0 mm	
	CONELOG® Titanium base CAD/CAM, bridge Bonding base for individual CAD/CAM fabricated dental prostheses, incl. dark purple anodized abutment screw and bonding aid (POM) Material Titanium alloy / POM	C2342.3308	3.3 mm	0.8 mm
		C2342.3808	3.8 mm	
		C2342.4308	4.3 mm	
		C2342.5008	5.0 mm	
	CONELOG® Titanium base CAD/CAM, bridge Bonding base for individual CAD/CAM fabricated dental prostheses, incl. dark purple anodized abutment screw and bonding aid (POM) Material Titanium alloy / POM	C2342.3320	3.3 mm	2.0 mm
		C2342.3820	3.8 mm	
		C2342.4320	4.3 mm	
		C2342.5020	5.0 mm	




* only for crown restorations in the region of the upper lateral and lower lateral and central incisors

The geometries of the CONELOG® Titanium bases CAD/CAM are available as a CAD library for leading dental CAD systems.

The libraries are available for free download at:
www.camlog.com/en/media-center/cad-libraries




DEDICAM® CAD/CAM prosthetics from Camlog

Find out more about DEDICAM® Products at your appropriate Camlog country representative.

	Article	Art. No.	Ø	Thread
	CONELOG® Modeling aid for CONELOG® Titanium base CAD/CAM, crown burn-out, for fabricating mesostructures and crowns Material POM	C2242.3302	3.3 mm	-
		C2242.3802	3.8 mm	
		C2242.4302	4.3 mm	
		C2242.5002	5.0 mm	
	CONELOG® Abutment screw for CONELOG® Titanium base CAD/CAM dark purple anodized Material Titanium alloy	C4015.1601	3.3 mm	M1.6
			3.8 mm	
			4.3 mm	
		C4015.2001	5.0 mm	M2.0
	CONELOG® Lab screw for CONELOG® Titanium base CAD/CAM partially brown anodized Material Titanium alloy	C4016.1601	3.3 mm	M1.6
			3.8 mm	
			4.3 mm	
		C4016.2001	5.0 mm	M2.0

CAM blanks

Milling of customized, one-piece abutments and healing caps using CAD/CAM technology

	Article	Art. No.	Ø
	CONELOG® CAM titanium blank, type IAC** Ø 12 mm, length 12.5 mm (2 units), Shipping incl. 2 separately packed abutment screws Material Titanium alloy	C2431.3313*	3.3 mm
		C2431.3813	3.8 mm
		C2431.4313	4.3 mm
		C2431.5013	5.0 mm
	CONELOG® CAM titanium blank, type ME*** Ø 12 mm, length 20 mm (2 units), Shipping incl. 2 separately packed abutment screws Material Titanium alloy	C2441.3320*	3.3 mm
		C2441.3820	3.8 mm
		C2441.4320	4.3 mm
		C2441.5020	5.0 mm
	CONELOG® CAM CoCr blank, type ME*** Ø 12 mm, length 20 mm (2 units), Shipping incl. 2 separately packed abutment screws Material Cobalt chrome alloy	C2461.3320*	3.3 mm
		C2461.4320	3.8 mm
			4.3 mm
		C2461.5020	5.0 mm

* only for crown restorations in the region of the upper lateral and lower lateral and central incisors (Ø 3.3 mm not for double crown restorations)

** Type IAC

For the milling process, the CAM titanium blank, type IAC is fixated to the implant-abutment connection via the CONELOG® Collet for CAM blanks. The machine-specific holders and adapters for the collet as well as the milling strategies are to be provided by the user.

*** Type ME


For the milling process, the CAM blank, type ME is fixed to a cylindrical section opposite the implant-abutment connection. Medentika® Preface® Abutment holders can be used as machine-specific clamping devices. These collets are available for selected machines from the respective machine manufacturers. The milling strategies are to be provided by the user.

The geometries of the CONELOG® CAM blanks are available as a CAD library for leading dental CAD systems.

The libraries are available for free download at:
www.camlog.com/en/media-center/cad-libraries

Medentika® and Preface® are registered trademarks of Medentika GmbH, D-Hügelshheim.

Accessories for CAM titanium blanks, type IAC

	Article	Art. No.	Ø
	CONELOG® Collet for CAM blank, type IAC* Ø 6 mm, length 17 mm, incl. 2 fixing screws for CAM blank, type IAC Material Stainless steel	C3720.3300	3.3 mm
		C3720.4300	3.8 mm
			4.3 mm
		C3720.5000	5.0 mm



* Type IAC

For the milling process, the CAM titanium blank, type IAC is fixated to the implant-abutment connection via the CONELOG® Collet for CAM blanks. The machine-specific holders and adapters for the collet as well as the milling strategies are to be provided by the user.



Esthomic® Abutments

Cemented crown and bridge restorations


	Article	Art. No.	Ø	GH
	CONOLOG® Esthomic® Abutments, straight preparable, incl. abutment screw Material Titanium alloy	C2226.3815	3.8 mm	1.5–2.5 mm
		C2226.3830		3.0–4.5 mm
		C2226.4315	4.3 mm	1.5–2.5 mm
		C2226.4330		3.0–4.5 mm
		C2226.5015	5.0 mm	1.5–2.5 mm
		C2226.5030		3.0–4.5 mm
	CONOLOG® Esthomic® Abutments, Inset preparable, incl. abutment screw Material Titanium alloy	C2235.3320*	3.3 mm	2.0–3.3 mm
		C2235.3820	3.8 mm	
		C2235.4320	4.3 mm	
		C2235.5020	5.0 mm	

* only for crown restorations in the region of the upper lateral and lower lateral and central incisors

	Article	Art. No.	Ø	GH
	CONELOG® Esthomic® Abutments 15° angled, type A preparable, incl. abutment screw Material Titanium alloy	C2227.3815	3.8 mm	1.5–2.5 mm
		C2227.3830		3.0–4.5 mm
		C2227.4315	4.3 mm	1.5–2.5 mm
		C2227.4330		3.0–4.5 mm
		C2227.5015	5.0 mm	1.5–2.5 mm
		C2227.5030		3.0–4.5 mm
	CONELOG® Esthomic® Abutments 15° angled, type B preparable, incl. abutment screw Material Titanium alloy	C2228.3815	3.8 mm	1.5–2.5 mm
		C2228.3830		3.0–4.5 mm
		C2228.4315	4.3 mm	1.5–2.5 mm
		C2228.4330		3.0–4.5 mm
		C2228.5015	5.0 mm	1.5–2.5 mm
		C2228.5030		3.0–4.5 mm
	CONELOG® Esthomic® Abutments 20° angled, type A preparable, incl. abutment screw Material Titanium alloy	C2231.3815	3.8 mm	1.5–2.5 mm
		C2231.3830		3.0–4.5 mm
		C2231.4315	4.3 mm	1.5–2.5 mm
		C2231.4330		3.0–4.5 mm
		C2231.5015	5.0 mm	1.5–2.5 mm
		C2231.5030		3.0–4.5 mm
	CONELOG® Esthomic® Abutments 20° angled, type B preparable, incl. abutment screw Material Titanium alloy	C2232.3815	3.8 mm	1.5–2.5 mm
		C2232.3830		3.0–4.5 mm
		C2232.4315	4.3 mm	1.5–2.5 mm
		C2232.4330		3.0–4.5 mm
		C2232.5015	5.0 mm	1.5–2.5 mm
		C2232.5030		3.0–4.5 mm


Universal abutments

Cemented crown and bridge restoration

	Article	Art. No.	Ø	Dimension
 <p>11 mm</p>	CONELOG® Universal abutment preparable, incl. abutment screw Material Titanium alloy	C2211.3300*	3.3 mm	
		C2211.3800	3.8 mm	
		C2211.4300	4.3 mm	
		C2211.5000	5.0 mm	




Gold-plastic abutment

Cemented crown and bridge restoration

	Article	Art. No.	Ø	Noble metal weight
 <p>11.7 mm</p>	CONELOG® Gold-plastic abutment cast-on, incl. abutment screw Material Cast-on gold alloy / POM	C2246.3300*	3.3 mm	approx. 0.31 g
		C2246.3800	3.8 mm	approx. 0.36 g
		C2246.4300	4.3 mm	approx. 0.36 g
		C2246.5000	5.0 mm	approx. 0.55 g











* only for crown restorations in the region of the upper lateral and lower lateral and central incisors
 (Ø 3.3 mm not for double crown restorations)











Occlusally screw-mounted prosthetics

	Article	Art. No.	Type	Ø	GH	PP Ø			
	CONELOG® Bar abutments, straight sterile Material Titanium alloy	C2254.3310	-	3.3 mm	1.0 mm	4.3 mm			
		C2254.3325			2.5 mm				
		C2254.3810		3.8 mm	1.0 mm		4.3 mm		
		C2254.3825			2.5 mm				
		C2254.3840		4.0 mm	4.3 mm				
		C2254.4310		4.3 mm				1.0 mm	
		C2254.4325				2.5 mm			
		C2254.4340		4.0 mm		4.3 mm			
		C2254.5010		5.0 mm			1.0 mm	6.0 mm	
		C2254.5025					2.5 mm		
C2254.5040	4.0 mm								
	CONELOG® Bar abutments, 17° angled incl. light blue anodized abutment screw with reduced head, sterile Material Titanium alloy	C2256.3325	A	3.3 mm	2.5 mm		4.3 mm		
		C2256.3340			4.0 mm				
		C2257.3325	B		2.5 mm	4.3 mm			
		C2257.3340			4.0 mm				
		C2256.3825	A		3.8 mm			2.5 mm	4.3 mm
		C2256.3840						4.0 mm	
		C2257.3825	B	2.5 mm	4.3 mm				
		C2257.3840		4.0 mm					
		C2256.4325	A	4.3 mm		2.5 mm	4.3 mm		
		C2256.4340				4.0 mm			
		C2257.4325	B			2.5 mm		4.3 mm	
		C2257.4340				4.0 mm			
		C2256.5025	A		5.0 mm	2.5 mm			6.0 mm
		C2256.5040				4.0 mm			
C2257.5025	B	2.5 mm	6.0 mm						
C2257.5040		4.0 mm							
	CONELOG® Bar abutments, 30° angled incl. light blue anodized abutment screw with reduced head, sterile Material Titanium alloy	C2258.3325		A		3.3 mm	2.5 mm	4.3 mm	
		C2258.3340					4.0 mm		
		C2259.3325		B	2.5 mm		4.3 mm		
		C2259.3340			4.0 mm				
		C2258.3825	A	3.8 mm	2.5 mm				4.3 mm
		C2258.3840			4.0 mm				
		C2259.3825	B	2.5 mm	4.3 mm				
		C2259.3840		4.0 mm					
		C2258.4325	A	4.3 mm		2.5 mm	4.3 mm		
		C2258.4340				4.0 mm			
		C2259.4325	B			2.5 mm		4.3 mm	
		C2259.4340				4.0 mm			
		C2258.5035	A		5.0 mm	3.5 mm			6.0 mm
		C2258.5050				5.0 mm			
		C2259.5035	B	3.5 mm		6.0 mm			
		C2259.5050		5.0 mm					

Types A and B see page 8

Occlusally screw-mounted prosthetics





	Article	Art. No.	Ø			Dimensionen
	Orientation gauge for COMFOUR® for Ø 2.0 mm pilot drilling Material Nitinol	J3551.0001	-			-
	Aligning tool for angled bar abutments, for insertion posts	J2269.0005	-			17°
	Material Stainless steel	J2269.0006	-			30°
	Gingiva height indicator, straight Material Titanium alloy	J3550.3300	3.3 mm			-
		J3550.3800	3.8 mm			
		J3550.4300	4.3 mm			
		J3550.5000	5.0 mm			
	Insertion tool for impression posts and healing caps for bar abutments Material Stainless steel	J5300.0027	3.3 mm	3.8 mm	4.3 mm	19.1 mm
		J5300.0028	5.0 mm			
	Healing cap for bar abutment light blue partially anodized, sterile Material Titanium alloy	J2029.4300	3.3 mm	3.8 mm	4.3 mm	-
		J2029.6000	5.0 mm			
	Impression cap, short, for bar abutment, closed tray (bridge/bar) light blue partially anodized, sterile Material Titanium alloy	J2129.4300	3.3 mm	3.8 mm	4.3 mm	6.5 mm
		J2129.6000	5.0 mm			7.0 mm
	Impression cap, long, for bar abutment, closed tray (bridge/bar) light blue partially anodized, sterile Material Titanium alloy	J2129.4310	3.3 mm	3.8 mm	4.3 mm	11.0 mm
		J2129.6010	5.0 mm			
	Bar lab analog for bar abutments Material Stainless steel	J3020.4300	3.3 mm	3.8 mm	4.3 mm	-
		J3020.6000	5.0 mm			
	Bar implant analog for bar abutments for printed and cast models Material Stainless steel	J3025.4300	3.3 mm	3.8 mm	4.3 mm	-
		J3025.6000	5.0 mm			
	Scanning cap for bar abutments incl. prosthetic screw, light blue anodized, sterile Material PEEK	J2610.4300	3.3 mm	3.8 mm	4.3 mm	-
		J2610.6000	5.0 mm			

	Article	Art. No.	Ø			Dimensions
	Titanium cap for bar abutment, for crown incl. prosthetic screw, light blue anodized, sterile	J2259.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy	J2259.6001	5.0 mm			
	Titanium cap for bar abutment, for bridge incl. prosthetic screw, light blue anodized, sterile	J2259.4302	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy	J2259.6002	5.0 mm			
	Titanium cap without retention for bar abutment, for bridge incl. prosthetic screw, light blue anodized	J2259.4322	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy	J2259.6022	5.0 mm			
	Crown base for bar abutment burn-out	J2256.4306	3.3 mm	3.8 mm	4.3 mm	-
	Material POM	J2256.6006	5.0 mm			
	Base for bar abutment burn-out	J2257.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material POM	J2257.6001	5.0 mm			
	Base for bar abutment cast-on	J2263.4300	3.3 mm	3.8 mm	4.3 mm	approx. 0.48 g
	Material Cast-on gold alloy / POM	J2263.6000	5.0 mm			approx. 0.70 g
	Base for bar abutment solderable	J2258.4300	3.3 mm	3.8 mm	4.3 mm	-
	Material Solderable gold alloy	J2258.6000	5.0 mm			
	Base for bar abutment, titanium laser-weldable	J2262.4300	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium Grade 4	J2262.6000	5.0 mm			
	Titanium bonding base for bar abutment Passive Fit	J2260.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy	J2260.6001	5.0 mm			
	Bar sleeve for titanium bonding base burn-out, Passive-Fit, incl. prosthetic screw for bar abutment, hex, (only for fabrication of the cast framework in conjunction with bar sleeves for titanium bonding base Passive Fit)	J2261.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material POM	J2261.6001	5.0 mm			

Occlusally screw-mounted prosthetics

	Article	Art. No.	Ø			Thread
	Polishing protection for caps and bases for bar abutment	J3021.4300	3.3 mm	3.8 mm	4.3 mm	M1.6
	Material Titanium alloy	J3021.6000	5.0 mm			M2.0
	CONELOG® Abutment screw with reduced head, hex, light blue anodized	C4004.1601	3.3 mm	3.8 mm	4.3 mm	M1.6
	Material Titanium alloy	C4004.2001	5.0 mm			M2.0
	CONELOG® Lab screw with reduced head, hex, light blue partially anodized	C4004.1600	3.3 mm	3.8 mm	4.3 mm	M1.6
	Material Titanium alloy	C4004.2000	5.0 mm			M2.0
	Prosthetic screw for bar abutment hex, light blue anodized (for final fixation of the restoration)	J4012.1601	3.3 mm	3.8 mm	4.3 mm	M1.6
	Material Titanium alloy	J4012.2001	5.0 mm			M2.0
	Lab prosthetic screw for bar abutment hex, brown anodized	J4013.1601	3.3 mm	3.8 mm	4.3 mm	M1.6
	Material Titanium alloy	J4013.2001	5.0 mm			M2.0

Lab screws must not be used on patients!

	Article	Art. No.	Ø	Thread
	Screw, hex, length 10 mm can be shortened by 2.5 mm, light blue anodized, sterile	J4012.1610	-	M1.6
	Material Titanium alloy	J4012.2010		M2.0
	Screw, hex, length 15 mm can be shortened by 2.5 mm, light blue anodized, sterile	J4012.1615	-	M1.6
	Material Titanium alloy	J4012.2015		M2.0
	Screw, hex, length 20 mm can be shortened by 2.5 mm, light blue anodized, sterile	J4012.1620	-	M1.6
	Material Titanium alloy	J4012.2020		M2.0
	Plastic screw for bar abutment Hex, length 27 mm, sterile	J4009.1627	-	M1.6
	Material PEEK	J4009.2027		M2.0



We are Implantology





Combined forces. Accelerated evolution.

Inspired to achieve excellence in oral reconstruction, we use our combined forces to accelerate evolution within global implantology.

Since 2016, BioHorizons and Camlog have been strategically joining forces under the umbrella of the Henry Schein Global Oral Reconstruction Group.

www.biohorizonscamlog.com





Ball abutment anchoring system



	Article	Art. No.	Ø	GH
	CONELOG® Ball abutment, male part incl. stabilizing ring Material Titanium alloy / plastic	C2249.3315	3.3 mm	1.5 mm
		C2249.3330		3.0 mm
		C2249.3815	3.8 mm	1.5 mm
		C2249.3830		3.0 mm
		C2249.3845	4.3 mm	4.5 mm
		C2249.4315		1.5 mm
		C2249.4330	5.0 mm	3.0 mm
		C2249.4345		4.5 mm
		C2249.5015	5.0 mm	1.5 mm
		C2249.5030		3.0 mm
C2249.5045	4.5 mm			
	CM Dalbo®-Plus matrix for ball abutment, incl. lamella retention insert and duplicating aid Material Titanium Grade 4 / gold alloy	05003503	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	
	Lamella retention insert for CM Dalbo®-Plus matrix Material Gold alloy	05003504	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	
	Ball abutment analog incl. stabilizing ring Material Brass/plastic	C3015.3300	3.3 mm	-
			3.8 mm	
			4.3 mm	
		C3015.5000	5.0 mm	

Dalbo®-Plus is a registered trademark of Cendres + Métaux SA, Bienne, Switzerland.

Locator® Anchoring System




CONELOG® Locator R-Tx®



	Article	Art. No.	Ø	GH
	CONELOG® Locator R-Tx® Abutment incl. retention housing with black processing replacement male, block out spacer white and four different replacement males Material Titanium alloy / Nylon	30805-01	3.3 mm	1.0 mm
		30805-02		2.0 mm
		30805-03		3.0 mm
		30805-04		4.0 mm
		30806-01	3.8 mm	1.0 mm
		30806-02		2.0 mm
		30806-03		3.0 mm
		30806-04		4.0 mm
		30806-05		5.0 mm
		30807-01	4.3 mm	1.0 mm
		30807-02		2.0 mm
		30807-03		3.0 mm
		30807-04		4.0 mm
		30807-05		5.0 mm
		30808-01	5.0 mm	1.0 mm
		30808-02		2.0 mm
		30808-03		3.0 mm
		30808-04		4.0 mm
		30808-05		5.0 mm
	Locator R-Tx® Impression cap (4 units) Material Polyethylene	30017-01	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	
	Locator R-Tx® Analog Ø 3.35 mm (4 units) Material Aluminum	30014-01	3.3 mm	-
			3.8 mm	
			4.3 mm	
	Locator R-Tx® Analog Ø 5.0 mm (4 units) Material Aluminum	30016-01	5.0 mm	-

	Article	Art. No.	Ø
	Locator R-Tx® Retention housing with processing replacement male, black (4 units) Material Titanium alloy / polyethylene	30013-01	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator R-Tx® Processing replacement male black (4 units) Material Polyethylene	30012-01	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator R-Tx® Spacer/duplication aid (4 units) Material Polyethylene	30018-01	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator R-Tx® Replacement male gray, NO RETENTION (4 units) Material Nylon	30001-01	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator R-Tx® Replacement male blue, LOW (4 units) Material Nylon	30002-01	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator R-Tx® Replacement male pink, MEDIUM (4 units) Material Nylon	30003-01	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator R-Tx® Replacement male white, HIGH (4 units) Material Nylon	30004-01	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm

Locator® Anchoring System

CONELOG® Locator®





	Article	Art. No.	Ø	GH
	CONELOG® Locator® Abutment Material Titanium alloy / TiN	C2253.3310	3.3 mm	1.0 mm
		C2253.3320		2.0 mm
		C2253.3330		3.0 mm
		C2253.3340		4.0 mm
		C2253.3810	3.8 mm	1.0 mm
		C2253.3820		2.0 mm
		C2253.3830		3.0 mm
		C2253.3840		4.0 mm
		C2253.3850		5.0 mm
		C2253.4310	4.3 mm	1.0 mm
		C2253.4320		2.0 mm
		C2253.4330		3.0 mm
		C2253.4340		4.0 mm
		C2253.4350		5.0 mm
		C2253.5010	5.0 mm	1.0 mm
		C2253.5020		2.0 mm
		C2253.5030		3.0 mm
C2253.5040	4.0 mm			
C2253.5050	5.0 mm			
	Locator® Impression cap (4 units) Material Aluminum/polyethylene	J2253.0200	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	
	Locator® Analog (4 units) Material Aluminum	J2253.0340	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	

	Article	Art. No.	Ø
	Locator® Lab kits (2 units) Contents per kit: 1 Retention housing with processing replacement male 1 Block out spacer, white 1 Replacement male, clear 1 Replacement male, pink 1 Replacement male, blue Material Titanium alloy / polyethylene / Teflon / Nylon	J2253.0102	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Lab kits for extended angulation (2 units) Contents per kit: 1 Retention housing with processing replacement male 1 Block out spacer, white 1 Replacement male, green 1 Replacement male, orange 1 Replacement male, red Material Titanium alloy / polyethylene / Teflon / Nylon	J2253.0112	3.8 mm
			4.3 mm
			5.0 mm
	Locator® Block out spacer (20 units) Material Teflon	J2253.0401	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Processing replacement male (4 units) Material Polyethylene	J2253.0402	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm

Prosthetics

Locator® Anchoring System



CONELOG® Locator®

	Article	Art. No.	Ø
	Locator® Replacement male clear, HIGH, Div.: 0°-10° (4 units) Material Nylon	J2253.1005	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male pink, MEDIUM, Div.: 0°-10° (4 units) Material Nylon	J2253.1003	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male blue, LOW, Div.: 0°-10° (4 units) Material Nylon	J2253.1002	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male for extended angulation green, HIGH, Div.: 10°-20° (4 units) Material Nylon	J2253.2004*	3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male for extended angulation orange, MEDIUM, Div.: 10°-20° (4 units) Material Nylon	J2253.2003*	3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male for extended angulation red, LOW, Div.: 10°-20° (4 units) Material Nylon	J2253.2002*	3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male for extended angulation gray, NO RETENTION, Div.: 0°-20° (4 units) Material Nylon	J2253.2000*	3.8 mm
			4.3 mm
			5.0 mm




* not permitted for implant Ø 3.3 mm

Manufacturer Locator®: Zest Anchors | 2875 Loker Avenue East, Carlsbad | California 92010 | USA
Locator® and Locator R-Tx® are registered trademarks of the Zest Anchors company.

Double crown restoration

	Article	Art. No.	Ø
 11 mm	CONELOG® Universal abutment for the double crown technique preparable, incl. CONELOG® Abutment screw Material Titanium alloy	C2211.3800	3.8 mm
		C2211.4300	4.3 mm
		C2211.5000	5.0 mm
 12 mm	CONELOG® Telescope abutment for the double crown technique preparable, incl. CONELOG® Abutment screw Material Titanium alloy	C2212.3800	3.8 mm
		C2212.4300	4.3 mm
		C2212.5000	5.0 mm

Accessories for abutments



	Article	Art. No.	Ø	Thread
	CONELOG® Abutment screw, hex for the final screwing of abutments into the implant Material Titanium alloy	C4005.1601	3.3 mm	M1.6
			3.8 mm	
			4.3 mm	
		C4005.2001	5.0 mm	M2.0
	CONELOG® Lab screw, hex for fixation on the working model, brown anodized Material Titanium alloy	C4006.1601	3.3 mm	M1.6
			3.8 mm	
			4.3 mm	
		C4006.2001	5.0 mm	M2.0
	CONELOG® Lab screw, hex (3 units) for fixation on the working model, brown anodized Material Titanium alloy	C4006.1603	3.3 mm	M1.6
			3.8 mm	
			4.3 mm	
		C4006.2003	5.0 mm	M2.0

"CONELOG® Abutment Screw for CONELOG® Titanium Base CAD/CAM dark purple anodized" must be used for titanium bases, (see page 69).


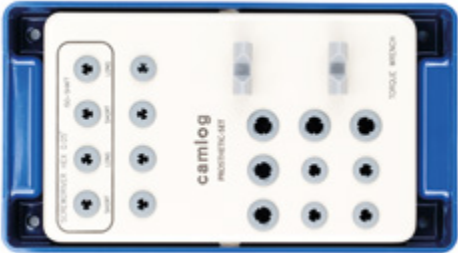




Lab screws must not be used on patients!




Prosthetic instruments



	Article	Art. No.	L
	<p>Torque wrench with continuous torque adjustment until maximal 30 Ncm</p> <p>Material Stainless steel</p>	J5320.1030	-
	<p>Insertion tool for ball abutment, manual/wrench</p> <p>Material Stainless steel</p>	J5300.0011	18.3 mm
	<p>Screwdriver activator for CM Dalbo®-Plus ball abutment matrix</p> <p>Material Stainless steel</p>	07000389	-
	<p>Insertion tool for straight bar abutments, short Ø 3.3/3.8/4.3 mm</p> <p>Material Stainless steel</p>	J5300.0020	18.6 mm
	<p>Insertion tool for straight bar abutments, short Ø 5.0 mm</p> <p>Material Stainless steel</p>	J5300.0025	18.6 mm

	Article	Art. No.	L
	Insertion tool for straight bar abutments, long Ø 3.3/3.8/4.3 mm Material Stainless steel	J5300.0021	28.0 mm
	Insertion tool for impression posts and healing caps for bar abutments Ø 3.3/3.8/4.3 mm Material Stainless steel	J5300.0027	19.1 mm
	Insertion tool for impression posts and healing caps for bar abutments Ø 5.0 mm Material Stainless steel	J5300.0028	19.1 mm
	Insertion tool for Locator®, manual/wrench Material Stainless steel	J2253.0001	24.3 mm
	Locator® Instrument 3-part Material Stainless steel	J2253.0002	83.0 mm
	Locator® Abutment holder sleeve for golden element of the Locator® Instrument (4 units) Material Polysulfone	08394	-
	Locator® Angle measurement guide Material Stainless steel	J2253.0003	-
	Locator® Parallel post (4 units) Material Polyethylene	J2253.0004	-






Prosthetic instruments

	Article	Art. No.	Dimensions
	<p>Locator R-Tx® Insertion tool for replacement males with plastic handle</p> <p>Material Stainless steel</p>	30021-01	-
	<p>Prosthetic tray (without content)</p> <p>Material Plastic</p>	J5330.8500	197 × 108 × 54 mm
	<p>Prosthetic tray Universal (without content) resterilizable</p> <p>Material Radel®, silicone</p>	J5330.8700	162 × 73 × 29 mm
	<p>Screwdriver hex, extra short, manual/wrench</p> <p>Material Stainless steel</p>	J5317.0510	14.5 mm
	<p>Screwdriver hex, short, manual/wrench</p> <p>Material Stainless steel</p>	J5317.0501	22.5 mm
	<p>Screwdriver hex, long, manual/wrench</p> <p>Material Stainless steel</p>	J5317.0502	30.3 mm

	Article	Art. No.	L
	Screwdriver hex, short, ISO shaft Material Stainless steel	J5317.0504	18.0 mm
	Screwdriver hex, long, ISO shaft Material Stainless steel	J5317.0503	26.0 mm
	Manual screwdriver hex, without wrench head connection Material Stainless steel	J5317.0511	23.0 mm

	Article	Art. No.	Ø	Thread
	CONELOG® Disconnecter for CONELOG® Abutments, short Material Stainless steel	C5300.1601	3.3 mm	M1.6
			3.8 mm	
			4.3 mm	
		C5300.2001	5.0 mm	M2.0
	CONELOG® Disconnecter for CONELOG® Abutments, long Material Stainless steel	C5300.1603	3.3 mm	M1.6
			3.8 mm	
			4.3 mm	
		C5300.2003	5.0 mm	M2.0

Instruments for dental technicians

	Article	Art. No.	Ø
	Handle for CAMLOG®/CONOLOG® Implant analog Material Stainless steel	J3025.0010	3.3 mm
			3.8 mm
			4.3 mm
		J3025.0015	5.0 mm
	Universal holder incl. 2 CONELOG® Lab screws, hex, and 1 each CONELOG® Abutment collet Ø 3.3/3.8/4.3/5.0 mm Material Stainless steel / titanium alloy	C3709.0010	-
	Universal holder Material Stainless steel	J3709.0015	-
	CONELOG® Abutment collet for universal holder, for grinding CONELOG® Abutments Material Titanium alloy	C3709.3300	3.3 mm
		C3709.3800	3.8 mm
		C3709.4300	4.3 mm
		C3709.5000	5.0 mm
	Reworking reamer, base for bar abutment plane surface/cone seat, for burn-out caps Material Stainless steel / brass	J3711.0010	3.3 mm
			3.8 mm
			4.3 mm
		J3711.0015	5.0 mm
	Reworking reamer, base for bar abutment screw seat, for burn-out caps Material Stainless steel / brass	J3711.0020	3.3 mm
			3.8 mm
			4.3 mm
		J3711.0025	5.0 mm

Selection Abutments


	Article	Art. No.
	CONELOG® Selection abutment kit (Contents: 2 units each, according to table below)	C8011.1000

Contents: CONELOG® Selection abutment kit					
Article	Material	Ø			GH
CONELOG® Esthomic® Selection abutment , straight*	POM	3.8 mm	4.3 mm	1.5-2.5	3.0-4.5
CONELOG® Esthomic® Selection abutment, 15° angled, type A*				1.5-2.5	
CONELOG® Esthomic® Selection abutment, 15° angled, type B*				1.5-2.5	
CONELOG® Esthomic® Selection abutment, 20° angled, type A*				1.5-2.5	
CONELOG® Esthomic® Selection abutment, 20° angled, type B*				1.5-2.5	

* These products are not available singly.



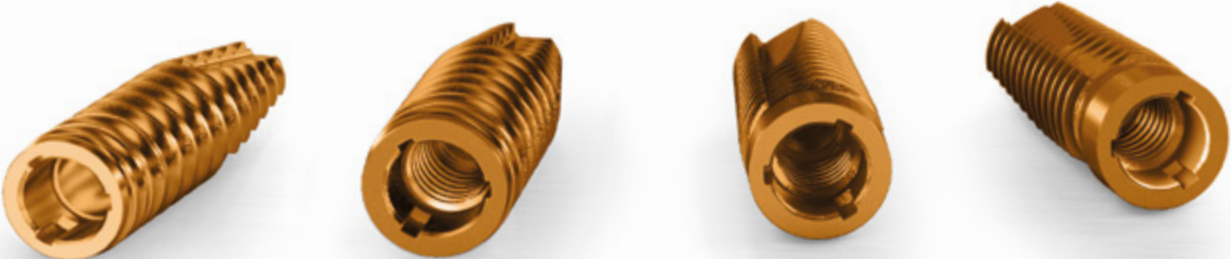

Selection abutments must not be used on patients!

Auxiliary Articles






Implants for practice




	Article	Art. No.	Ø	L
	CONELOG® PROGRESSIVE-LINE Implant for practice incl. snap-in insertion post and cover screw, brown anodized Material Titanium alloy	C1901.3813	3.8 mm	13 mm
	CONELOG® PROGRESSIVE-LINE Implant for practice incl. snap-in insertion post and cover screw, brown anodized Material Titanium alloy	C1901.4313	4.3 mm	
	CONELOG® SCREW-LINE Implant for practice incl. insertion post and cover screw, brown anodized Material Titanium alloy	C1069.3813	3.8 mm	13 mm
	CONELOG® SCREW-LINE Implant for practice incl. insertion post and cover screw, brown anodized Material Titanium alloy	C1069.4313	4.3 mm	

Implants for practice must not be used on patients!



Insertion posts

	Article	Art. No.	Ø
	CONELOG® Insertion post, screw-mounted for CONELOG® Lab analog/implant analog, incl. fixing screw (2 units) Material Titanium alloy	C2026.3303	3.3 mm
		C2026.3803	3.8 mm
		C2026.4303	4.3 mm
		C2026.5003	5.0 mm

Demonstration models




	Article	Art. No.
	<p>CONELOG® Demonstration model, acrylic glass Upper jaw, 4 CONELOG® SCREW-LINE Implants, 4 × Ø 4.3 mm</p> <p>Material Acrylic glass / titanium</p>	C8070.1020
	<p>CONELOG® Demonstration model, acrylic glass Lower jaw, 4 CONELOG® SCREW-LINE Implants, 4 × Ø 4.3 mm</p> <p>Material Acrylic glass / titanium</p>	C8050.1040
	<p>Edentulous mandible incl. mounting plate</p> <p>Material Plastic</p>	J8070.2050

Macro Models




	Article	Art. No.
	<p>CONELOG® PROGRESSIVE-LINE Macro model Scale 3:1</p> <p>Content: 1 CONELOG® PROGRESSIVE-LINE Implant 1 CONELOG® Esthomic® Abutment , straight 1 CONELOG® Abutment screw, hex 1 CONELOG® Screwdriver, hex 1 Premolar, suitable for CONELOG® Esthomic® Abutment, straight 1 Acrylic base</p> <p>Material Plastic / stainless steel</p>	C8010.1400
	<p>CONELOG® SCREW-LINE Macro model Scale 3:1</p> <p>Content: 1 CONELOG® SCREW-LINE Implant 1 CONELOG® Esthomic® Abutment , straight 1 CONELOG® Abutment screw, hex 1 Screwdriver, hex 1 Premolar, suitable for CONELOG® Esthomic® Abutment, straight 1 Acrylic base</p> <p>Material Plastic / stainless steel</p>	C8010.1010

Literature

	Article	Media No. / Art. No.
	<p>Patient brochure Dental implants – inspired by nature</p>	<p>M-0431-BRO-EN-INT- BHCL-00-052023</p>
	<p>COMFOUR® Patient brochure Bridge instead of dentures – dental prosthesis with feel-good factor</p>	<p>M-1437-BRO-EN-INT- BHCL-00-052023</p>
	<p>Biomaterial patient brochure Stable bone and a firm gingiva – the basis of oral health</p>	<p>M-0151-BRO-EN-INT- BHCL-00-052023</p>
	<p>Patient Documentation and Implant Card Patient-specific documentation of implant restoration</p>	<p>J8000.0372</p>
	<p>Patient advice sheets Set, A4</p>	<p>M-0584-FLY-EN-INT- BHCL-00-052023</p>

	Article	Media No.
	<p>Presentation folder A4, laminated</p>	<p>M-0258-BUE-EN-INT- BHCL-00-052023</p>
	<p>Poster Dental implants – inspired by nature Format: 50 × 70 cm</p>	<p>M-1628-PST-EN-INT- BHCL-00-052023</p>
	<p>Appointment pad 50 sheets/pad, A7 Packaging units: 5 units</p>	<p>M-1629-FOR-EN-INT- BHCL-052023</p>












Literature











	Article	Media No. / Art. No.
	<p>Patient flyer Single tooth</p>	<p>M-0446-FLY-EN-INT- BHCL-00-072021</p>
	<p>Patient flyer Multiple teeth solution</p>	<p>M-0447-FLY-EN-INT- BHCL-00-072021</p>
	<p>Patient flyer Edentulous</p>	<p>M-0448-FLY-EN-INT- BHCL-00-072021</p>



www.biohorizonscamlog.com/patient-information

Indication overview

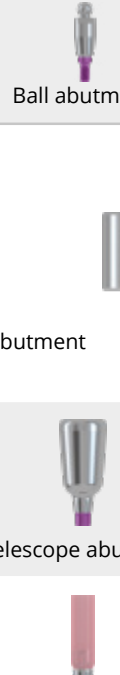Single-tooth restoration		Bridge re
Cemented	Screw-mounted	Cemented
	 <p>Temporary abutments, titanium alloy, crown</p>	
 <p>Esthomic® Abutments</p>		 <p>Esthomic® Abutments</p>
	 <p>Bar abutments</p>	
 <p>Titanium base CAD/CAM, crown</p>	 <p>Titanium base CAD/CAM, crown</p>	 <p>Titanium base CAD/CAM, bridge</p>
 <p>Universal abutment CAM blank</p>		 <p>Universal abutment CAM blank</p>
 <p>Gold-plastic abutment</p>	 <p>Gold-plastic abutment</p>	 <p>Gold-plastic abutment</p>



Restoration	Hybrid restoration
Screw-mounted	Removable (full denture)
 <p>Temporary abutments, titanium alloy, bridge</p>	
 <p>Bar abutments</p>	 <p>Bar abutments</p>
 <p>Titanium base CAD/CAM, bridge</p>	
	 <p>Locator® Anchoring System</p>
	 <p>Ball abutment</p>
	 <p>Universal abutment CAM blank</p>
	 <p>Telescope abutment</p>
	 <p>Gold-plastic abutment</p>
	 <p>Titanium base CAD/CAM, crown</p>


Double crown restoration

Additional Information



Implant overview

PROGRESSIVE-LINE

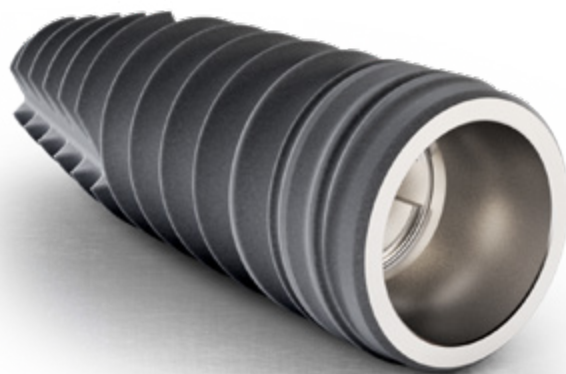	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article	Art. No. A Ø				L
 CONELOG® PROGRESSIVE-LINE Implant, Promote® plus with snap-in insertion post	-	C1086.3807 A Ø 3.0 mm	C1086.4307 A Ø 3.0 mm	C1086.5007 A Ø 3.5 mm	7 mm
	C1086.3309 A Ø 2.2 mm	C1086.3809 A Ø 3.0 mm	C1086.4309 A Ø 3.0 mm	C1086.5009 A Ø 3.5 mm	9 mm
	C1086.3311 A Ø 2.2 mm	C1086.3811 A Ø 2.7 mm	C1086.4311 A Ø 2.7 mm	C1086.5011 A Ø 3.2 mm	11 mm
	C1086.3313 A Ø 2.2 mm	C1086.3813 A Ø 2.7 mm	C1086.4313 A Ø 2.7 mm	C1086.5013 A Ø 3.2 mm	13 mm
	C1086.3316 A Ø 2.2 mm	C1086.3816 A Ø 2.7 mm	C1086.4316 A Ø 2.7 mm	C1086.5016 A Ø 3.2 mm	16 mm
 CONELOG® PROGRESSIVE-LINE Implant, Promote® plus with screw-mounted insertion post	-	C1085.3807 A Ø 3.0 mm	C1085.4307 A Ø 3.0 mm	C1085.5007 A Ø 3.5 mm	7 mm
	C1085.3309 A Ø 2.2 mm	C1085.3809 A Ø 3.0 mm	C1085.4309 A Ø 3.0 mm	C1085.5009 A Ø 3.5 mm	9 mm
	C1085.3311 A Ø 2.2 mm	C1085.3811 A Ø 2.7 mm	C1085.4311 A Ø 2.7 mm	C1085.5011 A Ø 3.2 mm	11 mm
	C1085.3313 A Ø 2.2 mm	C1085.3813 A Ø 2.7 mm	C1085.4313 A Ø 2.7 mm	C1085.5013 A Ø 3.2 mm	13 mm
	C1085.3316 A Ø 2.2 mm	C1085.3816 A Ø 2.7 mm	C1085.4316 A Ø 2.7 mm	C1085.5016 A Ø 3.2 mm	16 mm





SCREW-LINE

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm
		A Ø 2.7 mm	A Ø 3.5 mm	A Ø 3.9 mm	A Ø 4.6 mm
Article	Art. No.				L
 <p>CONELOG® SCREW-LINE Implant, Promote® plus with snap-in insertion post</p>	-	C1066.3807	C1066.4307	C1066.5007	7 mm
	C1066.3309	C1066.3809	C1066.4309	C1066.5009	9 mm
	C1066.3311	C1066.3811	C1066.4311	C1066.5011	11 mm
	C1066.3313	C1066.3813	C1066.4313	C1066.5013	13 mm
	C1066.3316	C1066.3816	C1066.4316	C1066.5016	16 mm
 <p>CONELOG® SCREW-LINE Implant, Promote® plus with screw-mounted insertion post</p>	-	C1065.3807	C1065.4307	C1065.5007	7 mm
	C1065.3309	C1065.3809	C1065.4309	C1065.5009	9 mm
	C1065.3311	C1065.3811	C1065.4311	C1065.5011	11 mm
	C1065.3313	C1065.3813	C1065.4313	C1065.5013	13 mm
	C1065.3316	C1065.3816	C1065.4316	C1065.5016	16 mm






Prosthetic overview


Scanbodies

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	CONELOG® Scanbody	C2600.3310	C2600.4310	C2600.4310	C2600.5010	-
	CONELOG® ScanPost for Sirona® Scanbody	C2620.3306	C2620.3806	C2620.4306	C2620.5006	-




Implant impression taking

	CONELOG® Impression post, open tray	C2121.3300	C2121.3800	C2121.4300	C2121.5000	-
	CONELOG® Impression post, closed tray	C2110.3300	C2110.3800	C2110.4300	C2110.5000	-
	Impression cap for impression posts, closed tray	J2111.3300	J2111.3800	J2111.4300	J2111.5000	-








Bite registration

	CONELOG® Bite registration post incl. bite registration cap	C2140.3300	C2140.3800	C2140.4300	C2140.5000	-
---	---	------------	------------	------------	------------	---

Cast fabrication









		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	CONELOG® Lab analog for cast models	C3010.3300	C2211.3300	C3010.4300	C3010.5000	-
		C3010.3303	C3010.3803	C3010.4303	C3010.5003	
	CONELOG® Implant analog for printed and cast models	C3025.3300	C3025.3800	C3025.4300	C3025.5000	-
		C3025.3303	C3025.3803	C3025.4303	C3025.5003	
	DIM Analog® for the CONELOG® Implant System for printed models	C3012.3300	C3012.4300	C3012.4300	C3012.5000	-

Abutments for crown and bridge restorations
















	CONELOG® Temporary abutment, crown, titanium alloy	C2239.3300	C2239.3800	C2239.4300	C2239.5000	-
	CONELOG® Temporary abutment, bridge, titanium alloy	C2339.3300	C2339.3800	C2339.4300	C2339.5000	-
	CONELOG® Titanium base CAD/CAM, crown	C2242.3308	C2242.3808	C2242.4308	C2242.5008	0.8 mm
		C2242.3320	C2242.3820	C2242.4320	C2242.5020	2.0 mm
	CONELOG® Titanium base CAD/CAM, bridge	C2342.3308	C2342.3808	C2342.4308	C2342.5008	0.8 mm
		C2342.3320	C2342.3820	C2342.4320	C2342.5020	2.0 mm
	CONELOG® CAM titanium blank, type IAC	C2431.3313	C2431.3813	C2431.4313	C2431.5013	
	CONELOG® CAM titanium blank, type ME	C2441.3320	C2441.3820	C2441.4320	C2441.5020	
	CONELOG® CAM CoCr blank, type ME	C2461.3320	-	C2461.4320	C2461.5020	

Prosthetic overview

Abutments for crown and bridge restorations

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	CONELOG® Esthomic® Abutments, straight	-	C2226.3815	C2226.4315	C2226.5015	1.5–2.5 mm
		-	C2226.3830	C2226.4330	C2226.5030	3.0–4.5 mm
	CONELOG® Esthomic® Abutment, Inset	C2235.3320	C2235.3820	C2235.4320	C2235.5020	2.0–3.3 mm
	CONELOG® Esthomic® Abutments 15° angled, type A	-	C2227.3815	C2227.4315	C2227.5015	1.5–2.5 mm
		-	C2227.3830	C2227.4330	C2227.5030	3.0–4.5 mm
	CONELOG® Esthomic® Abutments 15° angled, type B	-	C2228.3815	C2228.4315	C2228.5015	1.5–2.5 mm
		-	C2228.3830	C2228.4330	C2228.5030	3.0–4.5 mm
	CONELOG® Esthomic® Abutments 20° angled, type A	-	C2231.3815	C2231.4315	C2231.5015	1.5–2.5 mm
		-	C2231.3830	C2231.4330	C2231.5030	3.0–4.5 mm
	CONELOG® Esthomic® Abutments 20° angled, type B	-	C2232.3815	C2232.4315	C2232.5015	1.5–2.5 mm
		-	C2232.3830	C2232.4330	C2232.5030	3.0–4.5 mm
	CONELOG® Universal abutment	C2211.3300	C2211.3800	C2211.4300	C2211.5000	-
	CONELOG® Gold-plastic abutment	C2246.3300	C2246.3800	C2246.4300	C2246.5000	-





COMFOUR® Abutments for crown, bridge and hybrid restorations

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	CONELOG® Bar abutments, straight	C2254.3310	C2254.3810	C2254.4310	C2254.5010	1.0 mm
		C2254.3325	C2254.3825	C2254.4325	C2254.5025	2.5 mm
		-	C2254.3840	C2254.4340	C2254.5040	4.0 mm
	CONELOG® Bar abutments, 17° angled, type A	C2256.3325	C2256.3825	C2256.4325	C2256.5025	2.5 mm
		C2256.3340	C2256.3840	C2256.4340	C2256.5040	4.0 mm
	CONELOG® Bar abutments, 17° angled, type B	C2257.3325	C2257.3825	C2257.4325	C2257.5025	2.5 mm
		C2257.3340	C2257.3840	C2257.4340	C2257.5040	4.0 mm
	CONELOG® Bar abutments, 30° angled, type A	C2258.3325	C2258.3825	C2258.4325	C2258.5035	2.5 mm/ 3.5 mm*
		C2258.3340	C2258.3840	C2258.4340	C2258.5050	4.0 mm/ 5.0 mm*
	CONELOG® Bar abutments, 30° angled, type B	C2259.3325	C2259.3825	C2259.4325	C2259.5035	2.5 mm/ 3.5 mm*
		C2259.3340	C2259.3840	C2259.4340	C2259.5050	4.0 mm/ 5.0 mm*
	Healing cap for bar abutment	J2029.4300	J2029.4300	J2029.4300	J2029.6000	-
	Impression cap, short for bar abutment, closed tray	J2129.4300	J2129.4300	J2129.4300	J2129.6000	-
	Impression cap, long, for bar abutment, closed tray (bridge/bar)	J2129.4310	J2129.4310	J2129.4310	J2129.6010	-
	Scanning cap for bar abutments	J2610.4300	J2610.4300	J2610.4300	J2610.6000	-
	Titanium cap for bar abutment, for crown, sterile	J2259.4301	J2259.4301	J2259.4301	J2259.6001	-
	Titanium cap for bar abutment, for bridge, sterile	J2259.4302	J2259.4302	J2259.4302	J2259.6002	-
	Titanium cap without retention for bar abutment, for bridge	J2259.4322	J2259.4322	J2259.4322	J2259.6022	-
	Crown base for bar abutment, burn-out	J2256.4306	J2256.4306	J2256.4306	J2256.6006	-
	Base for bar abutment, burn-out	J2257.4301	J2257.4301	J2257.4301	J2257.6001	-
	Base for bar abutment, cast-on	J2263.4300	J2263.4300	J2263.4300	J2263.6000	-














* GH 3.5 and 5.0 mm only for Ø 5.0 mm

Prosthetic overview








COMFOUR® Abutments for crown, bridge and hybrid restorations

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	Base for bar abutment, solderable	J2258.4300	J2258.4300	J2258.4300	J2258.6000	-
	Base for bar abutment, titanium, laser-weldable	J2262.4300	J2262.4300	J2262.4300	J2262.6000	-
	Titanium bonding base for bar abutment, Passive-Fit	J2260.4301	J2260.4301	J2260.4301	J2260.6001	-
	Bar sleeve for titanium bonding base, burn-out, Passive-Fit	J2261.4301	J2261.4301	J2261.4301	J2261.6001	-

Hybrid restorations





















	CONELOG® Ball abutment, male part	C2249.3315	C2249.3815	C2249.4315	C2249.5015	1.5 mm
		C2249.3330	C2249.3830	C2249.4330	C2249.5030	3.0 mm
		-	C2249.3845	C2249.4345	C2249.5045	4.5 mm
	CM Dalbo®-Plus matrix	05003503	05003503	05003503	05003503	-
	Ball abutment analog	C3015.3300	C3015.3300	C3015.3300	C3015.5000	-
	CONELOG® Locator R-Tx® Abutment	30805-01	30806-01	30807-01	30808-01	1.0 mm
		30805-02	30806-02	30807-02	30808-02	2.0 mm
		30805-03	30806-03	30807-03	30808-03	3.0 mm
		30805-04	30806-04	30807-04	30808-04	4.0 mm
		-	30806-05	30807-05	30808-05	5.0 mm
	Locator R-Tx® Impression cap	30017-01	30017-01	30017-01	30017-01	-
	Locator R-Tx® Analog	30014-01	30014-01	30014-01	30016-01	-
	Locator R-Tx® Retention housing	30013-01	30013-01	30013-01	30013-01	-
	Locator R-Tx® Processing replacement male	30012-01	30012-01	30012-01	30012-01	-
	Locator R-Tx® Spacer/duplication aid	30018-01	30018-01	30018-01	30018-01	-
	Locator R-Tx® Replacement male gray, NO RETENTION	30001-01	30001-01	30001-01	30001-01	-
	Locator R-Tx® Replacement male, blue, LOW	30002-01	30002-01	30002-01	30002-01	-
	Locator R-Tx® Replacement male, pink, MEDIUM	30003-01	30003-01	30003-01	30003-01	-
	Locator R-Tx® Replacement male, white, HIGH	30004-01	30004-01	30004-01	30004-01	-

Hybrid restorations

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
 CONELOG® Locator® Abutment	C2253.3310	C2253.3810	C2253.4310	C2253.5010	1.0 mm	
	C2253.3320	C2253.3820	C2253.4320	C2253.5020	2.0 mm	
	C2253.3330	C2253.3830	C2253.4330	C2253.5030	3.0 mm	
	C2253.3340	C2253.3840	C2253.4340	C2253.5040	4.0 mm	
	-	C2253.3850	C2253.4350	C2253.5050	5.0 mm	
 Locator® Impression cap	J2253.0200	J2253.0200	J2253.0200	J2253.0200	-	
 Locator® Analog	J2253.0340	J2253.0340	J2253.0340	J2253.0340	-	
 Locator® Lab kit	J2253.0102	J2253.0102	J2253.0102	J2253.0102	-	
 Locator® Lab kit, for extended angulation	-	J2253.0112	J2253.0112	J2253.0112	-	
 CONELOG® Universal abutment	-	C2211.3800	C2211.4300	C2211.5000	-	
 CONELOG® Telescope abutment	-	C2212.3800	C2212.4300	C2212.5000	-	

Screw overview Abutment and prosthetic screws – intraoral use

Implant-abutment connection






	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
	M1.6			M2.0	
Article	CONELOG® Abutment screws				Tightening torque
 <p>Scanbodies ScanPost for Sirona® Scanbody</p>					hand-tight**
 <p>Temporary abutments titanium, crown and bridge</p>					
 <p>Esthomic® Abutments</p>					20 Ncm*
 <p>Universal abutment</p>	8.9 mm  C4005.1601		8.9 mm  C4005.2001		
 <p>Telescope abutment</p>					
 <p>Gold-plastic abutment</p>					
 <p>Logfit® Abutment</p>					
 <p>Vario SR abutments, 20° and 30° angled</p>					
 <p>CONELOG® CAM blank, type IAC and ME</p>					
CONELOG® Abutment screws for titanium base CAD/CAM, anodized dark purple					
 <p>Titanium base CAD/CAM, crown and bridge</p>	8.9 mm  C4015.1601		8.9 mm  C4015.2001		20 Ncm*
CONELOG® Vario SR abutment screws					
 <p>Vario SR abutment, straight</p>	10.6 mm  C4007.1600		10.6 mm  C4007.2000		20 Ncm*
CONELOG® Abutment screws with reduced head, light blue anodized					
 <p>COMFOUR® Bar abutments, 17° and 30° angled</p>	7.8 mm  C4004.1601		7.8 mm  C4004.2001		20 Ncm*

* with torque wrench J5320.1030

** optional for temporary abutments titanium: torque after completed healing phase 20 Ncm













All screws must be retightened with the corresponding torque after at least 5 minutes!

Abutment-Prosthetic connection

	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
	M1.6			M2.0	
Article	Prosthetic screws for bar abutments, light blue anodized				Tightening torque
 <p>COMFOUR® Bar abutments, straight, 17° and 30° angled</p>	3.6 mm  J4012.1601		3.8 mm  J4012.2001		15 Ncm*
	Vario SR prosthetic screw, yellow anodized				
 <p>Vario SR abutments, straight, 20° and 30° angled</p>	4 mm  J4005.2004				15 Ncm*

Overview Auxiliary Screws intra and extraoral use

Abutment-Prosthetic connection





















	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm		
	M1.6			M 2.0		
Article	Prosthetic screws for bar abutments, light blue anodized				Tightening torque	
 <p>Scanning cap for bar abutments</p>	3.6 mm  J4012.1601		3.8 mm  J4012.2001		hand-tight	
Screws for bar abutments, for open tray impression taking and for soldering, light blue anodized						
 <p>COMFOUR® Bar abutments, straight, 17° and 30° angled</p>	12 mm  J4012.1610		12.2 mm  J4012.2010		hand-tight	
	17 mm  J4012.1615		17.2 mm  J4012.2015			
	22 mm  J4012.1620		22.2 mm  J4012.2020			
	Plastic screws for bar abutment, as fixation and bonding aid, beige					
		29 mm  J4009.1627		29.2 mm  J4009.2027		hand-tight

* with torque wrench J5320.1030

All screws must be retightened with the corresponding torque after at least 5 minutes!

Screw Overview lab screws – extraoral use












Lab analog-abutment connection

	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
	M1.6			M2.0	
Article	CONELOG® Lab screws*, brown anodized				Tightening torque
 <p>Scanbodies ScanPost for Sirona® Scanbody</p>					hand-tight
 <p>Temporary abutments titanium, crown and bridge</p>					
 <p>Esthomic® Abutments</p>	8.9 mm  C4006.1601			8.9 mm  C4006.2001	
 <p>Universal abutment Telescope abutment Gold-plastic abutment</p>					
 <p>Vario SR abutments, 20° and 30° angled</p>					
 <p>CONELOG® CAM blank, type IAC and ME</p>					
CONELOG® Lab screws* for titanium base CAD/CAM brown, partially anodized					
 <p>Titanium base CAD/CAM, crown and bridge</p>	8.9 mm  C4016.1601			8.9 mm  C4016.2001	hand-tight
CONELOG® Bonding aids**					
 <p>Titanium base CAD/CAM, crown and bridge</p>	26 mm 			26 mm 	hand-tight
CONELOG® Vario SR lab screws*, brown anodized					
 <p>Vario SR abutment, straight</p>	10.6 mm  C4008.1600			10.6 mm  C4008.2000	hand-tight
CONELOG® Lab screws* with reduced head, light blue partially anodized					
 <p>COMFOUR® Bar abutments, 17° and 30° angled</p>	7.8 mm  C4004.1600			7.8 mm  C4004.2000	hand-tight

* Lab screws must not be used on patients!













** not available singly, are included in the packaging of the titanium base CAD/CAM

Abutment-Prosthetic connection

	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
	M1.6			M2.0	
Article	Lab prosthetic screws* for bar abutments, brown anodized				Tightening torque
 Scanning cap for bar abutments					
 COMFOUR® Bar abutments, straight, 17° and 30° angled	3.6 mm  J4013.1601			3.8 mm  J4013.2001	hand-tight
 Bar lab analog for bar abutments					
Vario SR prosthetic screw, yellow anodized					
 Vario SR abutments, straight, 20° and 30° angled	4 mm  J4005.2004				hand-tight
 Vario SR analog					
Prosthetic screws for bar abutments*, for fabricating the wax-up on the burn-out bar sleeve for titanium adhesive base, Passive-Fit, on the bar lab analog					
 Titanium bonding base for bar abutment and bar sleeve for titanium bonding base, burn-out, Passive-Fit	5.5 mm  J4005.1602			5.5 mm  J4005.2002	hand-tight

* Lab screws must not be used on patients!




























Overview tightening torques

Article	Instrument	Tightening torque
 <p>Implant cover screw</p>		
 <p>Healing caps cylindrical, wide body, bottleneck</p>		
 <p>Impression posts Bite registration posts</p>		hand-tight**
 <p>Lab screws Lab screws with reduced head</p>		
 <p>Temporary abutment, titanium alloy, crown and bridge</p>		
 <p>Abutment screws Abutment screws with reduced head</p>	 <p>J5317.0510 J5317.0501 J5317.0502</p>	
 <p>Esthomic® Abutment, straight Esthomic® Abutment, 15° and 20° angled Esthomic® Abutment, Inset</p>	 <p>J5317.0504 J5317.0503</p>	
 <p>Universal abutment Telescope abutment Gold-plastic abutment</p>		20 Ncm*
 <p>Logfit® Abutments Titanium bases CAD/CAM, crown and bridge</p>		
 <p>CONELOG® CAM blank, type IAC and ME</p>		

* with the torque wrench J5320.1030

** optional for temporary abutments titanium: torque after completed healing phase 20 Ncm

All screws must be retightened with the corresponding torque after at least 5 minutes!

	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	3.3	3.8	4.3	5.0
Article	Instrument				Tightening torque			
 Bar abutments, straight					20 Ncm*	30 Ncm*		
 Bar abutments, 17° and 30° angled	    				20 Ncm*			
 Scanning cap for bar abutment					hand-tight			
 Titanium caps for bar abutment, crown/bridge					15 Ncm*			
 Crown base for bar abutment, burn-out								
 Bar bases for bar abutment, burn-out, cast-on, solderable, laser-weldable								
 Titanium bonding base for bar abutment, Passive-Fit								
 Locator R-Tx® Abutments								
 Healing cap for bar abutment	hand-tight							
 Impression cap for bar abutment, closed tray (bridge/bar)								
 Ball abutments					20 Ncm*	30 Ncm*		
 Locator® Abutments					20 Ncm*			
 Locator® Fixture for bar abutment								
 Scanbodies	 				hand-tight			
 ScanPost for Sirona® Scanbody								

* with torque wrench J5320.1030

All screws must be retightened with the corresponding torque after at least 5 minutes!

Materials

Titanium Grade 4		
Properties (ASTM F67 and DIN EN ISO 5832-2)		
Chemical structure (in %)	O	≤ 0.4
	Fe	≤ 0.5
	C	≤ 0.08
	N	≤ 0.05
	H	≤ 0.0125
	Ti	Rest
Mechanical properties	Tensile strength	≥ 550 MPa
	Elongation at break	≥ 12 %

Titanium alloy Ti-6Al-4V ELI		
Properties (ASTM F136)		
Chemical structure (in %)	Al	5.5–6.5
	V	3.5–4.5
	Fe	≤ 0.25
	C	≤ 0.08
	N	≤ 0.05
	O	≤ 0.13
	H	≤ 0.012
	Ti	Rest
Mechanical properties	Tensile strength	≥ 860 MPa
	Elongation at break	≥ 10 %

Cast-on gold alloy CONELOG® Gold-plastic abutment		
Properties		
Chemical structure (in %)	Au	60
	Pd	20
	Pt	19
	Ir	1
Physical properties	Melting range	1400–1490 °C
	Density	17.5 g/cm ³
	Modulus of elasticity	136 GPa
	Coefficient of thermal expansion (25–500 °C)	11.9 µm/m × °C
	Coefficient of thermal expansion (25–600 °C)	12.2 µm/m × °C
	Color	white
Mechanical properties	Status	cold-formed
	Hardness HV5	> 215
	Tensile strength (Rm)	> 750 MPa
	0.2 % Elongation limit (Rp 0.2 %)	> 650 MPa
	Elongation at break	> 2 %

Cast-on gold alloy bar base for bar abutment		
Properties		
Chemical structure (in %)	Au	60
	Pt	19
	Pd	20
	Ir	1
Physical properties	Density	17.5 g/cm ³
	Color	white
	Liquidus	1490 °C
	Solidus	1400 °C
	Coefficient of thermal expansion (25–500 °C)	12.5 µm/m × °C
	Coefficient of thermal expansion (25–600 °C)	12.6 µm/m × °C
Mechanical properties	Modulus of elasticity	136 GPa
	Hardness HV5	210
	0.2 % Elongation limit	450–570 MPa
	Elongation at break	min. 10 %
	Tensile strength MPa	530–650

Solderable gold alloy bar base for bar abutment		
Properties		
Chemical structure (in %)	Au	68.60
	Pt	2.45
	Ag	11.85
	Pd	3.95
	Cu	10.60
	Zn	2.50
	Ir	0.05
	Rh	-
	Ru	-
	Physical properties	Color
Melting range		880–940 °C
Mechanical properties	Hardness annealed HV5	175
	hardened HV5	275
	self-hardened HV5	240

CoCr alloy		
Properties (ASTM F1537-20 and ISO 5832-12)		
Chemical structure (in wt %)	Cr	26.0–30.0
	Mo	5.0–7.0
	Fe	≤ 0.75
	Ni	≤ 0.1*
	Mn	< 1.0
	Si	< 1.0
	N	< 0.25
	C	≤ 0.14
	Co	Rest
	Physical properties	Coefficient of thermal expansion (25–500 °C)
Mechanical properties	Tensile strength	> 827 MPa
	Breaking strength	1172–1400 MPa
	Elongation at break	> 12 %
	Hardness (HRC)	38–48

* ASTM F1537-20 and ISO 5832-12: ≤ 1.0 weight-%

Index alphabetical

A		C	
Abutment collets	92	Collet for CAM blank, type IAC	71
Abutment screw for CONELOG® Titanium base CAD/CAM	69	COMFOUR® Patient brochure	98
Abutment screw with reduced head	78	Countersink	50
Abutment screw, hex	87	Crown base for bar abutment	77
Adapter, ISO shaft	53	D	
Aligning tool	76	Demonstration models, acrylic glass	97
Appointment pad	99	Dense bone drill PROGRESSIVE-LINE	25, 36
B		Depth stop for form drills PROGRESSIVE-LINE and SCREW-LINE	25, 43
Ball abutment analog	81	Depth stop SCREW-LINE for pilot drills and pre-drills	50
Ball abutment, male part	81	DIM Analog® for the CONELOG® Implant System	66
Bar abutments	75	Disconnecter	91
Bar implant analog for bar abutments	76	Drill extension, ISO shaft (not for drills with internal irrigation)	51
Bar lab analog for bar abutments	76	Drill extension, ISO shaft, for instruments with internal irrigation	47
Bar sleeve for titanium bonding base	77	Drills for placement of corrugated CT-tubes	19
Baring drill for cover screw	50	Drills PROGRESSIVE-LINE Flex	36
Base for bar abutment	77	E	
Base for bar abutment, titanium	77	Edentulous mandible	97
Biomaterial patient brochure	98	EP pilot drill set	44
Bite registration cap	66	Esthomic® Abutments	72, 73
Bite registration posts	66	Esthomic® Abutments, Inset	72
Bone profiler	50	F	
C		Form drills PROGRESSIVE-LINE	25
CAM blanks	70	Form drills SCREW-LINE	43
Cleaning cannula	55	Form drills SCREW-LINE cortical bone	43
Cleaning needle	55		
CM Dalbo®-Plus matrix	81		

G		I	
Gingiva height indicator, straight	76	Implants for practice	96
Gold-plastic abutment	74	Implants	
Guide System dense bone drill PROGRESSIVE-LINE	32	CONELOG® PROGRESSIVE-LINE Promote® plus	21
Guide System form drill for Ø 3.8 mm underpreparation PROGRESSIVE-LINE	32	CONELOG® SCREW-LINE Implant, Promote® plus	38, 39
Guide System form drill PROGRESSIVE-LINE	31	Impression cap for bar abutment, closed tray	76
Guide System form drill SCREW-LINE cortical bone	47	Impression cap for impression post, closed tray	65
Guide System gingiva punch PROGRESSIVE-LINE	31	Impression posts PS	67
Guide System gingiva punch	47	Impression posts	65
Guide System guiding sleeve PROGRESSIVE-LINE	32	Insertion aid	54
Guide System guiding sleeve	47	Insertion post, screw-mounted	96
Guide System pilot drill PROGRESSIVE-LINE	31	Insertion tool for ball abutment	88
Guide System pilot drill set	46	Insertion tool for impression posts and healing caps for bar abutments	76, 89
Guide System pre-drill PROGRESSIVE-LINE	31	Insertion tool for Locator®	89
Guide System pattern for surgery wash tray CAMLOG®/CONELOG® PROGRESSIVE-LINE	30	Insertion tool for screw implants	52
Guide System surgery set SCREW-LINE	46	Insertion tool for straight bar abutments	88, 89
Guide System surgery tray CAMLOG®/CONELOG® PROGRESSIVE-LINE	30	L	
Guide System surgery wash tray CAMLOG®/CONELOG® PROGRESSIVE-LINE	30	Lab analog	66
Guiding pin for bone profiler	50	Lab prosthetic screw for bar abutment	78
		Lab screw for CONELOG® Titanium base CAD/CAM	69
H		Lab screw with reduced head	78
Handle for CAMLOG®/CONELOG® Implant analog	92	Lab screw, hex	87
Healing cap for bar abutment	76	Lamella retention insert	81
Healing caps	62	Locator R-Tx® Abutment	82
		Locator R-Tx® Analog	82
I		Locator R-Tx® Impression cap	82
Implant analog	66	Locator R-Tx® Insertion tool for replacement males	90
Implant cover screw	62	Locator R-Tx® Processing replacement male	83

Index alphabetical

L		P	
Locator R-Tx® Replacement male	83	Paralleling pin PROGRESSIVE-LINE	25
Locator R-Tx® Retention housing	83	Paralleling pin SCREW-LINE	51
Locator R-Tx® Spacer/duplication aid	83	Patient advice sheets	98
Locator® Abutment holder sleeve	89	Patient brochures	98
Locator® Abutment	84	Patient Documentation and Implant Card	98
Locator® Analog	84	Patient flyer	100
Locator® Angle measurement guide	89	Patterns for surgery and wash tray	
Locator® Block out spacer	85	CAMLOG®/CONELOG® PROGRESSIVE-LINE	24
Locator® Impression cap	84	CAMLOG®/CONELOG® PROGRESSIVE-LINE Guide System	30
Locator® Instrument	89	CAMLOG®/CONELOG® SCREW-LINE	42
Locator® Lab kits for extended angulation	85	PickUp instrument	53
Locator® Lab kits	85	Pilot drill SCREW-LINE	49
Locator® Parallel post	89	Pilot drills	49
Locator® Processing replacement male	85	Plastic screw for bar abutment	79
Locator® Replacement male for extended angulation	86	Point drill	49
Locator® Replacement male	86	Polishing protection for caps and bases for bar abutment	78
		Poster	99
		Pre-drill SCREW-LINE	49
		Pre-Osteotome SCREW-LINE	57, 58, 59, 60
		Presentation folder	99
		Profile drill PROGRESSIVE-LINE Flex	36
		Prosthetic screw for bar abutment	78
		Prosthetic tray Universal	90
		Prosthetic tray	90
		R	
		Removal adapter for CAMLOG® and CONELOG®	51
		Reworking reamer, base for bar abutment	92
		Round bur	49

S		T	
<hr/>		<hr/>	
Scanbodies	64	Titanium base CAD/CAM, crown	68
Scanning cap for bar abutments	76	Titanium bonding base for bar abutment	77
ScanPost for Sirona® Scanbody	64	Titanium cap for bar abutment, for bridge	77
Screw, hex	79	Titanium cap for bar abutment, for crown	77
Screwdriver activator	88	Titanium cap without retention for bar abutment, for bridge	77
Screwdriver, hex, ISO shaft	55, 91	Torque wrench	53, 88
Screwdriver, hex, manual/wrench	54, 90	Tubing for CT planning	19
SCREW-LINE EP form drill	44		
SCREW-LINE EP pre-drill	44	U	
Selection abutment kit	93	<hr/>	
Sleeve for inserting the insertion aid into the implant	54	Universal abutment	74, 87
Surgery sets		Universal holder	91
CAMLOG®/CONELOG® PROGRESSIVE-LINE	24	Universal holding key	54
CAMLOG®/CONELOG® PROGRESSIVE-LINE Flex	35		
CAMLOG®/CONELOG® SCREW-LINE	42	W	
Surgery tray		<hr/>	
CAMLOG®/CONELOG® PROGRESSIVE-LINE Guide System	30	Wrench adapter	36
Surgery wash trays			
CAMLOG®/CONELOG® PROGRESSIVE-LINE	24	X	
CAMLOG®/CONELOG® PROGRESSIVE-LINE Guide System	30	<hr/>	
CAMLOG®/CONELOG® SCREW-LINE	42	X-Ray Planning foils	18
		X-Ray Transfer pictures 1.25:1, CONELOG® SCREW-LINE implants	18
T			
<hr/>			
Tap adapter	51		
Tap PROGRESSIVE-LINE	25, 36		
Tap SCREW-LINE	43		
Telescope abutment for the double crown technique	87		
Temporary abutment, bridge, titanium alloy	67		
Temporary abutment, crown, titanium alloy	67		
Titanium base CAD/CAM, bridge	68		

Index Article Number

05003503	CM Dalbo®-Plus matrix	81			
05003504	Lamella retention insert	81	C1065.3309	Ø 3.3 mm, L 9 mm	39
07000389	Screwdriver activator	88	C1065.3311	Ø 3.3 mm, L 11 mm	39
08394	Locator® Abutment holder sleeve	89	C1065.3313	Ø 3.3 mm, L 13 mm	39
			C1065.3316	Ø 3.3 mm, L 16 mm	39
			C1065.3807	Ø 3.8 mm, L 7 mm	39
			C1065.3809	Ø 3.8 mm, L 9 mm	39
			C1065.3811	Ø 3.8 mm, L 11 mm	39
30001-01	Locator R-Tx® Replacement male Ø 3.3/3.8/4.3/5.0 mm, gray, NO RET.	83	C1065.3813	Ø 3.8 mm, L 13 mm	39
30002-01	Ø 3.3/3.8/4.3/5.0 mm, blue, LOW	83	C1065.3816	Ø 3.8 mm, L 16 mm	39
30003-01	Ø 3.3/3.8/4.3/5.0 mm, pink, MEDIUM	83	C1065.4307	Ø 4.3 mm, L 7 mm	39
30004-01	Ø 3.3/3.8/4.3/5.0 mm, white, HIGH	83	C1065.4309	Ø 4.3 mm, L 9 mm	39
			C1065.4311	Ø 4.3 mm, L 11 mm	39
30012-01	Locator R-Tx® Processing replacement male	83	C1065.4313	Ø 4.3 mm, L 13 mm	39
			C1065.4316	Ø 4.3 mm, L 16 mm	39
			C1065.5007	Ø 5.0 mm, L 7 mm	39
30013-01	Locator R-Tx® Retention housing	83	C1065.5009	Ø 5.0 mm, L 9 mm	39
			C1065.5011	Ø 5.0 mm, L 11 mm	39
			C1065.5013	Ø 5.0 mm, L 13 mm	39
30014-01	Locator R-Tx® Analog Ø 3.3/3.8/4.3 mm	82			
30016-01	Ø 5.0 mm	82			
30017-01	Locator R-Tx® Impression cap	82	C1066.3309	Ø 3.3 mm, L 9 mm	38
			C1066.3311	Ø 3.3 mm, L 11 mm	38
30018-01	Locator R-Tx® Spacer/duplication aid	83	C1066.3313	Ø 3.3 mm, L 13 mm	38
			C1066.3316	Ø 3.3 mm, L 16 mm	38
30021-01	Locator R-Tx® Insertion tool for replacement males	90	C1066.3807	Ø 3.8 mm, L 7 mm	38
			C1066.3809	Ø 3.8 mm, L 9 mm	38
			C1066.3811	Ø 3.8 mm, L 11 mm	38
			C1066.3813	Ø 3.8 mm, L 13 mm	38
			C1066.3816	Ø 3.8 mm, L 16 mm	38
30805-01	Locator R-Tx® Abutment Ø 3.3 mm, GH 1.0 mm	82	C1066.4307	Ø 4.3 mm, L 7 mm	38
30805-02	Ø 3.3 mm, GH 2.0 mm	82	C1066.4309	Ø 4.3 mm, L 9 mm	38
30805-03	Ø 3.3 mm, GH 3.0 mm	82	C1066.4311	Ø 4.3 mm, L 11 mm	38
30805-04	Ø 3.3 mm, GH 4.0 mm	82	C1066.4313	Ø 4.3 mm, L 13 mm	38
30806-01	Ø 3.8 mm, GH 1.0 mm	82	C1066.4316	Ø 4.3 mm, L 16 mm	38
30806-02	Ø 3.8 mm, GH 2.0 mm	82	C1066.5007	Ø 5.0 mm, L 7 mm	38
30806-03	Ø 3.8 mm, GH 3.0 mm	82	C1066.5009	Ø 5.0 mm, L 9 mm	38
30806-04	Ø 3.8 mm, GH 4.0 mm	82	C1066.5011	Ø 5.0 mm, L 11 mm	38
30806-05	Ø 3.8 mm, GH 5.0 mm	82	C1066.5013	Ø 5.0 mm, L 13 mm	38
30807-01	Ø 4.3 mm, GH 1.0 mm	82	C1066.5016	Ø 5.0 mm, L 16 mm	38
30807-02	Ø 4.3 mm, GH 2.0 mm	82			
30807-03	Ø 4.3 mm, GH 3.0 mm	82			
30807-04	Ø 4.3 mm, GH 4.0 mm	82			
30807-05	Ø 4.3 mm, GH 5.0 mm	82	C1069.3813	Ø 3.8 mm, L 13 mm	96
30808-01	Ø 5.0 mm, GH 1.0 mm	82	C1069.4313	Ø 4.3 mm, L 13 mm	96
30808-02	Ø 5.0 mm, GH 2.0 mm	82			
30808-03	Ø 5.0 mm, GH 3.0 mm	82			
30808-04	Ø 5.0 mm, GH 4.0 mm	82			
30808-05	Ø 5.0 mm, GH 5.0 mm	82			
A2002.2000	Tubing for CT planning	19			
	Drill for placement of corrugated CT-tubes				
A2050.2600	Ø 2.6 mm	19			
A2050.2800	Ø 2.8 mm	19			
A2222.2200	Tubing for CT planning	19			

	PROGRESSIVE-LINE Implant, Promote® plus incl. screw-mounted insertion post			
C1085.3309	Ø 3.3 mm, L 9 mm	21		
C1085.3311	Ø 3.3 mm, L 11 mm	21		
C1085.3313	Ø 3.3 mm, L 13 mm	21		
C1085.3316	Ø 3.3 mm, L 16 mm	21		
C1085.3807	Ø 3.8 mm, L 7 mm	21		
C1085.3809	Ø 3.8 mm, L 9 mm	21		
C1085.3811	Ø 3.8 mm, L 11 mm	21		
C1085.3813	Ø 3.8 mm, L 13 mm	21		
C1085.3816	Ø 3.8 mm, L 16 mm	21		
C1085.4307	Ø 4.3 mm, L 7 mm	21		
C1085.4309	Ø 4.3 mm, L 9 mm	21		
C1085.4311	Ø 4.3 mm, L 11 mm	21		
C1085.4313	Ø 4.3 mm, L 13 mm	21		
C1085.4316	Ø 4.3 mm, L 16 mm	21		
C1085.5007	Ø 5.0 mm, L 7 mm	21		
C1085.5009	Ø 5.0 mm, L 9 mm	21		
C1085.5011	Ø 5.0 mm, L 11 mm	21		
C1085.5013	Ø 5.0 mm, L 13 mm	21		
C1085.5016	Ø 5.0 mm, L 16 mm	21		
	PROGRESSIVE-LINE Implant, Promote® plus incl. snap-in insertion post			
C1086.3309	Ø 3.3 mm, L 9 mm	21		
C1086.3311	Ø 3.3 mm, L 11 mm	21		
C1086.3313	Ø 3.3 mm, L 13 mm	21		
C1086.3316	Ø 3.3 mm, L 16 mm	21		
C1086.3807	Ø 3.8 mm, L 7 mm	21		
C1086.3809	Ø 3.8 mm, L 9 mm	21		
C1086.3811	Ø 3.8 mm, L 11 mm	21		
C1086.3813	Ø 3.8 mm, L 13 mm	21		
C1086.3816	Ø 3.8 mm, L 16 mm	21		
C1086.4307	Ø 4.3 mm, L 7 mm	21		
C1086.4309	Ø 4.3 mm, L 9 mm	21		
C1086.4311	Ø 4.3 mm, L 11 mm	21		
C1086.4313	Ø 4.3 mm, L 13 mm	21		
C1086.4316	Ø 4.3 mm, L 16 mm	21		
C1086.5007	Ø 5.0 mm, L 7 mm	21		
C1086.5009	Ø 5.0 mm, L 9 mm	21		
C1086.5011	Ø 5.0 mm, L 11 mm	21		
C1086.5013	Ø 5.0 mm, L 13 mm	21		
C1086.5016	Ø 5.0 mm, L 16 mm	21		
	PROGRESSIVE-LINE Implant for practice			
C1901.3813	Ø 3.8 mm, L 13 mm	96		
C1901.4313	Ø 4.3 mm, L 13 mm	96		
	Healing cap, bottleneck			
C2011.3340	Ø 3.3 mm, GH 4.0 mm	62		
C2011.3840	Ø 3.8 mm, GH 4.0 mm	62		
C2011.3860	Ø 3.8 mm, GH 6.0 mm	62		
C2011.4340	Ø 4.3 mm, GH 4.0 mm	62		
C2011.4360	Ø 4.3 mm, GH 6.0 mm	62		
C2011.5040	Ø 5.0 mm, GH 4.0 mm	62		
C2011.5060	Ø 5.0 mm, GH 6.0 mm	62		
	Healing cap, wide body			
C2014.3340	Ø 3.3 mm, GH 4.0 mm	62		
C2014.3840	Ø 3.8 mm, GH 4.0 mm	62		
C2014.3860	Ø 3.8 mm, GH 6.0 mm	62		
C2014.4340	Ø 4.3 mm, GH 4.0 mm	62		
C2014.4360	Ø 4.3 mm, GH 6.0 mm	62		
C2014.5040	Ø 5.0 mm, GH 4.0 mm	62		
C2014.5060	Ø 5.0 mm, GH 6.0 mm	62		
	Healing cap, cylindrical			
C2015.3320	Ø 3.3 mm, GH 2.0 mm	62		
C2015.3340	Ø 3.3 mm, GH 4.0 mm	62		
C2015.3820	Ø 3.8 mm, GH 2.0 mm	62		
C2015.3840	Ø 3.8 mm, GH 4.0 mm	62		
C2015.3860	Ø 3.8 mm, GH 6.0 mm	62		
C2015.4320	Ø 4.3 mm, GH 2.0 mm	62		
C2015.4340	Ø 4.3 mm, GH 4.0 mm	62		
C2015.4360	Ø 4.3 mm, GH 6.0 mm	62		
C2015.5020	Ø 5.0 mm, GH 2.0 mm	62		
C2015.5040	Ø 5.0 mm, GH 4.0 mm	62		
C2015.5060	Ø 5.0 mm, GH 6.0 mm	62		
	Implant cover screw			
C2019.3300	Ø 3.3 mm	62		
C2019.3800	Ø 3.8 mm	62		
C2019.4300	Ø 4.3 mm	62		
C2019.5000	Ø 5.0 mm	62		
	Insertion post, screw-mounted			
C2026.3303	Ø 3.3 mm	96		
C2026.3803	Ø 3.8 mm	96		
C2026.4303	Ø 4.3 mm	96		
C2026.5003	Ø 5.0 mm	96		
	Impression posts, closed tray			
C2110.3300	Ø 3.3 mm	65		
C2110.3800	Ø 3.8 mm	65		
C2110.4300	Ø 4.3 mm	65		
C2110.5000	Ø 5.0 mm	65		
	Impression posts, open tray			
C2121.3300	Ø 3.3 mm	65		
C2121.3800	Ø 3.8 mm	65		
C2121.4300	Ø 4.3 mm	65		
C2121.5000	Ø 5.0 mm	65		
	Bite registration posts			
C2140.3300	Ø 3.3 mm	66		
C2140.3800	Ø 3.8 mm	66		
C2140.4300	Ø 4.3 mm	66		
C2140.5000	Ø 5.0 mm	66		
	Universal abutment			
C2211.3300	Ø 3.3 mm	74		
C2211.3800	Ø 3.8 mm	74, 87		
C2211.4300	Ø 4.3 mm	74, 87		
C2211.5000	Ø 5.0 mm	74, 87		

Index Article Number

	Telescope abutment for the double crown technique				
C2212.3800	Ø 3.8 mm	87			
C2212.4300	Ø 4.3 mm	87			
C2212.5000	Ø 5.0 mm	87			
	Esthomic® Abutments, straight				
C2226.3815	Ø 3.8 mm, GH 1.5–2.5 mm	72			
C2226.3830	Ø 3.8 mm, GH 3.0–4.5 mm	72			
C2226.4315	Ø 4.3 mm, GH 1.5–2.5 mm	72			
C2226.4330	Ø 4.3 mm, GH 3.0–4.5 mm	72			
C2226.5015	Ø 5.0 mm, GH 1.5–2.5 mm	72			
C2226.5030	Ø 5.0 mm, GH 3.0–4.5 mm	72			
	Esthomic® Abutments, 15° angled				
C2227.3815	Ø 3.8 mm, GH 1.5–2.5 mm, type A	73			
C2227.3830	Ø 3.8 mm, GH 3.0–4.5 mm, type A	73			
C2227.4315	Ø 4.3 mm, GH 1.5–2.5 mm, type A	73			
C2227.4330	Ø 4.3 mm, GH 3.0–4.5 mm, type A	73			
C2227.5015	Ø 5.0 mm, GH 1.5–2.5 mm, type A	73			
C2227.5030	Ø 5.0 mm, GH 3.0–4.5 mm, type A	73			
C2228.3815	Ø 3.8 mm, GH 1.5–2.5 mm, type B	73			
C2228.3830	Ø 3.8 mm, GH 3.0–4.5 mm, type B	73			
C2228.4315	Ø 4.3 mm, GH 1.5–2.5 mm, type B	73			
C2228.4330	Ø 4.3 mm, GH 3.0–4.5 mm, type B	73			
C2228.5015	Ø 5.0 mm, GH 1.5–2.5 mm, type B	73			
C2228.5030	Ø 5.0 mm, GH 3.0–4.5 mm, type B	73			
	Esthomic® Abutments, 20° angled				
C2231.3815	Ø 3.8 mm, GH 1.5–2.5 mm, type A	73			
C2231.3830	Ø 3.8 mm, GH 3.0–4.5 mm, type A	73			
C2231.4315	Ø 4.3 mm, GH 1.5–2.5 mm, type A	73			
C2231.4330	Ø 4.3 mm, GH 3.0–4.5 mm, type A	73			
C2231.5015	Ø 5.0 mm, GH 1.5–2.5 mm, type A	73			
C2231.5030	Ø 5.0 mm, GH 3.0–4.5 mm, type A	73			
C2232.3815	Ø 3.8 mm, GH 1.5–2.5 mm, type B	73			
C2232.3830	Ø 3.8 mm, GH 3.0–4.5 mm, type B	73			
C2232.4315	Ø 4.3 mm, GH 1.5–2.5 mm, type B	73			
C2232.4330	Ø 4.3 mm, GH 3.0–4.5 mm, type B	73			
C2232.5015	Ø 5.0 mm, GH 1.5–2.5 mm, type B	73			
C2232.5030	Ø 5.0 mm, GH 3.0–4.5 mm, type B	73			
	Esthomic® Abutments, Inset				
C2235.3320	Ø 3.3 mm, GH 2.0–3.3 mm	72			
C2235.3820	Ø 3.8 mm, GH 2.0–3.3 mm	72			
C2235.4320	Ø 4.3 mm, GH 2.0–3.3 mm	72			
C2235.5020	Ø 5.0 mm, GH 2.0–3.3 mm	72			
	Temporary abutment, crown, titanium alloy				
C2239.3300	Ø 3.3 mm	67			
C2239.3800	Ø 3.8 mm	67			
C2239.4300	Ø 4.3 mm	67			
C2239.5000	Ø 5.0 mm	67			
	Modeling aid for CONELOG® Titanium base CAD/CAM, crown				
C2242.3302	Ø 3.3 mm	69			
C2242.3802	Ø 3.8 mm	69			
C2242.4302	Ø 4.3 mm	69			
C2242.5002	Ø 5.0 mm	69			
	Titanium base CAD/CAM, crown				
C2242.3308	Ø 3.3 mm, GH 0.8 mm	68			
C2242.3320	Ø 3.3 mm, GH 2.0 mm	68			
C2242.3808	Ø 3.8 mm, GH 0.8 mm	68			
C2242.3820	Ø 3.8 mm, GH 2.0 mm	68			
C2242.4308	Ø 4.3 mm, GH 0.8 mm	68			
C2242.4320	Ø 4.3 mm, GH 2.0 mm	68			
C2242.5008	Ø 5.0 mm, GH 0.8 mm	68			
C2242.5020	Ø 5.0 mm, GH 2.0 mm	68			
	Gold-plastic abutment				
C2246.3300	Ø 3.3 mm	74			
C2246.3800	Ø 3.8 mm	74			
C2246.4300	Ø 4.3 mm	74			
C2246.5000	Ø 5.0 mm	74			
	Ball abutment, male part				
C2249.3315	Ø 3.3 mm, GH 1.5 mm	81			
C2249.3330	Ø 3.3 mm, GH 3.0 mm	81			
C2249.3815	Ø 3.8 mm, GH 1.5 mm	81			
C2249.3830	Ø 3.8 mm, GH 3.0 mm	81			
C2249.3845	Ø 3.8 mm, GH 4.5 mm	81			
C2249.4315	Ø 4.3 mm, GH 1.5 mm	81			
C2249.4330	Ø 4.3 mm, GH 3.0 mm	81			
C2249.4345	Ø 4.3 mm, GH 4.5 mm	81			
C2249.5015	Ø 5.0 mm, GH 1.5 mm	81			
C2249.5030	Ø 5.0 mm, GH 3.0 mm	81			
C2249.5045	Ø 5.0 mm, GH 4.5 mm	81			
	Locator® Abutment				
C2253.3310	Ø 3.3 mm, GH 1.0 mm	84			
C2253.3320	Ø 3.3 mm, GH 2.0 mm	84			
C2253.3330	Ø 3.3 mm, GH 3.0 mm	84			
C2253.3340	Ø 3.3 mm, GH 4.0 mm	84			
C2253.3810	Ø 3.8 mm, GH 1.0 mm	84			
C2253.3820	Ø 3.8 mm, GH 2.0 mm	84			
C2253.3830	Ø 3.8 mm, GH 3.0 mm	84			
C2253.3840	Ø 3.8 mm, GH 4.0 mm	84			
C2253.3850	Ø 3.8 mm, GH 5.0 mm	84			
C2253.4310	Ø 4.3 mm, GH 1.0 mm	84			
C2253.4320	Ø 4.3 mm, GH 2.0 mm	84			
C2253.4330	Ø 4.3 mm, GH 3.0 mm	84			
C2253.4340	Ø 4.3 mm, GH 4.0 mm	84			
C2253.4350	Ø 4.3 mm, GH 5.0 mm	84			
C2253.5010	Ø 5.0 mm, GH 1.0 mm	84			
C2253.5020	Ø 5.0 mm, GH 2.0 mm	84			
C2253.5030	Ø 5.0 mm, GH 3.0 mm	84			
C2253.5040	Ø 5.0 mm, GH 4.0 mm	84			
C2253.5050	Ø 5.0 mm, GH 5.0 mm	84			

	Bar abutments, straight				Titanium base CAD/CAM, bridge	
C2254.3310	Ø 3.3 mm, GH 1.0 mm	75		C2342.3308	Ø 3.3 mm, GH 0.8 mm	68
C2254.3325	Ø 3.3 mm, GH 2.5 mm	75		C2342.3320	Ø 3.3 mm, GH 2.0 mm	68
C2254.3810	Ø 3.8 mm, GH 1.0 mm	75		C2342.3808	Ø 3.8 mm, GH 0.8 mm	68
C2254.3825	Ø 3.8 mm, GH 2.5 mm	75		C2342.3820	Ø 3.8 mm, GH 2.0 mm	68
C2254.3840	Ø 3.8 mm, GH 4.0 mm	75		C2342.4308	Ø 4.3 mm, GH 0.8 mm	68
C2254.4310	Ø 4.3 mm, GH 1.0 mm	75		C2342.4320	Ø 4.3 mm, GH 2.0 mm	68
C2254.4325	Ø 4.3 mm, GH 2.5 mm	75		C2342.5008	Ø 5.0 mm, GH 0.8 mm	68
C2254.4340	Ø 4.3 mm, GH 4.0 mm	75		C2342.5020	Ø 5.0 mm, GH 2.0 mm	68
C2254.5010	Ø 5.0 mm, GH 1.0 mm	75			CAM titanium blank, type IAC	
C2254.5025	Ø 5.0 mm, GH 2.5 mm	75		C2431.3313	Ø 3.3 mm	70
C2254.5040	Ø 5.0 mm, GH 4.0 mm	75		C2431.3813	Ø 3.8 mm	70
	Bar abutments, 17° angled			C2431.4313	Ø 4.3 mm	70
C2256.3325	Ø 3.3 mm, GH 2.5, type A	75		C2431.5013	Ø 5.0 mm	70
C2256.3340	Ø 3.3 mm, GH 4.0, type A	75			CAM titanium blank, type ME	
C2256.3825	Ø 3.8 mm, GH 2.5, type A	75		C2441.3320	Ø 3.3 mm	70
C2256.3840	Ø 3.8 mm, GH 4.0, type A	75		C2441.3820	Ø 3.8 mm	70
C2256.4325	Ø 4.3 mm, GH 2.5, type A	75		C2441.4320	Ø 4.3 mm	70
C2256.4340	Ø 4.3 mm, GH 4.0, type A	75		C2441.5020	Ø 5.0 mm	70
C2256.5025	Ø 5.0 mm, GH 2.5, type A	75			CAM CoCr blank, type ME	
C2256.5040	Ø 5.0 mm, GH 4.0, type A	75		C2461.3320	Ø 3.3 mm	70
C2257.3325	Ø 3.3 mm, GH 2.5, type B	75		C2461.4320	Ø 3.8/4.3 mm	70
C2257.3340	Ø 3.3 mm, GH 4.0, type B	75		C2461.5020	Ø 5.0 mm	70
C2257.3825	Ø 3.8 mm, GH 2.5, type B	75			Scanbodies	
C2257.3840	Ø 3.8 mm, GH 4.0, type B	75		C2600.3310	Ø 3.3 mm	64
C2257.4325	Ø 4.3 mm, GH 2.5, type B	75		C2600.4310	Ø 3.8/4.3 mm	64
C2257.4340	Ø 4.3 mm, GH 4.0, type B	75		C2600.5010	Ø 5.0 mm	64
C2257.5025	Ø 5.0 mm, GH 2.5, type B	75			ScanPost for Sirona® Scanbody	
C2257.5040	Ø 5.0 mm, GH 4.0, type B	75		C2620.3306	Ø 3.3 mm	64
	Bar abutments, 30° angled			C2620.3806	Ø 3.8 mm	64
C2258.3325	Ø 3.3 mm, GH 2.5, type A	75		C2620.4306	Ø 4.3 mm	64
C2258.3340	Ø 3.3 mm, GH 4.0, type A	75		C2620.5006	Ø 5.0 mm	64
C2258.3825	Ø 3.8 mm, GH 2.5, type A	75			Lab analog	
C2258.3840	Ø 3.8 mm, GH 4.0, type A	75		C3010.3300	Ø 3.3 mm	66
C2258.4325	Ø 4.3 mm, GH 2.5, type A	75		C3010.3303	Ø 3.3 mm (3 units)	66
C2258.4340	Ø 4.3 mm, GH 4.0, type A	75		C3010.3800	Ø 3.8 mm	66
C2258.5035	Ø 5.0 mm, GH 3.5, type A	75		C3010.3803	Ø 3.8 mm (3 units)	66
C2258.5050	Ø 5.0 mm, GH 5.0, type A	75		C3010.4300	Ø 4.3 mm	66
C2259.3325	Ø 3.3 mm, GH 2.5, type B	75		C3010.4303	Ø 4.3 mm (3 units)	66
C2259.3340	Ø 3.3 mm, GH 4.0, type B	75		C3010.5000	Ø 5.0 mm	66
C2259.3825	Ø 3.8 mm, GH 2.5, type B	75		C3010.5003	Ø 5.0 mm (3 units)	66
C2259.3840	Ø 3.8 mm, GH 4.0, type B	75			DIM Analog® for the CONELOG® Implant System	
C2259.4325	Ø 4.3 mm, GH 2.5, type B	75		C3012.3300	Ø 3.3 mm	66
C2259.4340	Ø 4.3 mm, GH 4.0, type B	75		C3012.3800	Ø 3.8 mm	66
C2259.5035	Ø 5.0 mm, GH 3.5, type B	75		C3012.4300	Ø 4.3 mm	66
C2259.5050	Ø 5.0 mm, GH 5.0, type B	75		C3012.5000	Ø 5.0 mm	66
	Temporary abutment, bridge, titanium alloy					
C2339.3300	Ø 3.3 mm	67				
C2339.3800	Ø 3.8 mm	67				
C2339.4300	Ø 4.3 mm	67				
C2339.5000	Ø 5.0 mm	67				

Index Article Number

	Ball abutment analog				
C3015.3300	Ø 3.3/3.8/4.3 mm	81	C5002.3300	Ø 3.3 mm	50
C3015.5000	Ø 5.0 mm	81	C5002.3800	Ø 3.8 mm	50
	Implant analog		C5002.4300	Ø 4.3 mm	50
C3025.3300	Ø 3.3 mm	66	C5002.5000	Ø 5.0 mm	50
C3025.3303	Ø 3.3 mm (3 units)	66			
C3025.3800	Ø 3.8 mm	66	Disconnecter, for CONELOG® Abutments		
C3025.3803	Ø 3.8 mm (3 units)	66	C5300.1601	Ø 3.3/3.8/4.3 mm, M1.6, short	91
C3025.4300	Ø 4.3 mm	66	C5300.1603	Ø 3.3/3.8/4.3 mm, M1.6, long	91
C3025.4303	Ø 4.3 mm (3 units)	66	C5300.2001	Ø 5.0 mm, M2.0, short	91
C3025.5000	Ø 5.0 mm	66	C5300.2003	Ø 5.0 mm, M2.0, long	91
C3025.5003	Ø 5.0 mm (3 units)	66			
	Universal holder, incl. lab screws and abutment collet	92	C5300.9010	X-Ray Planning foil 1.25:1	18
			C5300.9011	X-Ray Planning foil 1.4:1	18
	Abutment collets				
C3709.3300	Ø 3.3 mm	92	X-Ray Planning foil		
C3709.3800	Ø 3.8 mm	92	CONELOG® PROGRESSIVE-LINE Implants		
C3709.4300	Ø 4.3 mm	92	C5300.9014	X-Ray Planning foil 1.25:1	18
C3709.5000	Ø 5.0 mm	92	C5300.9015	X-Ray Planning foil 1.4:1	18
	Collet for CAM blank, type IAC				
C3720.3300	Ø 3.3 mm	71	C5300.9080	Ø 3.3 mm	18
C3720.4300	Ø 3.8/4.3 mm	71	C5300.9081	Ø 3.8 mm	18
C3720.5000	Ø 5.0 mm	71	C5300.9082	Ø 4.3 mm	18
	Lab screw, with reduced head		C5300.9083	Ø 5.0 mm	18
C4004.1600	Ø 3.3/3.8/4.3 mm, M1.6	78			
C4004.2000	Ø 5.0 mm, M2.0	78	Insertion aid		
	Abutment screw, with reduced head		C5302.3310	Ø 3.3 mm, long	54
C4004.1601	Ø 3.3/3.8/4.3 mm, M1.6	78	C5302.3311	Ø 3.3 mm, short	54
C4004.2001	Ø 5.0 mm, M2.0	78	C5302.4310	Ø 3.8/4.3 mm, long	54
	Abutment screw, hex		C5302.4311	Ø 3.8/4.3 mm, short	54
C4005.1601	Ø 3.3/3.8/4.3 mm, M1.6	87	C5302.5011	Ø 5.0 mm, short	54
C4005.2001	Ø 5.0 mm, M2.0	87			
	Lab screw, hex		Macro model		
C4006.1601	Ø 3.3/3.8/4.3 mm, M1.6	87	C8010.1010	SCREW-LINE	97
C4006.1603	Ø 3.3/3.8/4.3 mm, M1.6 (3 units)	87	C8010.1400	PROGRESSIVE-LINE	97
C4006.2001	Ø 5.0 mm, M2.0	87			
C4006.2003	Ø 5.0 mm, M2.0 (3 units)	87	C8011.1000	Selection abutment kit	93
	Abutment screw for CONELOG® Titanium base CAD/CAM				
C4015.1601	Ø 3.3/3.8/4.3 mm, M1.6	69	J2029.4300	Demonstration model, acrylic glass	
C4015.2001	Ø 5.0 mm, M2.0	69	J2029.6000	Lower jaw	97
	Lab screw for CONELOG® Titanium base CAD/CAM		C8070.1020	Upper jaw	97
C4016.1601	Ø 3.3/3.8/4.3 mm, M1.6	69			
C4016.2001	Ø 5.0 mm, M2.0	69	Healing cap for bar abutment		
			J2111.3300	Ø 3.3/3.8/4.3 mm	76
			J2111.3800	Ø 5.0 mm	76
			J2111.4300		
			J2111.5000	Impression cap for impression post, closed tray	
				Ø 3.3 mm	65
				Ø 3.8 mm	65
				Ø 4.3 mm	65
				Ø 5.0 mm	65

	Bite registration cap				Titanium cap for bar abutment	
J2112.3300	Ø 3.3 mm	66		J2259.4301	Ø 3.3/3.8/4.3 mm, for crown	77
J2112.3800	Ø 3.8 mm	66		J2259.4302	Ø 3.3/3.8/4.3 mm, for bridge	77
J2112.4300	Ø 4.3 mm	66		J2259.6001	Ø 5.0 mm, for crown	77
J2112.5000	Ø 5.0 mm	66		J2259.6002	Ø 5.0 mm, for bridge	77
	Impression cap for bar abutment, closed tray (bridge/bar)				Titanium cap without retention for bar abutment, for bridge	
J2129.4300	Ø 3.3/3.8/4.3 mm, short	76		J2259.4322	Ø 3.3/3.8/4.3 mm	77
J2129.4310	Ø 3.3/3.8/4.3 mm, long	76		J2259.6022	Ø 5.0 mm	77
J2129.6000	Ø 5.0 mm, short	76			Titanium bonding base for bar abutment	
J2129.6010	Ø 5.0 mm, long	76		J2260.4301	Ø 3.3/3.8/4.3 mm	77
J2253.0001	Insertion tool for Locator®	89		J2260.6001	Ø 5.0 mm	77
J2253.0002	Locator® Instrument	89			Bar sleeve for titanium bonding base	
J2253.0003	Locator® Angle measurement guide	89		J2261.4301	Ø 3.3/3.8/4.3 mm	77
J2253.0004	Locator® Parallel post	89		J2261.6001	Ø 5.0 mm	77
J2253.0102	Locator® Lab kits	85			Base for bar abutment, titanium, laser-weldable	
J2253.0112	Locator® Lab kits for extended angulation	85		J2262.4300	Ø 3.3/3.8/4.3 mm	77
J2253.0200	Locator® Impression cap	84		J2262.6000	Ø 5.0 mm	77
J2253.0340	Locator® Analog	84			Base for bar abutment, cast-on	
J2253.0401	Locator® Block out spacer	85		J2263.4300	Ø 3.3/3.8/4.3 mm	77
J2253.0402	Locator® Processing replacement male	85		J2263.6000	Ø 5.0 mm	77
	Locator® Replacement male				Aligning tool	
J2253.1002	Ø 3.3/3.8/4.3/5.0 mm, blue, LOW	86		J2269.0005	17°	76
J2253.1003	Ø 3.3/3.8/4.3/5.0 mm, pink, MEDIUM	86		J2269.0006	30°	76
J2253.1005	Ø 3.3/3.8/4.3/5.0 mm, clear, HIGH	86			Scanning cap for bar abutments	
	Locator® Replacement male for extended angulation			J2610.4300	Ø 3.3/3.8/4.3 mm	76
J2253.2000	Ø 3.8/4.3/5.0 mm, gray, NO RETENTION	86		J2610.6000	Ø 5.0 mm	76
J2253.2002	Ø 3.8/4.3/5.0 mm, red, LOW	86			Bar lab analog for bar abutments	
J2253.2003	Ø 3.8/4.3/5.0 mm, orange, MEDIUM	86		J3020.4300	Ø 3.3/3.8/4.3 mm	76
J2253.2004	Ø 3.8/4.3/5.0 mm, green, HIGH	86		J3020.6000	Ø 5.0 mm	76
	Crown base for bar abutment				Polishing protection for caps and bases for bar abutment	
J2256.4306	Ø 3.3/3.8/4.3 mm	77		J3021.4300	Ø 3.3/3.8/4.3 mm	78
J2256.6006	Ø 5.0 mm	77		J3021.6000	Ø 5.0 mm	78
	Base for bar abutment, burn-out				Handle for CAMLOG®/CONELOG® Implant analog	
J2257.4301	Ø 3.3/3.8/4.3 mm	77		J3025.0010	Ø 3.3/3.8/4.3 mm	92
J2257.6001	Ø 5.0 mm	77		J3025.0015	Ø 5.0 mm	92
	Base for bar abutment, solderable				Bar implant analog for bar abutments	
J2258.4300	Ø 3.3/3.8/4.3 mm	77		J3025.4300	Ø 3.3/3.8/4.3 mm	76
J2258.6000	Ø 5.0 mm	77		J3025.6000	Ø 5.0 mm	76

Index Article Number

	Gingiva height indicator, straight					
J3550.3300	Ø 3.3 mm	76		J5002.0011	Adapter, ISO shaft	53
J3550.3800	Ø 3.8 mm	76		J5002.0012	Cleaning needle	55
J3550.4300	Ø 4.3 mm	76		J5002.0013	Wrench adapter	36
J3550.5000	Ø 5.0 mm	76		J5002.0020	Cleaning cannula	55
J3551.0001	Orientation gauge for COMFOUR®	76				
J3709.0015	Universal holder	92			Bone profiler	
	Reworking reamer, base for bar abutment			J5003.3350	Ø 3.3 mm, Ø 5.0 mm	50
J3711.0010	Ø 3.3/3.8/4.3 mm, plane surface/cone seat	92		J5003.4360	Ø 3.8/4.3 mm, Ø 6.0 mm	50
J3711.0015	Ø 5.0 mm, plane surface/cone seat	92		J5003.5070	Ø 5.0 mm, Ø 7.0 mm	50
J3711.0020	Ø 3.3/3.8/4.3 mm, screw seat	92			Baring drill for cover screw	
J3711.0025	Ø 5.0 mm, screw seat	92		J5004.3300	Ø 3.3 mm	50
	Guide System guiding sleeve			J5004.3800	Ø 3.8 mm	50
J3734.3303	Ø 3.3 mm	47		J5004.4300	Ø 4.3 mm	50
J3734.3803	Ø 3.8 mm	47		J5004.5000	Ø 5.0 mm	50
J3734.4303	Ø 4.3 mm	47			Countersink	
	Guide System guiding sleeve			J5006.3346	Ø 3.3 mm, Ø 4.6 mm	50
	PROGRESSIVE-LINE			J5006.3852	Ø 3.8 mm, Ø 5.2 mm	50
J3754.3301	Ø 3.3 mm	32		J5006.4356	Ø 4.3 mm, Ø 5.6 mm	50
J3754.3801	Ø 3.8 mm	32		J5006.5063	Ø 5.0 mm, Ø 6.3 mm	50
J3754.4301	Ø 4.3 mm	32			Depth stop SCREW-LINE for pilot drills and pre-drills	
J3754.5001	Ø 5.0 mm	32		J5015.0009	L 9 mm	50
	Plastic screw for bar abutment			J5015.0011	L 11 mm	50
J4009.1627	M1.6	79		J5015.0013	L 13 mm	50
J4009.2027	M2.0	79			Depth stop for form drills	
	Prosthetic screw for bar abutment				PROGRESSIVE-LINE and SCREW-LINE	
J4012.1601	Ø 3.3/3.8/4.3 mm	78		J5015.3300	Ø 3.3 mm	25, 43
J4012.2001	Ø 5.0 mm	78		J5015.3800	Ø 3.8 mm	25, 43
	Screw, hex			J5015.4300	Ø 4.3 mm	25, 43
J4012.1610	L 10 mm, M1.6	79		J5015.5000	Ø 5.0 mm	25, 43
J4012.1615	L 15 mm, M1.6	79			Guide System gingiva punch	
J4012.1620	L 20 mm, M1.6	79		J5041.3303	Ø 3.3 mm	47
J4012.2010	L 10 mm, M2.0	79		J5041.3304	Ø 3.3 mm, PROGRESSIVE-LINE	31
J4012.2015	L 15 mm, M2.0	79		J5041.3803	Ø 3.8 mm	47
J4012.2020	L 20 mm, M2.0	79		J5041.3804	Ø 3.8 mm, PROGRESSIVE-LINE	31
	Lab prosthetic screw for bar abutment			J5041.4303	Ø 4.3 mm	47
J4013.1601	Ø 3.3/3.8/4.3 mm	78		J5041.4304	Ø 4.3 mm, PROGRESSIVE-LINE	31
J4013.2001	Ø 5.0 mm	78		J5041.5004	Ø 5.0 mm, PROGRESSIVE-LINE	31
	Drill extension, ISO shaft			J5050.2300	Round bur	49
J5002.0005	for instruments with internal irrigation	47		J5051.1500	Point drill	49
J5002.0006	not for drills with internal irrigation	51		J5051.2000	Pilot drill SCREW-LINE	49
				J5051.2003	Pilot drill	49
				J5051.2800	Pre-drill SCREW-LINE	49

	Form drill SCREW-LINE cortical bone				
J5053.3316	Ø 3.3 mm	43	J5063.3309	Ø 3.3 mm, L 5/9 mm	46
J5053.3816	Ø 3.8 mm	43	J5063.3311	Ø 3.3 mm, L 5/9/11 mm	46
J5053.4316	Ø 4.3 mm	43	J5063.3313	Ø 3.3 mm, L 5/9/11/13 mm	46
J5053.5016	Ø 5.0 mm	43	J5063.4307	Ø 3.8/4.3 mm, L 5/7 mm	46
	Tap SCREW-LINE		J5063.4309	Ø 3.8/4.3 mm, L 5/9 mm	46
J5054.3309	Ø 3.3 mm	43	J5063.4311	Ø 3.8/4.3 mm, L 5/9/11 mm	46
J5054.3809	Ø 3.8 mm	43	J5063.4313	Ø 3.8/4.3 mm, L 5/9/11/13 mm	46
J5054.4309	Ø 4.3 mm	43	J5064.3316	Ø 3.3 mm, L 16 mm	46
J5054.5009	Ø 5.0 mm	43	J5064.4316	Ø 3.8/4.3 mm, L 16 mm	46
J5060.0001	EP pilot drill set	44		Guide System surgery set SCREW-LINE	
J5060.2800	SCREW-LINE EP pre-drill	44	J5065.3309	Ø 3.3 mm, L 5/9 mm	46
	SCREW-LINE EP form drill		J5065.3311	Ø 3.3 mm, L 5/9/11 mm	46
J5060.3309	Ø 3.3 mm, L 9 mm	44	J5065.3313	Ø 3.3 mm, L 5/9/11/13 mm	46
J5060.3311	Ø 3.3 mm, L 11 mm	44	J5065.3807	Ø 3.8 mm, L 5/7 mm	46
J5060.3313	Ø 3.3 mm, L 13 mm	44	J5065.3809	Ø 3.8 mm, L 5/9 mm	46
J5060.3807	Ø 3.8 mm, L 7 mm	44	J5065.3811	Ø 3.8 mm, L 5/9/11 mm	46
J5060.3809	Ø 3.8 mm, L 9 mm	44	J5065.3813	Ø 3.8 mm, L 5/9/11/13 mm	46
J5060.3811	Ø 3.8 mm, L 11 mm	44	J5065.4307	Ø 4.3 mm, L 5/7 mm	46
J5060.3813	Ø 3.8 mm, L 13 mm	44	J5065.4309	Ø 4.3 mm, L 5/9 mm	46
J5060.4307	Ø 4.3 mm, L 7 mm	44	J5065.4311	Ø 4.3 mm, L 5/9/11 mm	46
J5060.4309	Ø 4.3 mm, L 9 mm	44	J5065.4313	Ø 4.3 mm, L 5/9/11/13 mm	46
J5060.4311	Ø 4.3 mm, L 11 mm	44	J5066.3316	Ø 3.3 mm, L 16 mm	46
J5060.4313	Ø 4.3 mm, L 13 mm	44	J5066.3816	Ø 3.8 mm, L 16 mm	46
J5060.5007	Ø 5.0 mm, L 7 mm	44	J5066.4316	Ø 4.3 mm, L 16 mm	46
J5060.5009	Ø 5.0 mm, L 9 mm	44		Guide System Form drill, SCREW-LINE cortical bone	
J5060.5011	Ø 5.0 mm, L 11 mm	44	J5068.3309	Ø 3.3 mm, L 9 mm	47
J5060.5013	Ø 5.0 mm, L 13 mm	44	J5068.3311	Ø 3.3 mm, L 11 mm	47
	Form drill SCREW-LINE		J5068.3313	Ø 3.3 mm, L 13 mm	47
J5062.3309	Ø 3.3 mm, L 9 mm	43	J5068.3316	Ø 3.3 mm, L 16 mm	47
J5062.3311	Ø 3.3 mm, L 11 mm	43	J5068.3807	Ø 3.8 mm, L 7 mm	47
J5062.3313	Ø 3.3 mm, L 13 mm	43	J5068.3809	Ø 3.8 mm, L 9 mm	47
J5062.3316	Ø 3.3 mm, L 16 mm	43	J5068.3811	Ø 3.8 mm, L 11 mm	47
J5062.3807	Ø 3.8 mm, L 7 mm	43	J5068.3813	Ø 3.8 mm, L 13 mm	47
J5062.3809	Ø 3.8 mm, L 9 mm	43	J5068.3816	Ø 3.8 mm, L 16 mm	47
J5062.3811	Ø 3.8 mm, L 11 mm	43	J5068.4307	Ø 4.3 mm, L 7 mm	47
J5062.3813	Ø 3.8 mm, L 13 mm	43	J5068.4309	Ø 4.3 mm, L 9 mm	47
J5062.3816	Ø 3.8 mm, L 16 mm	43	J5068.4311	Ø 4.3 mm, L 11 mm	47
J5062.4307	Ø 4.3 mm, L 7 mm	43	J5068.4313	Ø 4.3 mm, L 13 mm	47
J5062.4309	Ø 4.3 mm, L 9 mm	43	J5068.4316	Ø 4.3 mm, L 16 mm	47
J5062.4311	Ø 4.3 mm, L 11 mm	43			
J5062.4313	Ø 4.3 mm, L 13 mm	43			
J5062.4316	Ø 4.3 mm, L 16 mm	43			
J5062.5007	Ø 5.0 mm, L 7 mm	43			
J5062.5009	Ø 5.0 mm, L 9 mm	43			
J5062.5011	Ø 5.0 mm, L 11 mm	43			
J5062.5013	Ø 5.0 mm, L 13 mm	43			
J5062.5016	Ø 5.0 mm, L 16 mm	43			

Index Article Number

	Form drill PROGRESSIVE-LINE				
J5070.3309	Ø 3.3 mm, L 9 mm	25			
J5070.3311	Ø 3.3 mm, L 11 mm	25			
J5070.3313	Ø 3.3 mm, L 13 mm	25			
J5070.3316	Ø 3.3 mm, L 16 mm	25			
J5070.3807	Ø 3.8 mm, L 7 mm	25			
J5070.3809	Ø 3.8 mm, L 9 mm	25			
J5070.3811	Ø 3.8 mm, L 11 mm	25			
J5070.3813	Ø 3.8 mm, L 13 mm	25			
J5070.3816	Ø 3.8 mm, L 16 mm	25			
J5070.4307	Ø 4.3 mm, L 7 mm	25			
J5070.4309	Ø 4.3 mm, L 9 mm	25			
J5070.4311	Ø 4.3 mm, L 11 mm	25			
J5070.4313	Ø 4.3 mm, L 13 mm	25			
J5070.4316	Ø 4.3 mm, L 16 mm	25			
J5070.5007	Ø 5.0 mm, L 7 mm	25			
J5070.5009	Ø 5.0 mm, L 9 mm	25			
J5070.5011	Ø 5.0 mm, L 11 mm	25			
J5070.5013	Ø 5.0 mm, L 13 mm	25			
J5070.5016	Ø 5.0 mm, L 16 mm	25			
	Tap PROGRESSIVE-LINE				
J5071.3300	Ø 3.3 mm	25, 36			
J5071.3800	Ø 3.8 mm	25, 36			
J5071.4300	Ø 4.3 mm	25, 36			
J5071.5000	Ø 5.0 mm	25, 36			
	Dense bone drill PROGRESSIVE-LINE				
J5072.3300	Ø 3.3 mm	25, 36			
J5072.3800	Ø 3.8 mm	25, 36			
J5072.4300	Ø 4.3 mm	25, 36			
J5072.5000	Ø 5.0 mm	25, 36			
	Guide System pilot drill PROGRESSIVE-LINE				
J5074.3305	Ø 3.3 mm, L 5 mm	31			
J5074.3309	Ø 3.3 mm, L 9 mm	31			
J5074.3311	Ø 3.3 mm, L 11 mm	31			
J5074.3313	Ø 3.3 mm, L 13 mm	31			
J5074.3316	Ø 3.3 mm, L 16 mm	31			
J5074.4305	Ø 3.8/4.3 mm, L 5 mm	31			
J5074.4307	Ø 3.8/4.3 mm, L 7 mm	31			
J5074.4309	Ø 3.8/4.3 mm, L 9 mm	31			
J5074.4311	Ø 3.8/4.3 mm, L 11 mm	31			
J5074.4313	Ø 3.8/4.3 mm, L 13 mm	31			
J5074.4316	Ø 3.8/4.3 mm, L 16 mm	31			
J5074.5005	Ø 5.0 mm, L 5 mm	31			
J5074.5007	Ø 5.0 mm, L 7 mm	31			
J5074.5009	Ø 5.0 mm, L 9 mm	31			
J5074.5011	Ø 5.0 mm, L 11 mm	31			
J5074.5013	Ø 5.0 mm, L 13 mm	31			
J5074.5016	Ø 5.0 mm, L 16 mm	31			
	Guide System pre-drill PROGRESSIVE-LINE				
J5076.3305	Ø 3.3 mm, L 5 mm	31			
J5076.3805	Ø 3.8 mm, L 5 mm	31			
J5076.4305	Ø 4.3 mm, L 5 mm	31			
J5076.5005	Ø 5.0 mm, L 5 mm	31			
	Guide System form drill PROGRESSIVE-LINE				
J5076.3309	Ø 3.3 mm, L 9 mm	31			
J5076.3311	Ø 3.3 mm, L 11 mm	31			
J5076.3313	Ø 3.3 mm, L 13 mm	31			
J5076.3316	Ø 3.3 mm, L 16 mm	31			
J5076.3807	Ø 3.8 mm, L 7 mm	31			
J5076.3809	Ø 3.8 mm, L 9 mm	31			
J5076.3811	Ø 3.8 mm, L 11 mm	31			
J5076.3813	Ø 3.8 mm, L 13 mm	31			
J5076.3816	Ø 3.8 mm, L 16 mm	31			
J5076.4307	Ø 4.3 mm, L 7 mm	31			
J5076.4309	Ø 4.3 mm, L 9 mm	31			
J5076.4311	Ø 4.3 mm, L 11 mm	31			
J5076.4313	Ø 4.3 mm, L 13 mm	31			
J5076.4316	Ø 4.3 mm, L 16 mm	31			
J5076.5007	Ø 5.0 mm, L 7 mm	31			
J5076.5009	Ø 5.0 mm, L 9 mm	31			
J5076.5011	Ø 5.0 mm, L 11 mm	31			
J5076.5013	Ø 5.0 mm, L 13 mm	31			
J5076.5016	Ø 5.0 mm, L 16 mm	31			
	Guide System form drill for Ø 3.8 mm underpreparation PROGRESSIVE-LINE				
J5077.3309	Ø 3.3 mm, L 9 mm	32			
J5077.3311	Ø 3.3 mm, L 11 mm	32			
J5077.3313	Ø 3.3 mm, L 13 mm	32			
J5077.3316	Ø 3.3 mm, L 16 mm	32			
	Guide System dense bone drill PROGRESSIVE-LINE				
J5078.3309	Ø 3.3 mm, L 9 mm	32			
J5078.3311	Ø 3.3 mm, L 11 mm	32			
J5078.3313	Ø 3.3 mm, L 13 mm	32			
J5078.3316	Ø 3.3 mm, L 16 mm	32			
J5078.3807	Ø 3.8 mm, L 7 mm	32			
J5078.3809	Ø 3.8 mm, L 9 mm	32			
J5078.3811	Ø 3.8 mm, L 11 mm	32			
J5078.3813	Ø 3.8 mm, L 13 mm	32			
J5078.3816	Ø 3.8 mm, L 16 mm	32			
J5078.4307	Ø 4.3 mm, L 7 mm	32			
J5078.4309	Ø 4.3 mm, L 9 mm	32			
J5078.4311	Ø 4.3 mm, L 11 mm	32			
J5078.4313	Ø 4.3 mm, L 13 mm	32			
J5078.4316	Ø 4.3 mm, L 16 mm	32			
J5078.5007	Ø 5.0 mm, L 7 mm	32			
J5078.5009	Ø 5.0 mm, L 9 mm	32			
J5078.5011	Ø 5.0 mm, L 11 mm	32			
J5078.5013	Ø 5.0 mm, L 13 mm	32			
J5078.5016	Ø 5.0 mm, L 16 mm	32			

	Drill PROGRESSIVE-LINE Flex		J5300.8919	Guide System surgery tray CAMLOG®/CONELOG® PROGRESSIVE-LINE (without contents)	30
J5079.3300	Ø 3.3 mm	36			
J5079.3800	Ø 3.8 mm	36			
J5079.4300	Ø 4.3 mm	36			
J5079.5000	Ø 5.0 mm	36			
	Profile drill PROGRESSIVE-LINE Flex		J5300.8968	Surgery wash tray CAMLOG®/CONELOG®	
J5080.3300	Ø 3.3 mm	36	J5300.8970	SCREW-LINE	42
J5080.3800	Ø 3.8 mm	36	J5300.8971	PROGRESSIVE-LINE	24
J5080.4300	Ø 4.3 mm	36		Guide System PROGRESSIVE-LINE	30
J5080.5000	Ø 5.0 mm	36			
J5300.0011	Insertion tool for ball abutment	88	J5302.0010	Universal holding key	54
	Insertion tool for straight bar abutments		J5302.3300	Sleeve for inserting the insertion aid into the implant	
J5300.0020	Ø 3.3/3.8/4.3 mm, short	88	J5302.3800	Ø 3.3 mm	54
J5300.0021	Ø 3.3/3.8/4.3 mm, long	89	J5302.4300	Ø 3.8 mm	54
J5300.0025	Ø 5.0 mm, short	88	J5302.5000	Ø 4.3 mm	54
				Ø 5.0 mm	54
J5300.0022	Removal adapter for CAMLOG® and CONELOG®	51		Screwdriver, hex	
	Insertion tool for impression posts and healing caps for bar abutments		J5317.0501	short, manual/wrench	54, 90
J5300.0027	Ø 3.3/3.8/4.3 mm	76, 89	J5317.0502	long, manual/wrench	54, 90
J5300.0028	Ø 5.0 mm	76, 89	J5317.0503	long, ISO shaft	55, 91
			J5317.0504	short, ISO shaft	55, 91
J5300.0030	PickUp instrument	53	J5317.0510	extra short, manual/wrench	54, 90
	Insertion tool for screw implants		J5317.0511	Manual screwdriver, hex	55, 91
J5300.0031	extra short, manual/wrench	52	J5320.1030	Torque wrench	53, 88
J5300.0032	short, manual/wrench	52		Tap adapter	
J5300.0033	long, manual/wrench	52	J5322.0010	short	51
J5300.0034	short, with ISO shaft for angled hand piece	52	J5322.0011	long	51
J5300.0035	long, with ISO shaft for angled hand piece	52	J5330.8500	Prosthetic tray	90
	Insertion tool for screw implants (without hex on shaft)		J5330.8700	Prosthetic tray Universal	90
J5300.0036	short, with ISO shaft for angled hand piece	52	J5417.2800	Pre-osteotome SCREW-LINE, 1.7–2.8 mm, straight-convex	57, 58
J5300.0037	long, with ISO shaft for angled hand piece	52		Osteotomy Set CAMLOG®/CONELOG® SCREW-LINE	
	Surgery Set CAMLOG®/CONELOG®		J5418.0020	straight-convex	57
J5300.0063	SCREW-LINE	42	J5418.0030	angled-convex	58
J5300.0065	PROGRESSIVE-LINE	24		Osteotome SCREW-LINE	
J5300.0071	PROGRESSIVE-LINE Flex	35	J5418.3300	Ø 3.3 mm, straight-convex	57
	Pattern for surgery wash tray CAMLOG®/CONELOG®		J5418.3310	Ø 3.3 mm, angled-convex	58
J5300.1072	Guide System PROGRESSIVE-LINE	30	J5418.3800	Ø 3.8 mm, straight-convex	57
J5300.1073	SCREW-LINE	42	J5418.3810	Ø 3.8 mm, angled-convex	58
J5300.1074	PROGRESSIVE-LINE	24	J5418.4300	Ø 4.3 mm, straight-convex	57
	Paralleling pin		J5418.4310	Ø 4.3 mm, angled-convex	58
J5300.2000	PROGRESSIVE-LINE	25	J5418.5000	Ø 5.0 mm, straight-convex	57
J5300.2028	SCREW-LINE	51	J5418.5010	Ø 5.0 mm, angled-convex	58

Index Article Number

J5419.2800	Pre-Osteotome SCREW-LINE, 1.7-2.8 mm, straight-concave	59, 60
	Osteotomy Set	
	CAMLOG®/CONELOG® SCREW-LINE	
J5420.0020	straight-concave	59
J5420.0030	angled-concave	60
	Osteotome SCREW-LINE	
J5420.3300	Ø 3.3 mm, straight-concave	59
J5420.3310	Ø 3.3 mm, angled-concave	60
J5420.3800	Ø 3.8 mm, straight-concave	59
J5420.3810	Ø 3.8 mm, angled-concave	60
J5420.4300	Ø 4.3 mm, straight-concave	59
J5420.4310	Ø 4.3 mm, angled-concave	60
J5420.5000	Ø 5.0 mm, straight-concave	59
J5420.5010	Ø 5.0 mm, angled-concave	60
J8070.2050	Edentulous mandible	97

Further documentation

Further information on the CONELOG® Products can be found in the following documents:

- CONELOG® Working Instructions
- CONELOG® Instructions for Use
- Preparation instructions
- Camlog literature overview
- Clinical evidence and Science

The documents are available from the local Camlog representative.

See also:

<https://ifu.camlog.com>

www.camlog.com

References

- [1] Conserva E. Initial stability after placement of a new buttress-threaded implant. A case series study. *Implants*. 2019(3): 24-28.
- [2] Rupp J. One-year clinical experience with Progressive-Line implants. *EDI journal*. 2020(4): 54-63.
- [3] Semper-Hogg W, Kraft S, Stiller S, Mehrhof J, Nelson K. Analytical and experimental position stability of the abutment in different dental implant systems with a conical implant-abutment connection. *Clin Oral Investig*. 2013;17(3): 1017-23.
- [4] Semper-Hogg W, Zulauf K, Mehrhof J, Nelson K. The influence of torque tightening on the position stability of the abutment in conical implant-abutment connections. *Int J Prosthodont* 2015;28(5):538-41.

Legal

General disclaimer

The information provided is intended for marketing purposes only and does not qualify the user to use the product in a clinical setting. To ensure correct application, please refer to the relevant Instructions for Use and the Working Instructions before use.

Trade names and Copyright

Protected trade names (trademarks) are not always specially indicated. The absence of such a reference does NOT mean that it is not a protected trademarked name. The document including all its parts is protected by copyright. You may download the content regarding the intended use, but changes to or reproduction of the content are not permitted. Any use outside the narrow limits of copyright law without the prior written consent of CAMLOG Biotechnologies GmbH is prohibited and is subject to legal sanctions.

CAMLOG®, COMFOUR®, CONELOG®, DEDICAM®, Esthomic®, Logfit® and Promote® are registered trademarks of CAMLOG Biotechnologies GmbH. Locator®, Locator R-Tx®, R-Tx, ZEST and Zest Dental Solutions, as well as the color and shape of the retention inserts are registered trademarks of ZEST IP Holdings, LLC.

The referenced trademarks may not be registered in all countries. All third party trademarks belong to the respective trademark owners. CAMLOG Biotechnologies GmbH can only place products on the market after approval by the competent national authorities. Therefore, not all products and services are available in all countries.

Manufacturer

CAMLOG® and CONELOG® Products as well as all customized DEDICAM® Products are manufactured by:

ALTATEC GmbH | Maybachstr. 5 | 71299 Wimsheim | Germany

Locator® and Locator R-Tx® are manufactured by the Zest Anchors company.

CE 0123

Art. No. J8001.0009 Rev. 08 05/2023



+E219J800100091J



+S0080125505J\$

Headquarters

CAMLOG Biotechnologies GmbH | Margarethenstr. 38 | 4053 Basel | Switzerland

Phone +41 61 565 41 00 | Fax +41 61 565 41 01 | info@camlog.com | www.biohorizonscamlog.com

Inspiring excellence in oral reconstruction

