

a perfect fit™

CAMLOG® IMPLANT SYSTEM PRODUCT CATALOG 2014

Valid from September 2014

camlog

ADDED VALUE THROUGH COMPETENCE IN IMPLANTOLOGY

A partnership with CAMLOG encompasses the exceptional price-performance ratio of the CAMLOG® Products and a custom-built service program. CAMLOG's specific expertise clearly encompasses more than the product, its safety and ease of use. With all our implant expertise, we are fully committed to our customers. Rediscover the implant expertise of CAMLOG in your daily routine time and time again, and turn it into your own added value.

We are happy to help.

FOR PERFECTIONISTS

FOR MINIMALISTS

FOR FANS



THE CAMLOG® IMPLANT SYSTEM		CAMLOG® PROSTHETICS	41
SYSTEM INFORMATION	3	PROSTHETICS OVERVIEW	42
NEW PRODUCTS	3	TORQUE WRENCH SETTINGS	48
SURGERY	11	IMPRESSION TAKING, BITE REGISTRATION, FABRICATION OF THE PLASTER MODEL	50
PLANNING	12	IMPRESSION TAKING, CLOSED/OPEN TRAY	50
X-RAY PLANNING FOILS	12	BITE REGISTRATION	51
X-RAY TRANSFER PICTURES	12	FABRICATION OF THE PLASTER MODEL	51
CT-PLANNING	13	CROWN AND BRIDGE RESTORATIONS	52
IMPLANT OVERVIEW	14	CAMLOG® TEMPORARY ABUTMENTS	52
SCREW-LINE	16	CAMLOG® ESTHOMIC® ABUTMENTS	52
CAMLOG® SCREW-LINE IMPLANTS	16	CAMLOG® UNIVERSAL ABUTMENTS	55
SURGERY SET CAMLOG®/CONELOG® SCREW-LINE	18	CAMLOG® GOLD-PLASTIC ABUTMENTS	55
SURGICAL INSTRUMENTS SCREW-LINE	19	CAMLOG® CERAMIC ABUTMENTS	55
OSTEOTOMY SETS SCREW-LINE	22	CAMLOG® LOGFIT® PROSTHETIC SYSTEM	56
GUIDE SYSTEM	26	CROWN, BRIDGE AND HYBRID RESTORATIONS	57
ROOT-LINE 2	30	CAMLOG® TITANIUM BASES CAD/CAM	57
CAMLOG® ROOT-LINE 2 IMPLANTS	30	ACCESSORIES FOR CAMLOG® ABUTMENTS	58
SURGERY SET CAMLOG® ROOT-LINE 2	31	CAMLOG® VARIO SR ABUTMENTS	59
SURGICAL INSTRUMENTS ROOT-LINE 2	32	ACCESSORIES FOR VARIO SR	60
CAMLOG® HEALING CAPS	34	HYBRID RESTORATIONS	62
ALTAPIN SET	35	BAR RESTORATIONS	62
INSTRUMENTS	36	BALL ABUTMENT ANCHORING SYSTEM	64
SURGICAL INSTRUMENTS	36	LOCATOR® ANCHORING SYSTEM	66
SURGICAL-PROSTHETIC INSTRUMENTS	38	DOUBLE CROWN RESTORATIONS WITH CAMLOG®	
PROSTHETIC INSTRUMENTS	39	UNIVERSAL AND TELESCOPE ABUTMENTS	69
		ACCESSORIES FOR CAMLOG® ABUTMENTS	69
		INSTRUMENTS FOR DENTAL TECHNICIANS	70
		CAMLOG® SELECTION ABUTMENTS	72
		AUXILIARY ARTICLE	73
		INFORMATION	77
		INDEX	81
		ALPHABETICAL	82
		ARTICLE NUMBERS	90
		ORDER FORM	99

THE CAMLOG® IMPLANT SYSTEM

SYSTEM INFORMATION

THE CAMLOG® IMPLANT SYSTEM

The CAMLOG® Implant System is based on years of clinical and laboratory experience and is a user-friendly, consistent prosthetically oriented implant system.

The CAMLOG® Implant System is being continuously developed and adapted to the state of technology by the internal research and development team in collaboration with clinics, universities and dental technicians.

The CAMLOG® Implant System is well documented scientifically. Numerous studies based on various parameters, e.g. implant surface, time of implantation and/or implant loading, primary stability, connection design or type of suprastructure, support this. The long-term outcomes for the CAMLOG® Implant System are persuasive.

NEW PRODUCTS

CAMLOG® ROOT-LINE 2

CAMLOG® ROOT-LINE 2 Implants

The CAMLOG® ROOT-LINE Implants have been adapted and are now available with the proven Tube-in-Tube™ implant-abutment connection with short angular grooves, identical to the inner configuration of the CAMLOG® SCREW-LINE Implants. CAMLOG® ROOT-LINE 2 Implants are thus suitable for the Platform Switching option (not for Ø 3.3 mm).

In terms of outer geometry, the machined neck area was shortened to 0.4 mm (Promote® plus). The thus enlarged Promote® surface offers greater bone contact. The raised cutting groove delivers optimized tightening, even in hard bone.

The implant line was extended by the 3.3 mm diameter with implant lengths of 11, 13 and 16 mm.

CAMLOG® ROOT-LINE 2 Instruments

The adaptation of the outer geometry of the CAMLOG® ROOT-LINE Implants required new color-coded reusable form drills, including depth stops and reusable taps, new without internal irrigation.

LOCATOR®

A new replacement male is available for the Locator® Anchoring system for extended range without retention. The replacement male is colored gray and serves to adapt the cumulated retention force of a Locator® retained prosthesis on implants with diameters 3.8/4.3/5.0 mm.

GUIDE SYSTEM

The CAMLOG® Guide System for template-guided implant bed preparation and insertion has been extended by the CONELOG® SCREW-LINE Implants and is now called the Guide System.

Guide System CONELOG® SCREW-LINE Implants are available with a 3.3 mm diameter in the lengths 9, 11, 13 and 16 mm, as well as with 3.8 and 4.3 mm diameters in the lengths 7, 9, 11, 13 and 16 mm.

Additional Guide System CAMLOG® SCREW-LINE Implants were also added to the system. These are available new with a diameter of 3.3 mm in the lengths 11, 13 and 16 mm, as well as diameters 3.8 and 4.3 mm with a length of 16 mm, including the corresponding surgical instruments.

Newly available are guided pilot drills and a driver with ISO shaft for Guide System implants. The form drills were fitted with a four-edged cutting geometry with chip grooves to provide greater smoothness of operation. The guide sleeves were shortened by 1 mm for minimally invasive implantation at greater gingival thickness, provided with opposing bevels for use in narrow tooth gaps and fitted with a marking to give better groove alignment. The template drills are fitted newly with a spiral-shaped cutting edge and a longer shaft. All drills, gingiva punches, insertion posts and guide sleeves are color-coded throughout.

The new Guide System comprises 85 items.

CAMLOG® ScanPost for Sirona Scanbody

In conjunction with a Sirona Scanbody, the new CAMLOG® ScanPost serves for the digital recording of the implant position or laboratory analog position in relation to the remaining teeth and the soft tissue.

THE CAMLOG® IMPLANT SYSTEM

SYSTEM INFORMATION


CAMLOG® IMPLANTATLINIEN

CAMLOG® SCREW-LINE Implants

SCREW-LINE implants represent conical self-tapping screw implants in their geometry and are available with Promote® (1.4 mm machined implant neck part) and Promote® plus (0.4 mm machined implant neck part) surfaces.

Both implant versions include the Tube-in-Tube™ Inner configuration with square grooves making the Platform Switching option available to the user.

CAMLOG® SCREW-LINE Implants are mounted in the sterile packaging with an insertion post color-coded based on the diameter. Implant diameters: 3.3/3.8/4.3/5.0/6.0 mm. Implant lengths: 9/11/13/16 mm.

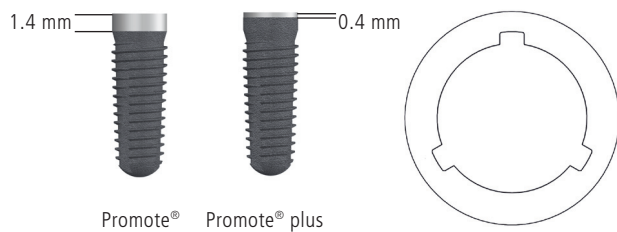

CAMLOG® ROOT-LINE 2 Implants

CAMLOG® ROOT-LINE 2 Implants represent root-shaped screw implants in terms of their outer geometry. The geometry of the implant body allows its use at limited apical bone and is easy to insert due to self-centering.


The outer surface of the implants is abrasive-blasted and acid-etched (Promote® surface structure). The implants are available with Promote® plus surface (0.4 mm machined implant neck area). The implant shoulder is machined.

The implants are equipped with the proven Tube-in-Tube™ implant-abutment connection and feature three symmetrically arranged angular grooves in the cylindrical part of the implant neck. The implants can therefore be used for the Platform Switching option.

CAMLOG® ROOT-LINE 2 Implants are mounted in the sterile packaging with an insertion post color-coded based on the diameter.

Implant diameters: 3.3/3.8/4.3/5.0/6.0 mm.

Implant lengths: 9/11/13/16 mm.

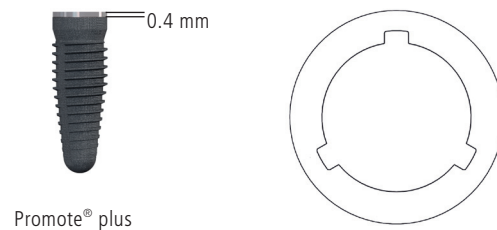

Note: The option of Platform Switching may only be used with CAMLOG® SCREW-LINE Implants with K article numbers!


THE CAMLOG® IMPLANT SYSTEM

SYSTEM INFORMATION

CAMLOG SURFACE STRUCTURES

Promote® surface



CAMLOG® Implants are available with the Promote® surface. On CAMLOG® SCREW-LINE Implants, the abrasive-blasted, acid-etched Promote® surface extends up to 1.4 mm under the implant shoulder and the Promote® plus surface up to 0.4 mm under the implant shoulder. In the case of CAMLOG® ROOT-LINE 2 Implants this reaches up to 0.4 mm under the implant shoulder (Promote® plus). The Promote® surface has proven its worth as a surface for anchoring dental implants in the bone and has shown good scientific results in osteohistology and in pull-out trials. These results suggest that the Promote® surface leads to rapid osseointegration of the CAMLOG® Implants.



Promote® surface

CAMLOG® Tube-in-Tube™ Implant-Abutment Connection


All CAMLOG® Implants are equipped with the proven Tube-in-Tube™ implant-abutment connection and feature three symmetrically arranged angular grooves (width 0.5 or 0.7 mm, depth 1.2 mm).



CAMLOG® Implant inner thread and outer geometry

Within the Tube-in-Tube™ Connection, an upper inner thread attaches for all CAMLOG® Implant lines with 3.8/4.3/5.0/6.0 mm outer diameter, in which the thread of the CAMLOG® Healing cap engages (for CAMLOG® Implants with \varnothing 3.3 mm lower inner thread only). There is a second inner thread towards the apex M 1.6 or M 2.0 (to receive the CAMLOG® Abutment and fixing screw).

For optimal positioning of the abutments in the implant, they should be aligned in the bone so that one of the three grooves points vestibularly. With the CAMLOG® SCREW-LINE and ROOT-LINE 2 Implants, the drivers include markings that correspond to the three grooves of the implant inner configuration.

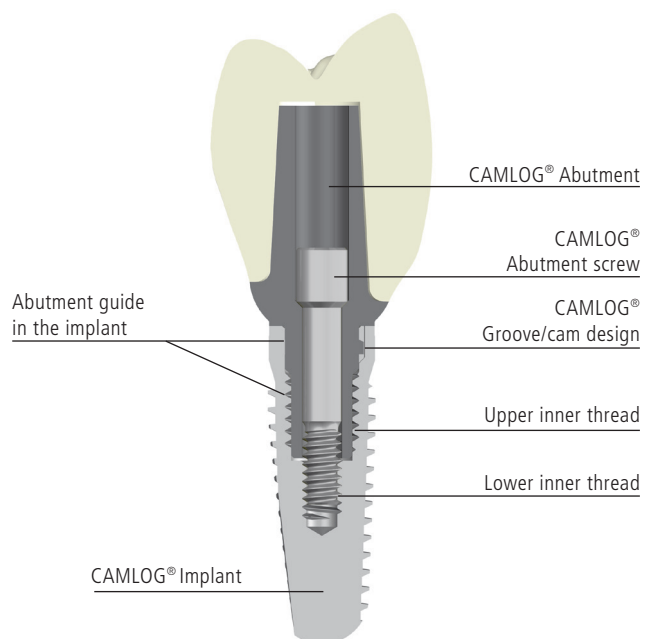

The inner and outer geometry of the CAMLOG® Implants and abutments are rotary machined for the most part. The tolerances can therefore be kept very low. The result is excellent part precision without impacting the material structure. The patented Tube-in-Tube™ Design of the implant abutment connection (Patent EP 851 744 and corresponding property rights) thus ensures a very precise, stable and rotation-securing connection to the prosthetic components.


THE CAMLOG® IMPLANT SYSTEM

SYSTEM INFORMATION

PLATFORM SWITCHING OPTION

CAMLOG® Healing caps PS for Platform Switching

The CAMLOG® Healing caps PS (cylindrical, wide body, bottle-neck) are tapered in diameter at the shoulder support making it possible to adapt soft tissue over the implant shoulder.




CAMLOG® Impression posts PS, open and closed tray for Platform Switching

Due to the adaptation of the soft tissue over the implant shoulder, the use of the CAMLOG® Healing cap PS necessitates the use of the CAMLOG® Impression post PS for Platform Switching, with both having an identical geometry. The cams of the impression posts are adapted to the grooves of the CAMLOG® Implants.




CAMLOG® Temporary abutments PS, CAMLOG® Esthomic® Abutments PS and CAMLOG® Universal abutments PS for Platform Switching

The CAMLOG® Abutments PS are also tapered in diameter in the area of the shoulder support and thus allow adapting soft tissue over the implant shoulder during prosthetic restoration. The cams of the abutments are adapted to the grooves of the CAMLOG® Implants.

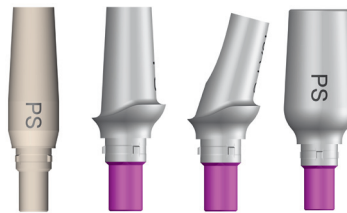

The Platform Switching option is used to support the hard and soft tissue in esthetic regions. Due to the horizontally reduced diameter of the CAMLOG® Abutment PS in relationship to the implant diameter, the implant-abutment interface on the implant shoulder is shifted towards the middle of the implant.

The CAMLOG® Healing caps PS, impression posts PS and abutments PS are for exclusive use only with CAMLOG® Implants with K article numbers.

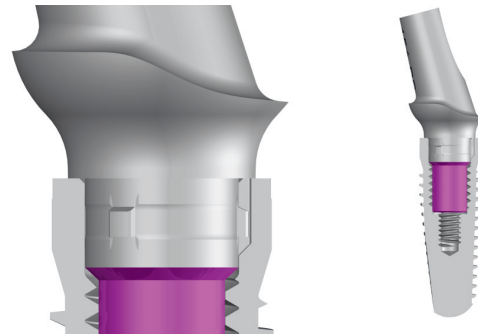

PS: Platform Switching


THE CAMLOG® IMPLANT SYSTEM

SYSTEM INFORMATION

CAMLOG® Abutments with K article numbers


The abutments are tubular and extended toward the apex (5.4 mm) and have three cams in the upper area that correspond to the three grooves in the implant.

All CAMLOG® Abutments with K article numbers are fitted with shortened cams which fit the shortened grooves of the CAMLOG® Implants.

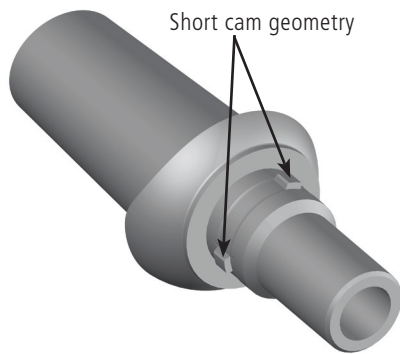

When inserting the abutments, their tubular extension toward the apex affects the simple, easy and safe orientation in the longitudinal axis before the three cams rest on the shoulder of the implant. The abutment is rotated until perceptible engagement of the cams into the grooves of the implant. The abutment is then in the final position.

The implant-abutment connection of the CAMLOG® Implant System is predominantly a form-fitting connection. The connection with the short cam geometry has been optimized biomechanically by means of extensive finite element analyses. The figure below shows the distribution of the von Mises tension in the implant-abutment connection at a load in accordance to ISO 14801 with 200 N.

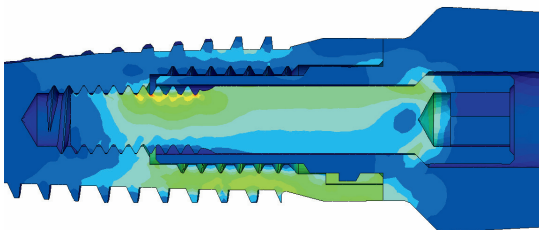


CAMLOG® Healing caps

The various healing caps are used for single-stage or two-stage procedures based on the indication. The CAMLOG® Healing caps are available in three geometries (cylindrical, wide body and bottleneck).

CAMLOG® Healing caps PS (cylindrical, wide body and bottleneck) for Platform Switching are also available.

CAMLOG® Bar and ball abutments, Locator® Abutments

These abutments differ from regular abutments through an apical thread that attaches into the upper or lower (implants with \varnothing 3.3 mm) implant inner thread. For hybrid prosthetics, CAMLOG® Bar, ball and Locator® Abutments are available that do not have cams due to their function.



CAMLOG® Bar, ball and Locator® Abutment

THE CAMLOG® IMPLANT SYSTEM

SYSTEM INFORMATION

PROSTHETIC RESTORATIONS

CAMLOG® Implants can be provided with a pallet of wide-ranging, anatomically appropriate prosthetic components. Esthetic solutions are easily achievable. Nearly all CAMLOG® Abutments are color-coded corresponding to implant diameters.

CAMLOG® Abutments for crown and bridge restorations

- CAMLOG® Temporary abutment
- CAMLOG® Temporary abutment PS for Platform Switching
- CAMLOG® Esthomic® Abutments
- CAMLOG® Esthomic® Abutments PS for Platform Switching
- CAMLOG® Universal abutment
- CAMLOG® Universal abutment PS for Platform Switching
- CAMLOG® Gold-plastic abutment
- CAMLOG® Titanium base CAD/CAM
- CAMLOG® Ceramic abutment
- CAMLOG® Logfit® Abutment
- CAMLOG® Vario SR abutment

CAMLOG® Abutments for hybrid restorations

- CAMLOG® Bar abutment
- CAMLOG® Ball abutment
- CAMLOG® Locator® Abutment
- CAMLOG® Universal and telescope abutment
- CAMLOG® Vario SR abutments

CAMLOG® Temporary abutment

The temporary abutments (PEEK material) can be used after immediate implantation or after opening for temporary restoration. Temporary abutments and temporary abutments PS for Platform Switching are also available.

CAMLOG® Esthomic® Abutments


The abutments of the Esthomic® Line have an anatomical shaped shoulder and are available in various gingival heights.

- CAMLOG® Esthomic® Abutment, straight
- CAMLOG® Esthomic® Abutment, 15° angled, in type A and B
- CAMLOG® Esthomic® Abutment, 20° angled, in type A and B
- CAMLOG® Esthomic® Abutment, inset

After fabricating the master model, the suitable CAMLOG® Esthomic® Abutments can be quickly and easily selected using the color-coded CAMLOG® Esthomic® Selection abutments in the dental laboratory. There is no longer any need for expensive and complicated storage of abutments, either by the dentist or at the prosthodontist or dental laboratory.

Angled CAMLOG® Esthomic® Abutments, type A and B

Angled abutments type A and B are available in the Esthomic® Line of abutments. Type A has a cam opposing the angle direction. In contrast to type A, type B has a 60° offset cam. Both types make six different rotation positions possible to achieve an optimal prosthetic axis alignment.

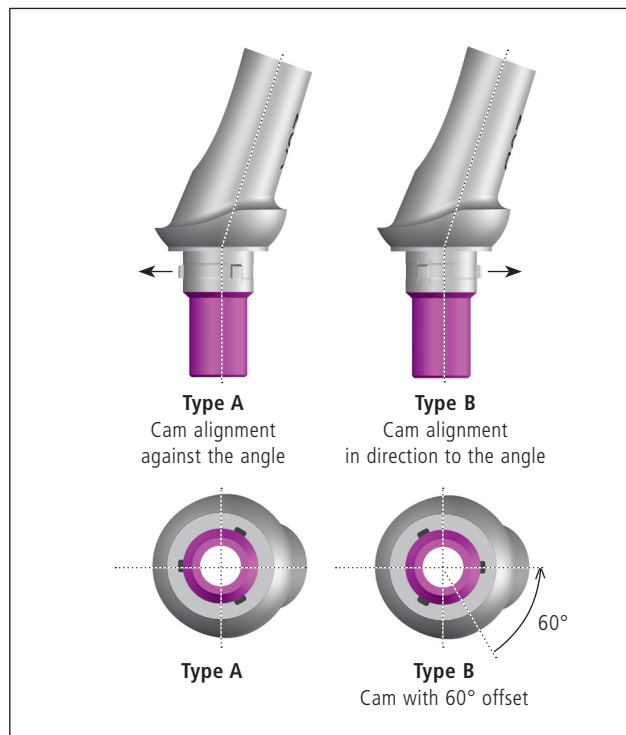

CAMLOG® Vario SR abutments

CAMLOG® Vario SR abutments are available in straight, in 20° and 30° angled versions. These abutments can compensate for large implant axis divergences. Prefabricated Vario SR prosthetic components make fabrication of occlusally screw-retained crown, bridge and bar restorations possible. Burn-out plastic copings can be used to fabricate cast crown and bridge restorations. The titanium caps have a retention surface on the outside and are designed for temporary or final bridge restorations made of plastic. Titanium bases for bar are available for laser-welded bar restorations.

Surgical instruments

The surgical instruments are matched to the individual implant lines and are color-coded to match the diameter of the implant.

For a simple overview and handling, autoclavable surgery sets are available for the respective implant lines with all required instruments. The instruments are sorted and marked in the set based on the sequence during implant bed preparation.

Healing with the various types of implants can in principle be performed transgingival (single phase) or subgingival (two-phase) according to indication. See also description of indications in the respective instructions for use.

THE CAMLOG® IMPLANT SYSTEM

SYSTEM INFORMATION

GENERAL SAFETY INSTRUCTIONS AND WARNINGS

The descriptions in this product catalog are not sufficient to allow immediate use of the CAMLOG® Implant System. Instruction by a surgeon experienced in using the CAMLOG® Implant System is strongly recommended.

An improper procedure during use of the CAMLOG® Products can lead to failures, implant damage, bone loss or unsatisfactory esthetic results. The products may be used only by dentists, surgeons and dental technicians trained in the implant system. Use of these products requires specialized knowledge and experience in implant dentistry. Detailed information on the choice of suitable implants, prosthetic components, treatment planning and application is contained in the user information. Your local representative will be happy to provide you with information.

Consulting and technical advice on the use of our products is provided orally, in writing, by electronic media and/or by demonstration. The provided information represents the current state of science and technology known to us at the point in time that the product is placed on the market.

This does not exempt the user from the responsibility to personally test the product for suitability for the intended purpose, indication and procedure. Handling and use of the product take place outside of our control and is the direct responsibility of the user. All liability for damages resulting from such use is waived. ALTATEC GmbH/CAMLOG Biotechnologies AG does not warrant nor provide replacement services when non-system components are used.

The CAMLOG® Implant System is part of a comprehensive treatment concept and must be used only with the pertinent original parts and tools according to the suggestions and instructions for use provided by the manufacturer. All components of the CAMLOG® Implant System are matched precisely to one another. The use of third party components can affect the function and safety of the system.

Instruments and system components are designed for specific implant and prosthetic lines and implant diameters. Their use with any other implant or prosthetic product lines or a different diameter can lead to the mechanical failure of system components, tissue injury, or esthetically unsatisfactory results. Because of this, some implant and prosthetic product lines have some dedicated components and tools. Pay attention to the color markings when choosing instruments for the required implant diameter.

Products intended for single use must not be reused because safe preparation and/or functional safety cannot be ensured.

Within the bounds of our sales and delivery terms, we guarantee the flawless quality of our products.

Because of the small sizes involved, it may happen that a product is swallowed and/or aspirated. Aspiration can lead to dyspnea and in the worst case to asphyxiation. For this reason, products must be secured in general against aspiration and swallowing during intraoral use.

Where indications are listed for a particular product, it should be noted that any indications that are not listed are in fact contraindicated.










Sterile packaged products must be kept dry, out of direct sunlight and at room temperature. The packaging must be checked before opening for damage and for the expiration date and should only be opened immediately before the products are used.

Not all products are available in all countries.

PACKAGING UNITS

If not otherwise specified, the packaging unit is 1 each.

EXPLANATION OF SYMBOLS/CHARACTERS ON LABELS/PRODUCT LABELS AND PACKAGE INSERTS

	Sterilization using irradiation
	Non-sterile
	Caution, consult accompanying documents
	Use by
	Do not reuse
	Article number
	Lot number
	Manufacturer
	Temperature limitation
Rx only	Caution: US Federal law restricts this device to sale by or on the order of a dentist or physician.

COLOR-CODING OF THE SURGICAL AND PROSTHETICAL CAMLOG® PRODUCTS

	Color	Diameter
	gray	3.3 mm
	yellow	3.8 mm
	red	4.3 mm
	blue	5.0 mm
	green	6.0 mm

THE CAMLOG® IMPLANT SYSTEM

SYSTEM INFORMATION

Exterior packaging:

Sealed, color-coded, folding carton with product label


Secondary packaging:

Sealed

Implant internal packaging (primary packaging):

Sealed, color-coded

Example product label of exterior implant packaging

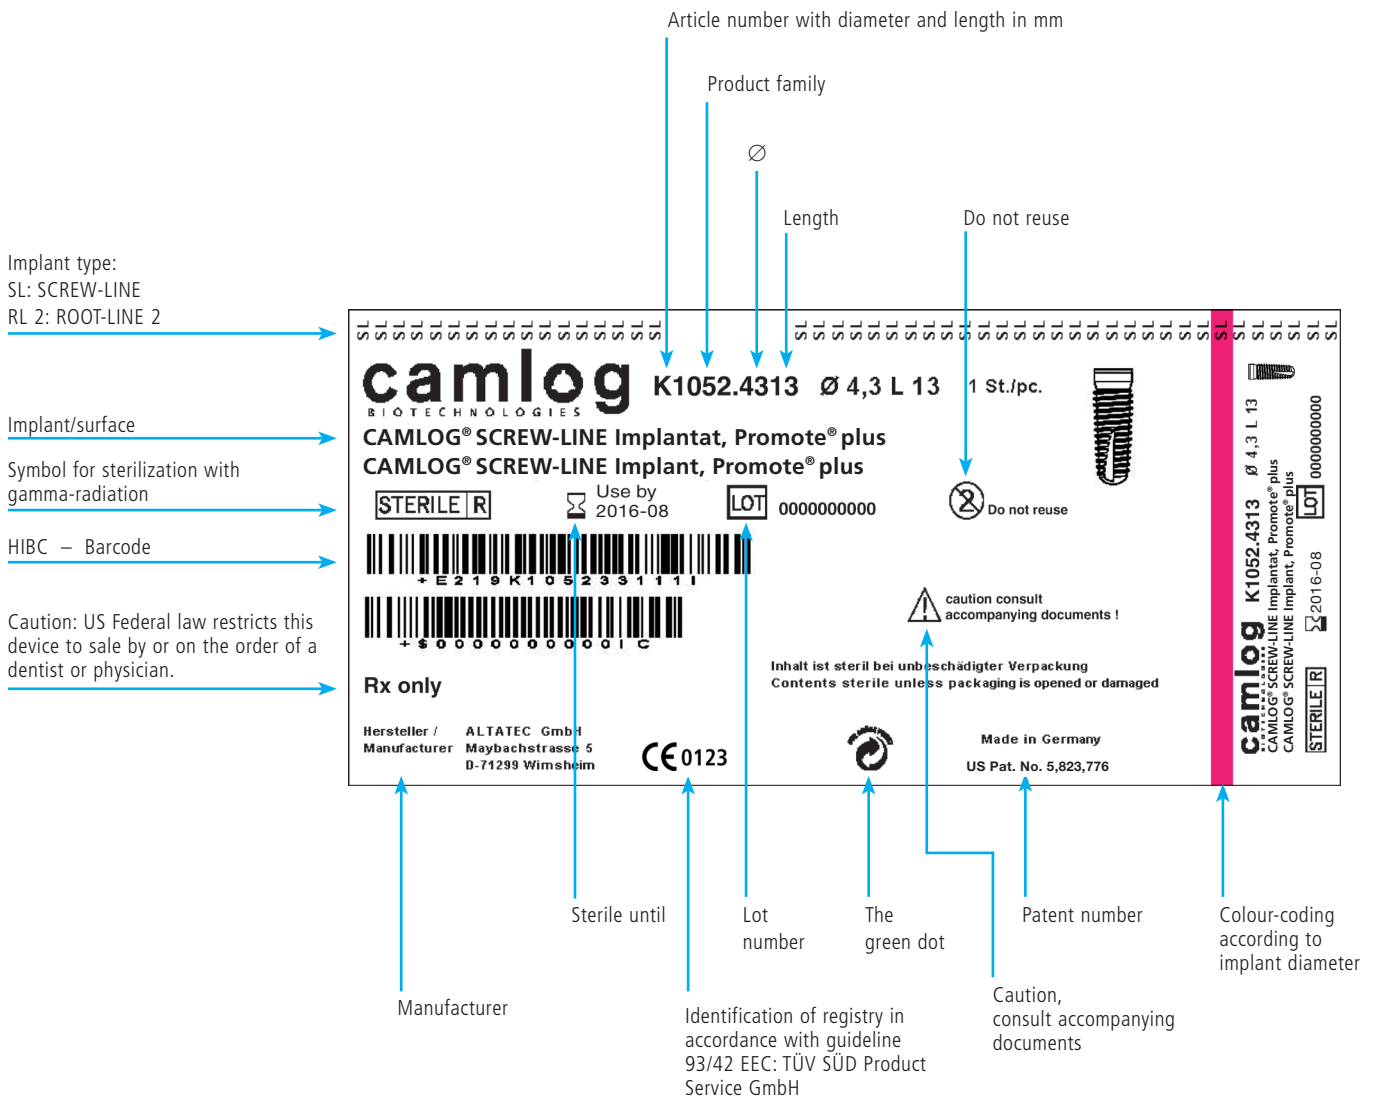

SURGERY	11
PLANNING	12
X-RAY PLANNING FOILS	12
X-RAY TRANSFER PICTURES	12
CT-PLANNING	13
IMPLANT OVERVIEW	14
SCREW-LINE	16
CAMLOG® SCREW-LINE IMPLANTS	16
SURGERY SET CAMLOG®/CONELOG® SCREW-LINE	18
SURGICAL INSTRUMENTS SCREW-LINE	19
OSTEOTOMY SETS SCREW-LINE	22
GUIDE SYSTEM	26
ROOT-LINE 2	30
CAMLOG® ROOT-LINE 2 IMPLANTS	30
SURGERY SET CAMLOG® ROOT-LINE 2	31
SURGICAL INSTRUMENTS ROOT-LINE 2	32
CAMLOG® HEALING CAPS	34
ALTAPIN SET	35
INSTRUMENTS	36
SURGICAL INSTRUMENTS	36
SURGICAL-PROSTHETIC INSTRUMENTS	38
PROSTHETIC INSTRUMENTS	39

SURGERY


X-RAY PLANNING FOILS / X-RAY TRANSFER PICTURES

Art. No.

Article


∅
in mm

K5300.9010

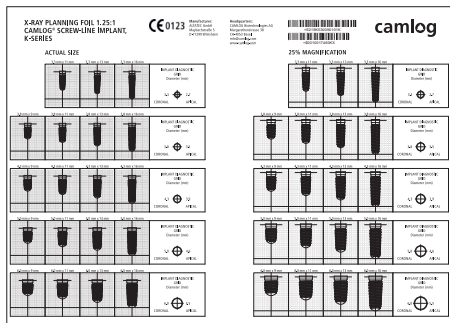


**X-Ray Planning foil 1.25:1
CAMLOG® SCREW-LINE Implants**
Magnification 25%

K5300.9012

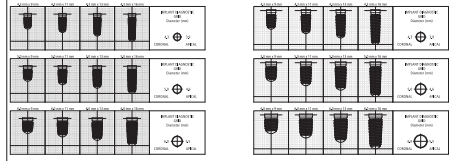


**X-Ray Planning foil 1.25:1
CAMLOG® ROOT-LINE 2 Implants**
Magnification 25%

K5300.9011

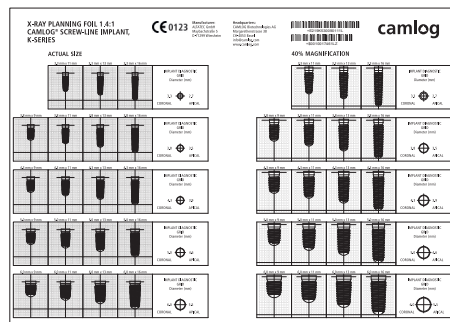


**X-Ray Planning foil 1.4:1
CAMLOG® SCREW-LINE Implants**
Magnification 40%

K5300.9013

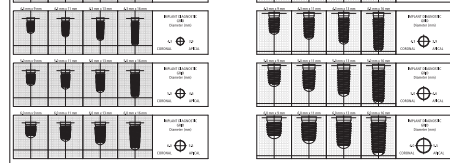

**X-Ray Planning foil 1.4:1
CAMLOG® ROOT-LINE 2 Implants**
Magnification 40%

K5300.9080

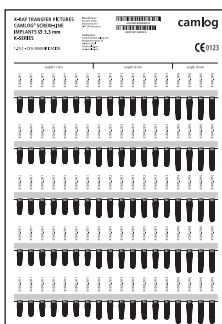

**X-Ray Transfer pictures 1.25:1
CAMLOG® SCREW-LINE Implants**

3.3

K5300.9081

Planning slide, self-adhesive
Magnification 25%

3.8

K5300.9082

4.3


K5300.9083

5.0

K5300.9084

6.0

K5300.9070

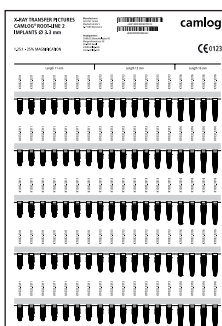

**X-Ray Transfer pictures 1.25:1
CAMLOG® ROOT-LINE 2 Implants**

3.3

K5300.9071

Planning slide, self-adhesive
Magnification 25%

3.8

K5300.9072





4.3

K5300.9073

5.0

K5300.9074


6.0

Art. No.		Article	Material
A2002.2000		<p>CT-tube for drill \varnothing 2.0 mm, corrugated tubing, length 4.0/10.0 mm, internal diameter 2.1 mm, external diameter 2.5 mm, pack of 10</p>	Titanium alloy
A2222.2200		<p>CT-tube for drill \varnothing 2.2 mm, corrugated tubing, length 4.0/10.0 mm, internal diameter 2.3 mm, external diameter 2.7 mm, pack of 10</p>	Titanium alloy
A2050.2600		<p>Drill for CT-tube (for A2002.2000), \varnothing 2.6 mm</p>	Stainless steel
A2050.2800		<p>Drill for CT-tube (for A2222.2200), \varnothing 2.8 mm</p>	Stainless steel

SURGERY

IMPLANT OVERVIEW

CAMLOG® SCREW-LINE IMPLANT Promote®



Length: 9 mm

Length: 11 mm


Length: 13 mm

Length: 16 mm

∅ apical
(mean value)

	∅ 3.3 mm	∅ 3.8 mm	∅ 4.3 mm	∅ 5.0 mm	∅ 6.0 mm
Length: 9 mm		K1042.3809	K1042.4309	K1042.5009	K1042.6009
Length: 11 mm	K1042.3311	K1042.3811	K1042.4311	K1042.5011	K1042.6011
Length: 13 mm	K1042.3313	K1042.3813	K1042.4313	K1042.5013	K1042.6013
Length: 16 mm	K1042.3316	K1042.3816	K1042.4316	K1042.5016	K1042.6016
∅ apical (mean value)	2.7 mm	3.5 mm	3.9 mm	4.6 mm	5.5 mm

CAMLOG® SCREW-LINE IMPLANT Promote® plus



Length: 9 mm

Length: 11 mm




















Length: 13 mm

Length: 16 mm

∅ apical
(mean value)

	∅ 3.3 mm	∅ 3.8 mm	∅ 4.3 mm	∅ 5.0 mm	∅ 6.0 mm
Length: 9 mm		K1052.3809	K1052.4309	K1052.5009	K1052.6009
Length: 11 mm	K1052.3311	K1052.3811	K1052.4311	K1052.5011	K1052.6011
Length: 13 mm	K1052.3313	K1052.3813	K1052.4313	K1052.5013	K1052.6013
Length: 16 mm	K1052.3316	K1052.3816	K1052.4316	K1052.5016	K1052.6016
∅ apical (mean value)	2.7 mm	3.5 mm	3.9 mm	4.6 mm	5.5 mm

SURGERY IMPLANT OVERVIEW

	∅ 3.3 mm	∅ 3.8 mm	∅ 4.3 mm	∅ 5.0 mm	∅ 6.0 mm
		K1032.3809 	K1032.4309 	K1032.5009 	K1032.6009 
K1032.3311 	K1032.3811 	K1032.4311 	K1032.5011 	K1032.6011 	
K1032.3313 	K1032.3813 	K1032.4313 	K1032.5013 	K1032.6013 	
K1032.3316 	K1032.3816 	K1032.4316 	K1032.5016 	K1032.6016 	
2.2 mm	2.3 mm	2.55 mm	2.9 mm	3.8 mm	


CAMLOG® ROOT-LINE 2 IMPLANT Promote® plus

Length: 9 mm

Length: 11 mm

Length: 13 mm





Length: 16 mm



∅ apical
(mean value)





SURGERY SCREW-LINE

CAMLOG® SCREW-LINE IMPLANTS PROMOTE®

Art. No.	Article	Ø in mm	Length in mm	Material
K1042.3311	CAMLOG® SCREW-LINE Implant, Promote® incl. insertion post and cover screw, sterile	3.3	11	Titanium Grade 4
K1042.3313			13	
K1042.3316			16	
K1042.3809		3.8	9	
K1042.3811			11	
K1042.3813			13	
K1042.3816			16	
K1042.4309		4.3	9	
K1042.4311			11	
K1042.4313			13	
K1042.4316			16	
K1042.5009		5.0	9	
K1042.5011			11	
K1042.5013			13	
K1042.5016			16	
K1042.6009		6.0	9	
K1042.6011			11	
K1042.6013			13	
K1042.6016			16	

SURGERY SCREW-LINE

CAMLOG® SCREW-LINE IMPLANTS PROMOTE® PLUS

Art. No.	Article	Ø in mm	Length in mm	Material
K1052.3311	CAMLOG® SCREW-LINE Implant, Promote® plus incl. insertion post and cover screw, sterile	3.3	11	Titanium Grade 4
K1052.3313			13	
K1052.3316			16	
K1052.3809		3.8	9	
K1052.3811			11	
K1052.3813			13	
K1052.3816			16	
K1052.4309		4.3	9	
K1052.4311			11	
K1052.4313			13	
K1052.4316			16	
K1052.5009		5.0	9	
K1052.5011			11	
K1052.5013			13	
K1052.5016			16	
K1052.6009		6.0	9	
K1052.6011			11	
K1052.6013			13	
K1052.6016			16	

The Promote® surface has proven its worth as a reliable dental implant surface. Numerous scientific studies demonstrate this. To provide the bone with a larger rough surface as an anchor, the Promote® plus area of CAMLOG® SCREW-LINE Implants Promote® plus was increased by an additional portion of 1.0 mm, right up to the bone-soft tissue margin compared to the Promote® surface. This extends the bone-implant contact surface of Promote® plus upward to the esthetically relevant coronal zone. Since they have the same insertion protocol, Promote® and Promote® plus implants can be used freely in combination.

Note: With CAMLOG® SCREW-LINE Implants with diameter 3.8/4.3/5.0/6.0 mm the option of Platform Switching is possible. See also information on page 6.

SURGERY SCREW-LINE

SURGERY SET CAMLOG®/CONELOG® SCREW-LINE

Art. No.

Article

J5300.0057

Surgery set CAMLOG®/CONELOG® SCREW-LINE







Contains all necessary color-code ordered surgical instruments, incl. torque wrench and holding key for insertion post (drills and taps for \varnothing 6.0 mm are not included)



Note: The preparation of the implant bed for CAMLOG® SCREW-LINE Implants and for CONELOG® SCREW-LINE Implants is identical.

SURGERY SCREW-LINE











SURGICAL INSTRUMENTS SCREW-LINE

Art. No.	Image	Article	∅ in mm	Length in mm	Material
J5050.2300*		Round bur resterilizable	2.3	–	Stainless steel
J5050.3500		Round bur resterilizable	3.5	–	Stainless steel
J5051.2003		Pilot drill without coil, resterilizable	2.0	–	Stainless steel
J5051.2000*		Pilot drill SCREW-LINE reduced coil, resterilizable	2.0	–	Stainless steel
J5051.2800*		Pre-drill SCREW-LINE resterilizable	1.7-2.8	–	Stainless steel
J5015.0009*		Depth stop SCREW-LINE	–	9	Stainless steel
J5015.0011*		for pilot drill (J5051.2000) and	–	11	
J5015.0013*		pre-drill (J5051.2800) with reduced coil, resterilizable	–	13	

* The instruments listed above are also included in the surgery set CAMLOG®/CONELOG® SCREW-LINE.

SURGERY SCREW-LINE



SURGICAL INSTRUMENTS SCREW-LINE

Art. No.	Article	Ø in mm	Length in mm	Material
J5052.3309 J5052.3311 J5052.3313 J5052.3316	 Form drill SCREW-LINE with reduced coil, resterilizable	3.3	9 11 13 16	Stainless steel
J5052.3809 J5052.3811 J5052.3813 J5052.3816		3.8	9 11 13 16	
J5052.4309 J5052.4311 J5052.4313 J5052.4316		4.3	9 11 13 16	
J5052.5009 J5052.5011 J5052.5013 J5052.5016		5.0	9 11 13 16	
J5052.6009 J5052.6011 J5052.6013 J5052.6016		6.0	9 11 13 16	
J5015.3300	 Depth stop for form drills SCREW-LINE and ROOT-LINE 2 with reduced coil, resterilizable	3.3	–	Titanium alloy
J5015.3800		3.8	–	
J5015.4300		4.3	–	
J5015.5000		5.0	–	
J5015.6000		6.0	–	

The instruments listed above are also included in the surgery set CAMLOG®/CONELOG® SCREW-LINE (drills with Ø 6.0 mm are not included).

SURGERY SCREW-LINE

SURGICAL INSTRUMENTS SCREW-LINE

Art. No.	Article	\varnothing in mm	Length in mm	Material
J5053.3316	 Form drill SCREW-LINE, Cortical bone, resterilizable	3.3	–	Stainless steel
J5053.3816		3.8	–	
J5053.4316		4.3	–	
J5053.5016		5.0	–	
J5053.6016		6.0	–	
J5054.3309	 Tap SCREW-LINE, with hexagon, resterilizable	3.3	–	Stainless steel
J5054.3809		3.8	–	
J5054.4309		4.3	–	
J5054.5009		5.0	–	
J5054.6009		6.0	–	

The instruments listed above are also included in the surgery set CAMLOG®/CONELOG® SCREW-LINE (drills and taps with \varnothing 6.0 mm are not included).

SURGERY SCREW-LINE

OSTEOTOMY SET SCREW-LINE

Art. No.	Article	Ø in mm	Material
----------	---------	------------	----------

J5418.0020



Osteotomy set CAMLOG®/CONELOG® SCREW-LINE, straight convex

Content:

J5417.2800 Pre-Osteotome SCREW-LINE, straight convex	1.7-2.8
J5418.3300 Osteotome SCREW-LINE, straight convex	3.3
J5418.3800 Osteotome SCREW-LINE, straight convex	3.8
J5418.4300 Osteotome SCREW-LINE, straight convex	4.3
J5418.5000 Osteotome SCREW-LINE, straight convex	5.0
J5418.6000 Osteotome SCREW-LINE, straight convex	6.0

J5417.2800



Pre-Osteotome SCREW-LINE
straight convex

1.7-2.8 Stainless steel

J5418.3300



Osteotome SCREW-LINE
straight convex

3.3 Stainless steel

J5418.3800



3.8

J5418.4300



4.3

J5418.5000



5.0

J5418.6000




6.0



SURGERY SCREW-LINE OSTEOTOMY SET SCREW-LINE

Art. No.	Article	Ø in mm	Material
----------	---------	------------	----------

J5418.0030

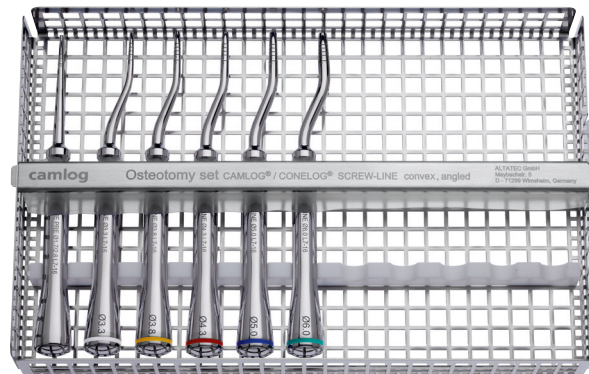

Osteotomy set CAMLOG®/CONELOG® SCREW-LINE, angled convex

Content:

J5417.2800 Pre-Osteotome SCREW-LINE, straight convex	1.7-2.8
J5418.3310 Osteotome SCREW-LINE, angled convex	3.3
J5418.3810 Osteotome SCREW-LINE, angled convex	3.8
J5418.4310 Osteotome SCREW-LINE, angled convex	4.3
J5418.5010 Osteotome SCREW-LINE, angled convex	5.0
J5418.6010 Osteotome SCREW-LINE, angled convex	6.0

J5417.2800



Pre-Osteotome SCREW-LINE
straight convex

1.7-2.8 Stainless steel

J5418.3310



Osteotome SCREW-LINE
angled convex

3.3
Stainless steel

J5418.3810



3.8

J5418.4310



4.3

J5418.5010



5.0

J5418.6010



6.0



SURGERY SCREW-LINE

OSTEOTOMY SET SCREW-LINE

Art. No.

Article

∅
in mm

Material

J5420.0020



Osteotomy set CAMLOG®/CONELOG® SCREW-LINE, straight concave

Content:

J5419.2800	Pre-Osteotome SCREW-LINE, straight concave	1.7-2.8
J5420.3300	Osteotome SCREW-LINE, straight concave	3.3
J5420.3800	Osteotome SCREW-LINE, straight concave	3.8
J5420.4300	Osteotome SCREW-LINE, straight concave	4.3
J5420.5000	Osteotome SCREW-LINE, straight concave	5.0
J5420.6000	Osteotome SCREW-LINE, straight concave	6.0

J5419.2800



Pre-Osteotome SCREW-LINE
straight concave

1.7-2.8 Stainless steel

J5420.3300



Osteotome SCREW-LINE
straight concave

3.3 Stainless steel

J5420.3800



3.8

J5420.4300



4.3

J5420.5000



5.0

J5420.6000




6.0



SURGERY SCREW-LINE OSTEOTOMY SET SCREW-LINE

Art. No.	Article	Ø in mm	Material
----------	---------	------------	----------

J5420.0030

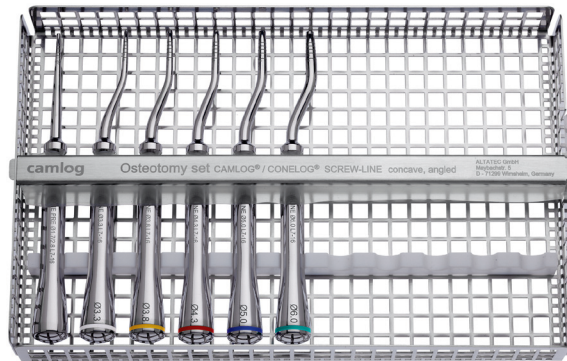

Osteotomy set CAMLOG®/CONELOG® SCREW-LINE, angled concave

Content:

J5419.2800	Pre-Osteotome SCREW-LINE, straight concave	1.7-2.8
J5420.3310	Osteotome SCREW-LINE, angled concave	3.3
J5420.3810	Osteotome SCREW-LINE, angled concave	3.8
J5420.4310	Osteotome SCREW-LINE, angled concave	4.3
J5420.5010	Osteotome SCREW-LINE, angled concave	5.0
J5420.6010	Osteotome SCREW-LINE, angled concave	6.0

J5419.2800



Pre-Osteotome SCREW-LINE
straight concave

1.7-2.8 Stainless steel

J5420.3310



Osteotome SCREW-LINE
angled concave

3.3 Stainless steel

J5420.3810



3.8

J5420.4310



4.3

J5420.5010



5.0

J5420.6010






6.0










SURGERY SCREW-LINE GUIDE SYSTEM

TEMPLATE-GUIDED IMPLANT BED PREPARATION AND IMPLANTATION

Art. No.	Article	Ø in mm	Length in mm	Material	
K1053.3311		Guide System CAMLOG® SCREW-LINE Implant, Promote® plus, incl. Guide System CAMLOG® Insertion post and CAMLOG® Cover screw	3.3	11	Titanium Grade 4
K1053.3313			3.3	13	
K1053.3316			3.3	16	
K1053.3809			3.8	9	
K1053.3811			3.8	11	
K1053.3813			3.8	13	
K1053.3816			3.8	16	
K1053.4309			4.3	9	
K1053.4311			4.3	11	
K1053.4313			4.3	13	
K1053.4316			4.3	16	












Guide System Pilotbohrer

J5043.3311		Guide System Pilot drill set, for Ø 3.3 mm, internal irrigation, sterile, Content: Guide System pilot drills Ø 2.0 mm, length 5, 9 and 11 mm	3.3	11	Stainless steel
J5043.3313		Guide System Pilot drill set, for Ø 3.3 mm, internal irrigation, sterile, Content: Guide System pilot drills Ø 2.0 mm, length 5, 9, 11 and 13 mm	3.3	13	
J5044.3316		Guide System Pilot drill, for Ø 3.3 mm, internal irrigation, sterile, Ø 2.0 mm, length 16 mm	3.3	16	
J5043.4309		Guide System Pilot drill set, for Ø 3.8/4.3 mm, internal irrigation, sterile, Content: Guide System pilot drills Ø 2.0 mm, length 5 and 9 mm	3.8	9	Stainless steel
J5043.4311		Guide System Pilot drill set, for Ø 3.8/4.3 mm, internal irrigation, sterile, Content: Guide System pilot drills Ø 2.0 mm, length 5, 9 and 11 mm	3.8	11	
J5043.4313		Guide System Pilot drill set, for Ø 3.8/4.3 mm, internal irrigation, sterile, Content: Guide System pilot drills Ø 2.0 mm, length 5, 9, 11 and 13 mm	3.8	13	
J5044.4316		Guide System Pilot drill, for Ø 3.8/4.3 mm, internal irrigation, sterile, Ø 2.0 mm, length 16 mm	3.8	16	

Note: All Guide System drills and gingiva punches are intended for single use only!

SURGERY SCREW-LINE GUIDE SYSTEM












TEMPLATE-GUIDED IMPLANT BED PREPARATION AND IMPLANTATION

Art. No.	Article	Ø in mm	Length in mm	Material
J5045.3311	 Guide System Surgery set, SCREW-LINE, Ø 3.3 mm , internal irrigation, sterile, Content: Guide System pre-drills Ø 3.3 mm, length 5 mm and Guide System form drills Ø 3.3 mm, length 9 and 11 mm	3.3	11	Stainless steel
J5045.3313	 Guide System Surgery set, SCREW-LINE, Ø 3.3 mm , internal irrigation, sterile, Content: Guide System pre-drills Ø 3.3 mm, length 5 mm and Guide System form drills Ø 3.3 mm, length 9, 11 and 13 mm	3.3	13	
J5046.3316	 Guide System Form drill, SCREW-LINE, Ø 3.3 mm , internal irrigation, sterile, length 16 mm	3.3	16	
J5045.3809	 Guide System Surgery set, SCREW-LINE, Ø 3.8 mm , internal irrigation, sterile, Content: Guide System pre-drills Ø 3.8 mm, length 5 mm and Guide System form drills Ø 3.8 mm, length 9 mm	3.8	9	Stainless steel
J5045.3811	 Guide System Surgery set, SCREW-LINE, Ø 3.8 mm , internal irrigation, sterile, Content: Guide System pre-drills Ø 3.8 mm, length 5 mm and Guide System form drills Ø 3.8 mm, length 9 and 11 mm	3.8	11	
J5045.3813	 Guide System Surgery set, SCREW-LINE, Ø 3.8 mm , internal irrigation, sterile, Content: Guide System pre-drills Ø 3.8 mm, length 5 mm and Guide System form drills Ø 3.8 mm, length 9, 11 and 13 mm	3.8	13	
J5046.3816	 Guide System Form drill, SCREW-LINE, Ø 3.8 mm , internal irrigation, sterile, length 16 mm	3.8	16	
J5045.4309	 Guide System Surgery set, SCREW-LINE, Ø 4.3 mm , internal irrigation, sterile, Content: Guide System pre-drills Ø 4.3 mm, length 5 mm and Guide System form drills Ø 4.3 mm, length 9 mm	4.3	9	Stainless steel
J5045.4311	 Guide System Surgery set, SCREW-LINE, Ø 4.3 mm , internal irrigation, sterile, Content: Guide System pre-drills Ø 4.3 mm, length 5 mm and Guide System form drills Ø 4.3 mm, length 9 and 11 mm	4.3	11	
J5045.4313	 Guide System Surgery set, SCREW-LINE, Ø 4.3 mm , internal irrigation, sterile, Content: Guide System pre-drills Ø 4.3 mm, length 5 mm and Guide System form drills Ø 4.3 mm, length 9, 11 and 13 mm	4.3	13	
J5046.4316	 Guide System Form drill, SCREW-LINE, Ø 4.3 mm , internal irrigation, sterile, length 16 mm	4.3	16	




Note: All Guide System drills and gingiva punches are intended for single use only!

SURGERY SCREW-LINE GUIDE SYSTEM

TEMPLATE-GUIDED IMPLANT BED PREPARATION AND IMPLANTATION




Art. No.	Article	Ø in mm	Length in mm	Material
Guide System Form Drills Cortical Bone				
J5048.3311	 Guide System Form drill, SCREW-LINE, Cortical bone, internal irrigation, sterile	3.3	11	Stainless steel
J5048.3313		3.3	13	
J5048.3316		3.3	16	
J5048.3809		3.8	9	
J5048.3811		3.8	11	
J5048.3813		3.8	13	
J5048.3816		3.8	16	
J5048.4309		4.3	9	
J5048.4311		4.3	11	
J5048.4313		4.3	13	
J5048.4316		4.3	16	

Guide System Gingiva punches, sterile

J5041.3300	 Ø 3.3	3.3	Stainless steel
J5041.3800	 Ø 3.8	3.8	
J5041.4300	 Ø 4.3	4.3	













Note: All Guide System drills and gingiva punches are intended for single use only!

Guide System Guiding sleeves, height 3.0 mm (2 units)

J3714.3303		3.3	Stainless steel
J3714.3803		3.8	
J3714.4303		4.3	







SURGERY SCREW-LINE GUIDE SYSTEM

TEMPLATE-GUIDED IMPLANT BED PREPARATION AND IMPLANTATION

Art. No.	Article	∅ in mm	Length in mm	Material
Guide System Insertion Posts				
K2026.3300	 Guide System CAMLOG® Insertion post, for CAMLOG® Lab analogs, incl. fixing screw (2 units)	3.3		Titanium alloy
K2026.3800		3.8		
K2026.4300		4.3		
Guide System Instruments				
J3713.3300	 Guide System Template drill, for Guide System Guiding sleeve	3.3		Stainless steel
J3713.4300		3.8		
		4.3		
J3716.3300	 Guide System Seating tool, for Guide System Guiding sleeve	3.3		Stainless steel
J3716.4300		3.8		
		4.3		
J5301.3300	 Guide System Check-up pin, for Guide System Guiding sleeve	3.3		Stainless steel
J5301.4300		3.8		
		4.3		
J5303.4300	 Guide System Driver, for Guide System Implant ∅ 3.3/3.8/4.3 mm, manual/wrench	3.3		Stainless steel
		3.8		
		4.3		
J5304.4300	 Guide System Driver, for Guide System Implant ∅ 3.3/3.8/4.3 mm, with ISO shaft for angled hand piece	3.3		
		3.8		
		4.3		
J5002.0005	 Drill extension ISO shaft, for drills with internal irrigation		26.6	Stainless steel

SURGERY ROOT-LINE 2

CAMLOG® ROOT-LINE 2 IMPLANTS

Art. No.	Article	Ø in mm	Length in mm	Material
K1032.3311	 CAMLOG® ROOT-LINE 2 Implant, Promote® plus incl. insertion post and cover screw, sterile	3.3	11	Titanium alloy
K1032.3313			13	
K1032.3316			16	
K1032.3809			9	
K1032.3811	 	3.8	11	
K1032.3813			13	
K1032.3816			16	
K1032.4309			9	
K1032.4311		4.3	11	
K1032.4313			13	
K1032.4316			16	
K1032.5009			9	
K1032.5011		5.0	11	
K1032.5013			13	
K1032.5016			16	
K1032.6009			9	
K1032.6011		6.0	11	
K1032.6013			13	
K1032.6016			16	

Note: With CAMLOG® ROOT-LINE 2 Implants with diameter 3.8/4.3/5.0/6.0 mm the option of Platform Switching is possible. See also information on page 6.

SURGERY ROOT-LINE 2

SURGERY SET ROOT-LINE 2

Art. No.


Article

J5300.0059

Surgery set

CAMLOG® ROOT-LINE 2

Contains all necessary color-code ordered surgical instruments, incl. torque wrench and holding key for insertion post (drills and taps for \varnothing 6.0 mm are not included)

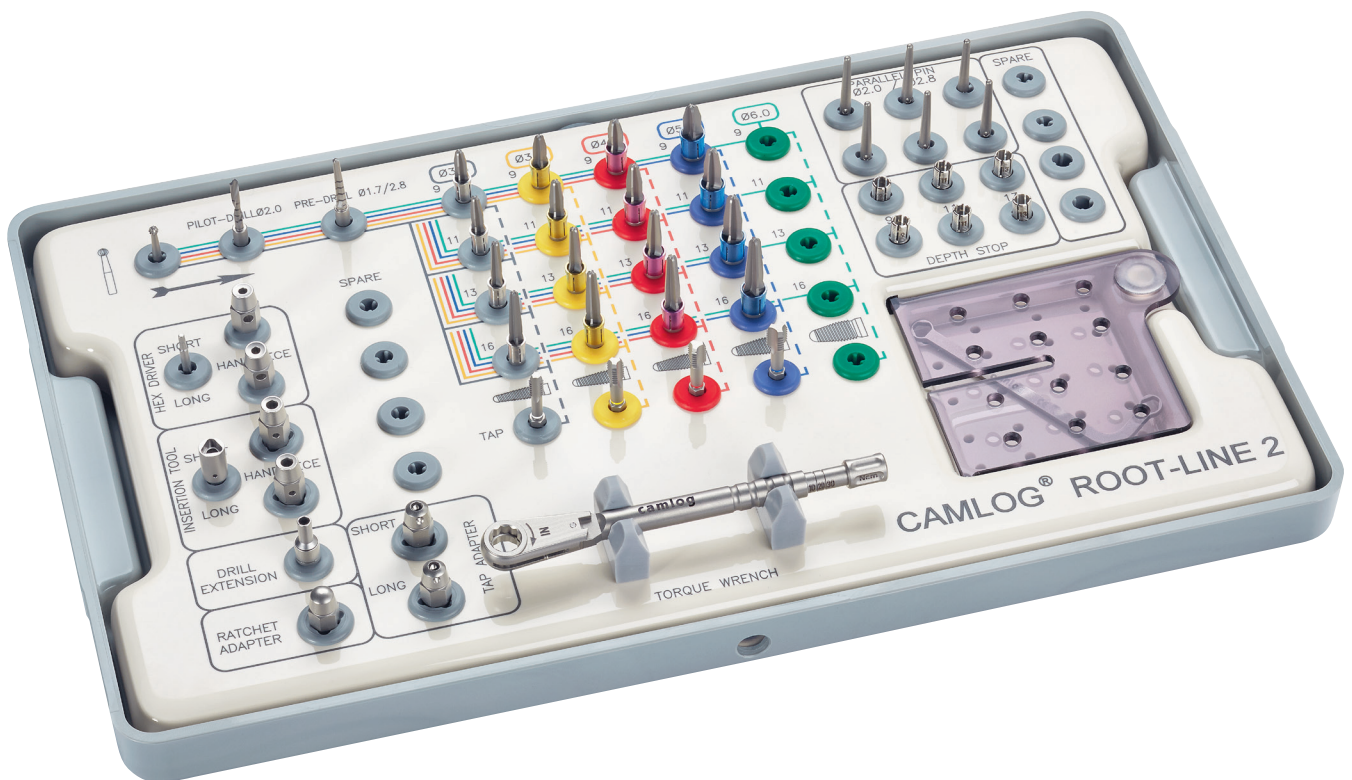









J5300.8915

Surgery tray CAMLOG® ROOT-LINE 2
without content

SURGERY ROOT-LINE 2

SURGICAL INSTRUMENTS ROOT-LINE 2
















Art. No.		Article	∅ in mm	Length in mm	Material
J5050.2300*		Round bur resterilizable	2.3	–	Stainless steel
J5050.3500		Round bur resterilizable	3.5	–	Stainless steel
J5051.2003		Pilot drill without coil, resterilizable	2.0	–	Stainless steel
J5051.2000*		Pilot drill SCREW-LINE** reduced coil, resterilizable	2.0	–	Stainless steel
J5051.2800*		Pre-drill SCREW-LINE** resterilizable	1.7-2.8	–	Stainless steel
J5015.0009*		Depth stop SCREW-LINE** for pilot drill (J5051.2000) and pre-drill (J5051.2800), resterilizable	–	9	Stainless steel
J5015.0011*			–	11	
J5015.0013*			–	13	

* The instruments listed above are also included in the surgery set CAMLOG® ROOT-LINE 2

** Can also be used for the preparation of the implant bed for CAMLOG® ROOT-LINE 2 implants

SURGERY ROOT-LINE 2

SURGICAL INSTRUMENTS ROOT-LINE 2


Art. No.	Image	Article	∅ in mm	Length in mm	Material
J5055.3309 J5055.3311 J5055.3313 J5055.3316		Form drill ROOT-LINE 2 with reduced coil, resterilizable	3.3	9	Stainless steel
	11				
	13				
	16				
J5055.3809 J5055.3811 J5055.3813 J5055.3816			3.8	9	
	11				
	13				
	16				
J5055.4309 J5055.4311 J5055.4313 J5055.4316			4.3	9	
	11				
	13				
	16				
J5055.5009 J5055.5011 J5055.5013 J5055.5016			5.0	9	
	11				
	13				
	16				
J5055.6009 J5055.6011 J5055.6013 J5055.6016			6.0	9	
	11				
	13				
	16				
J5015.3300		Depth stop for form drill SCREW-LINE and ROOT-LINE 2 with reduced coil, resterilizable	3.3	–	Titanium alloy
J5015.3800				–	
J5015.4300				–	
J5015.5000				–	
J5015.6000				–	
J5056.3309		Tap ROOT-LINE 2 with hexagon, resterilizable	3.3	–	Stainless steel
J5056.3809				–	
J5056.4309				–	
J5056.5009				–	
J5056.6009				–	

The instruments listed above are also included in the surgery set CAMLOG® ROOT-LINE 2 (drills and taps for ∅ 6.0 mm are not included).

SURGERY


CAMLOG® HEALING CAPS

CAMLOG® Healing cap, cylindrical, titanium alloy, sterile


		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm
GH 	GH 2.0	J2015.3320	J2015.3820	J2015.4320	J2015.5020	J2015.6020
	GH 4.0	J2015.3340	J2015.3840	J2015.4340	J2015.5040	J2015.6040
	GH 6.0		J2015.3860*	J2015.4360*	J2015.5060*	J2015.6060*

* Suitable for bite registration.

CAMLOG® Healing cap, wide body, titanium alloy, sterile


		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm
GH 	GH 2.0	J2014.3320	J2014.3820	J2014.4320	J2014.5020	J2014.6020
	GH 4.0	J2014.3340	J2014.3840	J2014.4340	J2014.5040	J2014.6040
	GH 6.0		J2014.3860	J2014.4360	J2014.5060	J2014.6060

CAMLOG® Healing cap, bottleneck, titanium alloy, sterile

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm
GH 	GH 4.0	J2011.3340	J2011.3840	J2011.4340	J2011.5040	J2011.6040
	GH 6.0		J2011.3860	J2011.4360	J2011.5060	J2011.6060




CAMLOG® Healing cap PS, cylindrical, titanium alloy, sterile, for Platform Switching with CAMLOG® Implants with K article number

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm
GH 	GH 2.0		K2005.3820	K2005.4320	K2005.5020	K2005.6020
	GH 4.0		K2005.3840	K2005.4340	K2005.5040	K2005.6040
	GH 6.0		K2005.3860*	K2005.4360*	K2005.5060*	K2005.6060*

* Suitable for bite registration.




CAMLOG® Healing cap PS, wide body, titanium alloy, sterile, for Platform Switching with CAMLOG® Implants with K article number

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm
GH 	GH 4.0		K2004.3840	K2004.4340	K2004.5040	K2004.6040
	GH 6.0		K2004.3860	K2004.4360	K2004.5060	K2004.6060













CAMLOG® Healing cap PS, bottleneck, titanium alloy, sterile, for Platform Switching with CAMLOG® Implants with K article number

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm
GH 	GH 4.0		K2001.3840	K2001.4340	K2001.5040	K2001.6040
	GH 6.0		K2001.3860	K2001.4360	K2001.5060	K2001.6060

H: height in mm, Ø = implant diameter, GH = gingiva height in mm








SURGERY

ALTAPIN SET

Art. No.	Article	Material
M5600.0110	ALTApin set Membrane fixation system, resterilizable Content: M5100.0010 ALTApin applicator, straight M5100.0050 ALTApin pricker (holder) M5100.0070 ALTApin membrane fixator M5200.0055 ALTApin pricker, insert, 2 units M1000.0050 ALTApin magazine, 7 Titanium pins, sterile, 4 units	Plastic/ Titanium alloy/ Stainless steel
		
M5600.0210	ALTApin-Tray (without content)	Plastic
M5100.0010	ALTApin applicator, straight incl. activator	Stainless steel
		
M5100.0030	ALTApin applicator, angled 90° incl. activator	Stainless steel
		
M5200.0010	ALTApin applicator, straight, work element incl. activator	Stainless steel
		
M5100.0050	ALTApin pricker	Stainless steel
		
M5100.0070	ALTApin membrane fixator	Stainless steel
		
M5100.0100	ALTApin surgery mallet	Stainless steel
		
M5500.0050	ALTApin single patient drill, ISO shaft	Stainless steel
		
M5200.0055	ALTApin pricker, insert	Stainless steel
		
M1000.0050	ALTApin magazine 7 titanium pins, sterile, 1 unit	Titanium alloy
		
M1000.0100	ALTApin magazine 7 titanium pins, sterile, 3 units	Titanium alloy

SURGERY







SURGICAL INSTRUMENTS

Art. No.		Article	Dimension in mm	Material
J5300.2028		Paralleling pin SCREW-LINE*, with depth marks	∅ 1.7-2.8/ 2.0	Titanium alloy
J5002.0006		Drill extension ISO shaft	26.5	Stainless steel
J5322.0010		Tap adapter, short for tap SCREW-LINE*	18.0	Stainless steel
J5322.0011		Tap adapter, long for tap SCREW-LINE*	23.0	Stainless steel
J5300.0007		Driver for screw implants, with ISO shaft for angled hand piece	27.5	Stainless steel
J5300.0008		Driver, short for screw implants, manual/wrench, with borehole for screwdriver, hex, long	18.0	Stainless steel
J5300.0009		Driver, long for screw implants, manual/wrench	27.0	Stainless steel

*Can also be used for ROOT-LINE 2.








SURGERY

SURGICAL INSTRUMENTS

Art. No.	Article	Dimension in mm	Material
J5300.0010	Cardanic driver (30°) for screw implants, adjustable length	–	Stainless steel
			
J5300.0030	PickUp instrument holder for carrying implants	–	Stainless steel
			
J5002.0011	Adapter ISO shaft for angled hand piece	21.0	Stainless steel
			
J5302.0010	Holding key for insertion post	–	Stainless steel
			
K5302.3310	Adapter for screw implants, long for CAMLOG® SCREW-LINE and ROOT-LINE 2 Implants	3.3	Stainless steel
K5302.3810		3.8	
K5302.4310		4.3	
J5302.3300	Holding sleeve for screw implants color-coded	3.3	Titanium alloy
J5302.3800		3.8	
J5302.4300		4.3	
J5002.0012	Cleaning needle for drills with internal irrigation		Stainless steel
			
J5002.0020	Cleaning cannula for drills with internal irrigation		Stainless steel
			











SURGERY

SURGICAL-PROSTHETIC INSTRUMENTS

Art. No.	Article	Length in mm	Material
J5330.8600	Prosthetic set Content: J5320.1030 Torque wrench Screwdriver: J5316.0501 hex, short, manual/wrench J5316.0502 hex, long, manual/wrench J5316.0503 hex, long, ISO shaft J5316.0504 hex, short, ISO shaft	Plastic/ Stainless steel	
			
J5330.8500	Prosthetic tray (without content)		Plastic
J5316.0510		Screwdriver hex, extra short, manual/wrench	14.5 Stainless steel
J5316.0501		Screwdriver hex, short, manual/wrench	22.5 Stainless steel
J5316.0502		Screwdriver hex, long, manual/wrench	30.3 Stainless steel
J5316.0504		Screwdriver hex, short, ISO shaft	18.0 Stainless steel
J5316.0503		Screwdriver hex, long, ISO shaft	26.0 Stainless steel
J5320.1030	Torque wrench with continuous torque adjustment until maximal 30 Ncm	–	Stainless steel
			

SURGERY














PROSTHETIC INSTRUMENTS

Art. No.		Article	Length in mm	Material
J5300.0011		Driver for ball abutment, manual/wrench	18.3	Stainless steel
J5315.0005		Screwdriver Activator for ball abutment matrix CM Dalbo®-Plus	–	Stainless steel
J5300.0020		Driver for bar abutment Ø 3.3/3.8/4.3 mm	18.6	Stainless steel
J5300.0025		Driver for bar abutment Ø 5.0/6.0 mm	18.6	Stainless steel
J5300.0027		Driver for impression post and healing cap for bar abutment Ø 3.3/3.8/4.3 mm	19.1	Stainless steel
J5300.0028		Driver for impression post and healing cap for bar abutment Ø 5.0/6.0 mm	19.1	Stainless steel
J2253.0001		Driver for Locator®, manual/wrench	24.3	Stainless steel
J2253.0002		Locator® Instrument threepart	83.0	Stainless steel
J2253.0003		Locator® Angle measurement guide	–	Stainless steel
J2253.0004		Locator® Parallel post (4 units)	–	Nylon

CAMLOG® PROSTHETICS	41
PROSTHETICS OVERVIEW	42
TORQUE WRENCH SETTINGS	48
IMPRESSION TAKING, BITE REGISTRATION, FABRICATION OF THE PLASTER MODEL	50
IMPRESSION TAKING, CLOSED/OPEN TRAY	50
BITE REGISTRATION	51
FABRICATION OF THE PLASTER MODEL	51
CROWN AND BRIDGE RESTORATIONS	52
CAMLOG® TEMPORARY ABUTMENTS	52
CAMLOG® ESTHOMIC® ABUTMENTS	52
CAMLOG® UNIVERSAL ABUTMENTS	55
CAMLOG® GOLD-PLASTIC ABUTMENTS	55
CAMLOG® CERAMIC ABUTMENTS	55
CAMLOG® LOGFIT® PROSTHETIC SYSTEM	56
CROWN, BRIDGE AND HYBRID RESTORATIONS	57
CAMLOG® TITANIUM BASES CAD/CAM	57
ACCESSORIES FOR CAMLOG® ABUTMENTS	58
CAMLOG® VARIO SR ABUTMENTS	59
ACCESSORIES FOR VARIO SR	60
HYBRID RESTORATIONS	62
BAR RESTORATIONS	62
BALL ABUTMENT ANCHORING SYSTEM	64
LOCATOR® ANCHORING SYSTEM	66
DOUBLE CROWN RESTORATIONS WITH CAMLOG®	
UNIVERSAL AND TELESCOPE ABUTMENTS	69
ACCESSORIES FOR CAMLOG® ABUTMENTS	69
INSTRUMENTS FOR DENTAL TECHNICIANS	70
CAMLOG® SELECTION ABUTMENTS	72

CAMLOG® PROSTHETICS















PROSTHETICS OVERVIEW

Article		GH in mm	∅ 3.3 mm	∅ 3.8 mm	∅ 4.3 mm	∅ 5.0 mm	∅ 6.0 mm	
Impression takings	CAMLOG® Impression posts, open tray			K2121.3300	K2121.3800	K2121.4300	K2121.5000	K2121.6000
	CAMLOG® Impression posts, closed tray			K2110.3300	K2110.3800	K2110.4300	K2110.5000	K2110.6000
	CAMLOG® Impression posts PS, open tray, for Platform Switching with CAMLOG® Implants with Article No. K		–	K2119.3800	K2119.4300	K2119.5000	K2119.6000	
	CAMLOG® Impression posts PS, closed tray, for Platform Switching with CAMLOG® Implants with Article No. K		–	K2109.3800	K2109.4300	K2109.5000	K2109.6000	
	Impression caps for impression posts, closed tray		J2111.3300	J2111.3800	J2111.4300	J2111.5000	J2111.6000	
Bite registration	CAMLOG® Bite registration posts, incl. bite registration caps		J2140.3300	J2140.3800	J2140.4300	J2140.5000	J2140.6000	
Fabrication of the plaster model	CAMLOG® Lab analogs for CAMLOG® Abutments		K3010.3300	K3010.3800	K3010.4300	K3010.5000	K3010.6000	
Abutments for crown and bridge restorations	CAMLOG® Temporary abutments		–	K2241.3800	K2241.4300	K2241.5000	K2241.6000	
	 CAMLOG® Temporary abutment PS, for Platform Switching with CAMLOG® Implants with Article No. K		–	K2208.3800	K2208.4300	K2208.5000	K2208.6000	
	CAMLOG® Esthomic® Abutments, straight		1.0-1.8 3.0-4.5	–	K2226.3810 K2226.3830	K2226.4310 K2226.4330	K2226.5010 K2226.5030	K2226.6010 K2226.6030
	CAMLOG® Esthomic® Abutments, 15° angled, type A		1.0-1.8 3.0-4.5	–	K2227.3810 K2227.3830	K2227.4310 K2227.4330	K2227.5010 K2227.5030	K2227.6010 K2227.6030

GH: gingiva height

CAMLOG® PROSTHETICS













PROSTHETICS OVERVIEW

Article		GH in mm	∅ 3.3 mm	∅ 3.8 mm	∅ 4.3 mm	∅ 5.0 mm	∅ 6.0 mm
Abutments für crown and bridge restorations	CAMLOG® Esthomic® Abutments, 15° angled, type B	 1.0-1.8 3.0-4.5	–	K2228.3810 K2228.3830	K2228.4310 K2228.4330	K2228.5010 K2228.5030	K2228.6010 K2228.6030
	CAMLOG® Esthomic® Abutments, 20° angled, type A	 1.0-1.8 3.0-4.5	–	K2231.3810 K2231.3830	K2231.4310 K2231.4330	K2231.5010 K2231.5030	K2231.6010 K2231.6030
	CAMLOG® Esthomic® Abutments, 20° angled, type B	 1.0-1.8 3.0-4.5	–	K2232.3810 K2232.3830	K2232.4310 K2232.4330	K2232.5010 K2232.5030	K2232.6010 K2232.6030
	CAMLOG® Esthomic® Abutment PS, straight, for Platform Switching with CAMLOG® Implants with Article No. K	 1.5-2.5	–	K2202.3815	K2202.4315	K2202.5015	K2202.6015
	CAMLOG® Esthomic® Abutment PS, 15° angled, type A, for Platform Switching with CAMLOG® Implants with Article No. K	 1.5-2.5	–	K2203.3815	K2203.4315	K2203.5015	K2203.6015
	CAMLOG® Esthomic® Abutment PS, 15° angled, type B, for Platform Switching with CAMLOG® Implants with Article No. K	 1.5-2.5	–	K2204.3815	K2204.4315	K2204.5015	K2204.6015
	CAMLOG® Esthomic® Abutments, Inset	 1.5-2.8	K2235.3315	K2235.3815	K2235.4315	K2235.5015	K2235.6015
	CAMLOG® Universal abutments		K2211.3300	K2211.3800	K2211.4300	K2211.5000	K2211.6000
	CAMLOG® Universal abutment PS, for Platform Switching with CAMLOG® Implants with Article No. K	 PS	–	K2201.3800	K2201.4300	K2201.5000	K2201.6000
	CAMLOG® Gold-plastic abutments		K2246.3300	K2246.3800	K2246.4300	K2246.5000	K2246.6000

GH: gingiva height

CAMLOG® PROSTHETICS













PROSTHETICS OVERVIEW

Article		GH in mm	∅ 3.3 mm	∅ 3.8 mm	∅ 4.3 mm	∅ 5.0 mm	∅ 6.0 mm	
Abutments für crown and bridge restorations	CAMLOG® Titanium bases CAD/CAM			K2244.3348	K2244.3848	K2244.4348	K2244.5048	K2244.6048
	CAMLOG® Ceramic abutments			K2242.3340	K2242.3840	K2242.4340	K2242.5040	K2242.6040
	CAMLOG® Logfit® Abutments	 0.8 1.5	–	K2550.3808 K2550.3815	K2550.4308 K2550.4315	K2550.5008 K2550.5015	K2550.6008 K2550.6015	
	Logfit® Impression caps			–	J2551.4300	J2551.4300	J2551.6000	J2551.6000
	Logfit® Analogs			–	J2552.4300	J2552.4300	J2552.6000	J2552.6000
	Logfit® Plastic copings, for crowns			–	J2553.4302	J2553.4302	J2553.6002	J2553.6002
	Logfit® Plastic copings, for bridge			–	J2553.4301	J2553.4301	J2553.6001	J2553.6001
Abutments for crowns, bridges and hybrid restorations	CAMLOG® Vario SR abutments, straight	 0.8	–	K2560.3808	K2560.4308	K2560.5008	K2560.6008	
	CAMLOG® Vario SR abutments, 20° angled		–	K2561.3800	K2561.4300	K2561.5000	K2561.6000	
	CAMLOG® Vario SR abutments, 30° angled		–	K2562.3800	K2562.4300	K2562.5000	K2562.6000	
	Vario SR impression caps, open tray			–	J2566.4300	J2566.4300	J2566.6000	J2566.6000
	Vario SR impression caps, closed tray			–	J2565.4300	J2565.4300	J2565.6000	J2565.6000
	Vario SR analogs			–	J2567.4300	J2567.4300	J2567.6000	J2567.6000

GH: gingiva height

CAMLOG® PROSTHETICS










PROSTHETICS OVERVIEW

Article		GH in mm	∅ 3.3 mm	∅ 3.8 mm	∅ 4.3 mm	∅ 5.0 mm	∅ 6.0 mm
Vario SR plastic copings, crown, with triple-surface antirotation		–	J2563.4302	J2563.4302	J2563.6002	J2563.6002	J2563.6002
Vario SR plastic copings, bridge		–	J2563.4301	J2563.4301	J2563.6001	J2563.6001	J2563.6001
Vario SR plastic copings, crown, with single-surface antirotation for angled Vario SR abutments		–	J2563.4303	J2563.4303	J2563.6003	J2563.6003	J2563.6003
Vario SR titanium caps, bridge		–	J2564.4301	J2564.4301	J2564.6001	J2564.6001	J2564.6001
Vario SR bases for bar		–	J2570.4300	J2570.4300	J2570.6000	J2570.6000	J2570.6000
Abutments for hybrid restorations	CAMLOG® Bar abutments 	0.5	J2255.3305	J2255.3805	J2255.4305	J2255.5005	J2255.6005
		2.0	J2255.3320	J2255.3820	J2255.4320	J2255.5020	J2255.6020
		4.0		J2255.3840	J2255.4340	J2255.5040	J2255.6040
Impression post for bar abutments			J2130.4300	J2130.4300	J2130.4300	J2130.6000	J2130.6000
Healing caps for bar abutments			J2030.4300	J2030.4300	J2030.4300	J2030.6000	J2030.6000
Lab analogs/ Soldering aids for bar abutments			J3020.4300	J3020.4300	J3020.4300	J3020.6000	J3020.6000
Bases for bar abutments, plastic, burn-out			J2257.3300	J2257.3800	J2257.4300	J2257.5000	J2257.6000
Bases for bar abutments, cast-on			J2263.4300	J2263.4300	J2263.4300	J2263.6000	J2263.6000
Bases for bar abutments, solderable			J2258.4300	J2258.4300	J2258.4300	J2258.6000	J2258.6000

GH: gingiva height

CAMLOG® PROSTHETICS









PROSTHETICS OVERVIEW

Article			GH in mm	∅ 3.3 mm	∅ 3.8 mm	∅ 4.3 mm	∅ 5.0 mm	∅ 6.0 mm
Abutments for hybrid restorations	Bases for bar abutments, Titanium, laser-weldable			J2262.4300	J2262.4300	J2262.4300	J2262.6000	J2262.6000
	Titanium bonding bases for bar abutments			J2260.3300	J2260.3800	J2260.4300	J2260.5000	J2260.6000
	Sleeves for titanium bonding bases			J2261.3300	J2261.3800	J2261.4300	J2261.5000	J2261.6000
CAMLOG® Ball abutment sets, incl. male part and matrix CM Dalbo®-Plus		1.5	J2250.3315	J2250.3815	J2250.4315	J2250.5015	–	
		3.0	J2250.3330	J2250.3830	J2250.4330	J2250.5030	–	
		4.5		J2250.3845	J2250.4345	J2250.5045	–	
CAMLOG® Ball abutments, male part		1.5	J2249.3315	J2249.3815	J2249.4315	J2249.5015	–	
		3.0	J2249.3330	J2249.3830	J2249.4330	J2249.5030	–	
		4.5		J2249.3845	J2249.4345	J2249.5045	–	
Ball abutments lab analog			J3015.3300	J3015.3800	J3015.4300	J3015.5000	–	
CAMLOG® Locator® Abutments		1.0	J2253.3310	J2253.3810	J2253.4310	J2253.5010	–	
		2.0	J2253.3320	J2253.3820	J2253.4320	J2253.5020	–	
		3.0	J2253.3330	J2253.3830	J2253.4330	J2253.5030	–	
		4.0	J2253.3340	J2253.3840	J2253.4340	J2253.5040	–	
		5.0		J2253.3850	J2253.4350	J2253.5050	–	
Locator® Impression caps			J2253.0200	J2253.0200	J2253.0200	J2253.0200	–	
Locator® Analogs			J2253.0340	J2253.0340	J2253.0340	J2253.0350	–	

GH: gingiva height

CAMLOG® PROSTHETICS

PROSTHETICS OVERVIEW

Article		∅ 3.3 mm	∅ 3.8 mm	∅ 4.3 mm	∅ 5.0 mm	∅ 6.0 mm
Abutments for hybrid restorations	Locator® Male processing packages 	J2253.0102	J2253.0102	J2253.0102	J2253.0102	–
	Locator® Male processing packages, for extended range 	–	J2253.0112	J2253.0112	J2253.0112	–
	CAMLOG® Universal abutments 	–	K2211.3800	K2211.4300	K2211.5000	K2211.6000
	 CAMLOG® Universal abutment PS, for Platform Switching with CAMLOG® Implants with Article No. K 	–	K2201.3800	K2201.4300	K2201.5000	K2201.6000
	CAMLOG® Telescope abutments for double crown restorations 	–	K2212.3800	K2212.4300	K2212.5000	K2212.6000
CAD/CAM PROSTHETICS	CAMLOG® Scanbody 	K2610.3310	K2610.3810	K2610.4310	K2610.6010	K2610.6010
	CAMLOG® ScanPosts 	K2620.3306	K2620.3806	K2620.4306	K2620.5006	K2620.6006

CAMLOG® PROSTHETICS TORQUE WRENCH SETTINGS

FOR FINAL FIXATION OF SURGICAL COMPONENTS AND SUPRASTRUCTURES

Article



CAMLOG® Implant cover screw



CAMLOG® Healing caps (incl. PS)
cylindrical
wide body
bottleneck



CAMLOG® Impression posts (incl. PS)
CAMLOG® Bite registration post



CAMLOG® Lab screws

J4006.1601
(∅ 3.3/3.8/4.3 mm)



J4006.2001
(∅ 5.0/6.0 mm)



CAMLOG® Vario SR lab screws

J4008.1600
(∅ 3.8/4.3 mm)



J4008.2000
(∅ 5.0/6.0 mm)



**CAMLOG®
Temporary abutment (incl. PS)**



CAMLOG® Abutment screws

J4005.1601
(∅ 3.3/3.8/4.3 mm)



J4005.2001
(∅ 5.0/6.0 mm)



CAMLOG® Vario SR abutment screws


J4007.1600
(∅ 3.8/4.3 mm)



J4007.2000
(∅ 5.0/6.0 mm)



**CAMLOG® Esthomic® Abutment,
straight (incl. PS)**
**CAMLOG® Esthomic® Abutment,
angled 15°/20° (incl. PS)**
CAMLOG® Esthomic® Abutment, Inset



CAMLOG® Gold-plastic abutment
CAMLOG® Universal abutment
CAMLOG® Telescope abutment
CAMLOG® Ceramic abutment



CAMLOG® Logfit® Abutments
CAMLOG® Titanium bases CAD/CAM



(from left to right)

**CAMLOG® Vario SR abutments,
straight, 20°/30° angled**



Vario SR protection caps



Vario SR prosthetic screw


J4005.2004
(∅ 3.8/4.3/5.0/6.0 mm)



Vario SR
Plastic copings/titanium
caps/bases for bar



Tightening torque
tightened by hand



20 Ncm





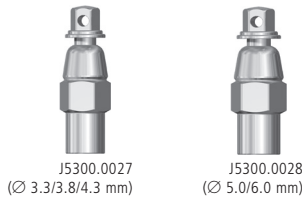











tightened by hand

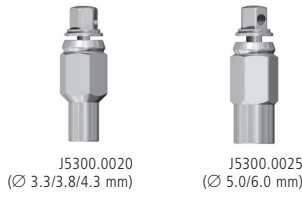15 Ncm

All screws have to be retighten after at least 5 minutes with the corresponding torque!

CAMLOG® PROSTHETICS TORQUE WRENCH SETTINGS

FOR FINAL FIXATION OF SURGICAL COMPONENTS AND SUPRASTRUCTURES






Article			
		Tightening torque in mm ^Ø	
CAMLOG® Bar abutments			20 Ncm 3.3
			30 Ncm 3.8 4.3 5.0 6.0
Healing cap for bar abutment			tightened by hand
Prosthetic screws	J4005.1602 (Ø 3.3/3.8/4.3 mm)  J4005.2002 (Ø 5.0/6.0 mm) 		15 Ncm
Bases for bar abutments Titanium bonding bases for bar abutments			
CAMLOG® Ball abutments			20 Ncm 3.3 30 Ncm 3.8 4.3 5.0
CAMLOG® Locator® Abutments			20 Ncm 3.3 30 Ncm 3.8 4.3 5.0
CAMLOG® Scanbodies			tightened by hand
CAMLOG® ScanPosts			






All screws have to be retighten after at least 5 minutes with the corresponding torque!





CAMLOG® PROSTHETICS





IMPRESSION TAKING, BITE REGISTRATION, FABRICATION OF THE PLASTER MODEL

IMPRESSION TAKING

Art. No.	Article	∅ in mm	Dimension in mm	Material
CAMLOG® Impression posts, open tray, incl. fixing screw (The fixing screw can be shortened extra-oral by 3 mm with a screwdriver, hex.)				
K2121.3300		3.3	21.0/24.0	Titanium alloy
K2121.3800		3.8	21.0/24.0	
K2121.4300		4.3	21.0/24.0	
K2121.5000		5.0	21.0/24.0	
K2121.6000		6.0	21.0/24.0	

CAMLOG® Impression posts, closed tray, incl. impression cap, bite registration cap and fixing screw				
K2110.3300		3.3	–	Titanium alloy
K2110.3800		3.8	–	
K2110.4300		4.3	–	
K2110.5000		5.0	–	
K2110.6000		6.0	–	

CAMLOG® Impression posts PS, open tray, for Platform Switching, incl. fixing screw (The fixing screw can be shortened extra-oral by 3 mm with a screwdriver, hex)				
K2119.3800		3.8	21.0/24.0	Titanium alloy
K2119.4300		4.3	21.0/24.0	
K2119.5000		5.0	21.0/24.0	
K2119.6000		6.0	21.0/24.0	


CAMLOG® Impression posts PS, closed tray, for Platform Switching, incl. impression cap, bite registration cap and fixing screw				
K2109.3800		3.8	–	Titanium alloy
K2109.4300		4.3	–	
K2109.5000		5.0	–	
K2109.6000		6.0	–	

Note: CAMLOG® Impression posts PS should only be used for impression taking of CAMLOG® Implants with K article number!

H: height in mm


IMPRESSION TAKING, BITE REGISTRATION, FABRICATION OF THE PLASTER MODEL

IMPRESSION TAKING


Art. No.	Article	∅ in mm	Dimension in mm	Material
Impression caps for impression post, closed tray (5 units)				
J2111.3300		3.3	–	POM
J2111.3800		3.8	–	
J2111.4300		4.3	–	
J2111.5000		5.0	–	
J2111.6000		6.0	–	

BITE REGISTRATION

CAMLOG® Bite registration posts, incl. fixing screw and bite registration cap (also for Platform Switching)


J2140.3300		3.3	–	Titanium alloy/POM
J2140.3800		3.8	–	
J2140.4300		4.3	–	
J2140.5000		5.0	–	
J2140.6000		6.0	–	

Bite registration caps (5 units)

J2112.3300		3.3	–	POM
J2112.3800		3.8	–	
J2112.4300		4.3	–	
J2112.5000		5.0	–	
J2112.6000		6.0	–	

FABRICATION OF THE PLASTER MODEL

CAMLOG® Lab analogs


K3010.3300		3.3	–	Titanium alloy
K3010.3800		3.8	–	
K3010.4300		4.3	–	
K3010.5000		5.0	–	
K3010.6000		6.0	–	

POM: Polyoxymethylene
H: height in mm


CAMLOG® PROSTHETICS

CROWN AND BRIDGE RESTORATIONS

TEMPORARY RESTORATION

Art. No.	Article	Ø in mm	GH in mm	Material
CAMLOG® Temporary abutments (PEEK) preparable, incl. CAMLOG® Abutment screw				
K2241.3800		3.8	–	PEEK
K2241.4300		4.3	–	
K2241.5000		5.0	–	
K2241.6000		6.0	–	


CAMLOG® Temporary abutments PS (PEEK), for Platform Switching, preparable, incl. CAMLOG® Abutment screw

K2208.3800		3.8	–	PEEK
K2208.4300		4.3	–	
K2208.5000		5.0	–	
K2208.6000		6.0	–	


Note: CAMLOG® Temporary abutments PS should only be used on CAMLOG® Implants with K article number!

CAMLOG® ESTHOMIC® ABUTMENTS FOR CEMENTED CROWN AND BRIDGE RESTORATIONS

CAMLOG® Esthomic® Abutments, straight, preparable, incl. CAMLOG® Abutment screw

K2226.3810		3.8	1.0-1.8	Titanium alloy
K2226.3830			3.0-4.5	
K2226.4310		4.3	1.0-1.8	
K2226.4330			3.0-4.5	
K2226.5010		5.0	1.0-1.8	
K2226.5030			3.0-4.5	
K2226.6010	6.0	1.0-1.8		
K2226.6030		3.0-4.5		

CAMLOG® Esthomic® Abutments, 15° angled, type A, preparable, incl. CAMLOG® Abutment screw

K2227.3810		3.8	1.0-1.8	Titanium alloy
K2227.3830			3.0-4.5	
K2227.4310		4.3	1.0-1.8	
K2227.4330			3.0-4.5	
K2227.5010		5.0	1.0-1.8	
K2227.5030			3.0-4.5	
K2227.6010	6.0	1.0-1.8		
K2227.6030		3.0-4.5		


GH: gingiva height


PEEK: Poly ether ether ketone
H: height in mm


CAMLOG® PROSTHETICS


CROWN AND BRIDGE RESTORATIONS

CAMLOG® ESTHOMIC® ABUTMENTS FOR CEMENTED CROWN AND BRIDGE RESTORATIONS

Art. No.	Article	\varnothing in mm	GH in mm	Material
CAMLOG® Esthomic® Abutments, 15° angled, type B, preparable, incl. CAMLOG® Abutment screw				
K2228.3810 K2228.3830		3.8	1.0-1.8	Titanium alloy
			3.0-4.5	
K2228.4310 K2228.4330		4.3	1.0-1.8	
			3.0-4.5	
K2228.5010 K2228.5030		5.0	1.0-1.8	
	3.0-4.5			
K2228.6010 K2228.6030	6.0	1.0-1.8		
		3.0-4.5		

CAMLOG® Esthomic® Abutments, 20° angled, type A, preparable, incl. CAMLOG® Abutment screw				
K2231.3810 K2231.3830		3.8	1.0-1.8	Titanium alloy
			3.0-4.5	
K2231.4310 K2231.4330		4.3	1.0-1.8	
			3.0-4.5	
K2231.5010 K2231.5030		5.0	1.0-1.8	
	3.0-4.5			
K2231.6010 K2231.6030	6.0	1.0-1.8		
		3.0-4.5		

CAMLOG® Esthomic® Abutments, 20° angled, type B, preparable, incl. CAMLOG® Abutment screw				
K2232.3810 K2232.3830		3.8	1.0-1.8	Titanium alloy
			3.0-4.5	
K2232.4310 K2232.4330		4.3	1.0-1.8	
			3.0-4.5	
K2232.5010 K2232.5030		5.0	1.0-1.8	
	3.0-4.5			
K2232.6010 K2232.6030	6.0	1.0-1.8		
		3.0-4.5		


CAMLOG® Esthomic® Abutments, Inset, preparable, incl. CAMLOG® Abutment screw				
K2235.3315		3.3	1.5-2.8	Titanium alloy
K2235.3815		3.8	1.5-2.8	
K2235.4315		4.3	1.5-2.8	
K2235.5015		5.0	1.5-2.8	
K2235.6015		6.0	1.5-2.8	

GH: gingiva height
H: height in mm


CAMLOG® PROSTHETICS

CROWN AND BRIDGE RESTORATIONS

CAMLOG® ESTHOMIC® ABUTMENTS PS, straight, for Platform Switching, preparable, incl. CAMLOG® Abutment screw

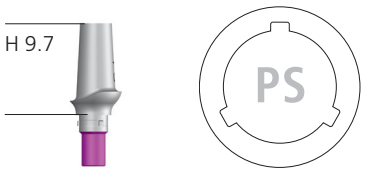Art. No.	Article	Ø in mm	GH in mm	Material
K2202.3815		3.8	1.5-2.5	Titanium alloy
K2202.4315		4.3	1.5-2.5	
K2202.5015		5.0	1.5-2.5	
K2202.6015		6.0	1.5-2.5	

CAMLOG® Esthomic® Abutments PS, 15° angled, type A, for Platform Switching, preparable, incl. CAMLOG® Abutment screw

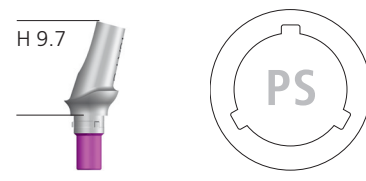K2203.3815		3.8	1.5-2.5	Titanium alloy
K2203.4315		4.3	1.5-2.5	
K2203.5015		5.0	1.5-2.5	
K2203.6015		6.0	1.5-2.5	


CAMLOG® Esthomic® Abutments PS, 15° angled, type B, for Platform Switching, preparable, incl. CAMLOG® Abutment screw

K2204.3815		3.8	1.5-2.5	Titanium alloy
K2204.4315		4.3	1.5-2.5	
K2204.5015		5.0	1.5-2.5	
K2204.6015		6.0	1.5-2.5	

Note: CAMLOG® Esthomic® Abutments PS should only be used on CAMLOG® Implants with K article number!

GH: gingiva height
H: height in mm


Specification CAMLOG® Esthomic® Abutments type A and B

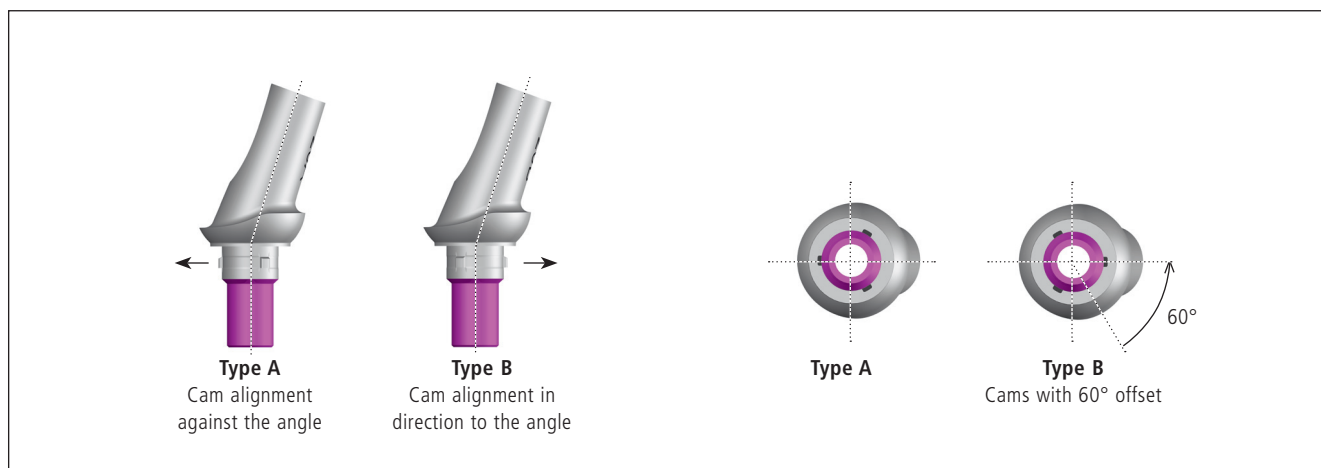


CAMLOG® PROSTHETICS

CROWN AND BRIDGE RESTORATIONS


CAMLOG® UNIVERSAL ABUTMENTS FOR CEMENTED CROWN AND BRIDGE RESTORATIONS

Art. No.	Article	Ø in mm	Dimension in mm	Material
CAMLOG® Universal abutments , preparable, incl. CAMLOG® Abutment screw				
K2211.3300		3.3*	–	Titanium alloy
K2211.3800		3.8	–	
K2211.4300		4.3	–	
K2211.5000		5.0	–	
K2211.6000		6.0	–	

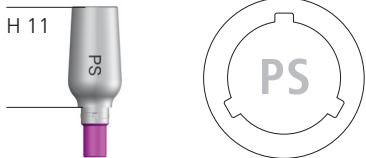CAMLOG® Universal abutments PS for Platform Switching , preparable, incl. CAMLOG® Abutment screw				
K2201.3800		3.8	–	Titanium alloy
K2201.4300		4.3	–	
K2201.5000		5.0	–	
K2201.6000		6.0	–	


Note: CAMLOG® Universal abutments PS should only be used on CAMLOG® Implants with K article number!

CAMLOG® GOLD-PLASTIC ABUTMENTS FOR CEMENTED CROWN AND BRIDGE RESTORATIONS

CAMLOG® Gold-plastic abutments , cast-on, incl. CAMLOG® Abutment screw				
K2246.3300		3.3*	0,42 g**	Cast-on gold alloy/POM
K2246.3800		3.8	0,46 g**	
K2246.4300		4.3	0,65 g**	
K2246.5000		5.0	0,81 g**	
K2246.6000		6.0	0,89 g**	

** Noble metal weight approx.

CAMLOG® CERAMIC ABUTMENTS FOR CROWN RESTORATIONS

CAMLOG® Ceramic abutments, 2-parts, for bonded/cemented full ceramic crowns preparable, incl. CAMLOG® Titanium base, zirconium oxide sleeve and CAMLOG® Abutment screw				
K2242.3340		3.3*	–	Titanium alloy/ Zirkonium oxide
K2242.3840		3.8	–	
K2242.4340		4.3	–	
K2242.5040		5.0	–	
K2242.6040		6.0	–	


H: height in mm

* only for crown restorations in the region of the upper lateral and lower lateral and central incisors (Ø 3.3 mm not for double crown restorations)


CAMLOG® PROSTHETICS

CROWN AND BRIDGE RESTORATIONS

CAMLOG® CERAMIC ABUTMENTS FOR CROWN RESTORATIONS

Art. No.	Article	Ø in mm	GH in mm	Material
Zirkonium oxide sleeves, for CAMLOG® Ceramic abutment, preparable				
J2242.3341		3.3*	–	Zirkonium oxide
J2242.3841		3.8	–	
J2242.4341		4.3	–	
J2242.5041		5.0	–	
J2242.6041		6.0	–	


CAMLOG® Titanium bases, for CAMLOG® Ceramic abutment

K2242.3342		3.3*	–	Titanium alloy
K2242.3842		3.8	–	
K2242.4342		4.3	–	
K2242.5042		5.0	–	
K2242.6042		6.0	–	

* only for crown restorations in the region of the upper lateral and lower lateral and central incisors

CAMLOG® LOGFIT® PROSTHETIC SYSTEM FOR CEMENTED CROWN AND BRIDGE RESTORATIONS


CAMLOG® Logfit® Abutments, incl. CAMLOG® Abutment screw

K2550.3808		3.8	0.8	Titanium alloy
K2550.3815			1.5	
K2550.4308		4.3	0.8	
K2550.4315			1.5	
K2550.5008		5.0	0.8	
K2550.5015			1.5	
K2550.6008	6.0	0.8		
K2550.6015		1.5		

Logfit® Impression caps

J2551.4300		3.8	–	POM
J2551.4300		4.3	–	
J2551.6000		5.0	–	
J2551.6000		6.0	–	

Logfit® Analogs

J2552.4300		3.8	–	Titanium alloy
J2552.4300		4.3	–	
J2552.6000		5.0	–	
J2552.6000		6.0	–	


GH: gingiva height


POM: Polyoxymethylene
H: height in mm

CAMLOG® PROSTHETICS

CROWN AND BRIDGE RESTORATIONS

CAMLOG® LOGFIT® PROSTHETIC SYSTEM FOR CEMENTED CROWN AND BRIDGE RESTORATIONS


Art. No.	Article	Ø in mm	GH in mm	Material
Logfit® Plastic copings, for crowns (with rotation securing device), burn-out				
J2553.4302		3.8	–	POM
J2553.4302		4.3	–	
J2553.6002		5.0	–	
J2553.6002		6.0	–	

Logfit® Plastic copings, for bridges (without rotation securing device), burn-out				
J2553.4301		3.8	–	POM
J2553.4301		4.3	–	
J2553.6001		5.0	–	
J2553.6001		6.0	–	

CROWN, BRIDGE AND HYBRID RESTORATIONS

CAD/CAM PROSTHETICS


CAMLOG® Titanium bases CAD/CAM, bonding base for individual CAD/CAM fabricated dental prosthesis
incl. CAMLOG® Abutment screw and CAMLOG® Bonding aid (POM)

K2244.3348		3.3*	–	Titanium alloy
K2244.3848		3.8	–	
K2244.4348		4.3	–	
K2244.5048		5.0	–	
K2244.6048		6.0	–	

* only for crown restorations in the region of the upper lateral and lower lateral and central incisors

Note: In order to achieve a level of user friendliness and high precision, the geometries of the CAMLOG® Titanium bases CAD/CAM are already available as a parts library for a number of dental CAD systems. For more information see [www.camlog.com/Products/CAMLOG/Digital Technology](http://www.camlog.com/Products/CAMLOG/Digital%20Technology).

CAMLOG® Modeling aids for CAMLOG® Titanium bases CAD/CAM, burn-out, for fabricating mesostructures and crowns

J2244.3302		3.3	–	POM
J2244.3802		3.8	–	
J2244.4302		4.3	–	
J2244.5002		5.0	–	
J2244.6002		6.0	–	

GH: gingiva height POM: Polyoxymethylene
H: height in mm

CAMLOG® PROSTHETICS

CROWN, BRIDGE AND HYBRID RESTORATIONS

CAD/CAM PROSTHETICS

Art. No.	Article	Ø in mm	Dimension in mm	Material
CAMLOG® Scanbodies, for optical, 3-dimensional localization of CAMLOG® Implants in the mouth or CAMLOG® Lab analogs in the working model, incl. CAMLOG® Abutment screw, sterile				
K2610.3310		3.3	–	PEEK
K2610.3810*		3.8	–	
K2610.4310*		4.3	–	
K2610.6010*		5.0	–	
		6.0	–	

*also for Platform Switching

Note: Some scan systems require the use of system-intrinsic scan abutments.
For information on the compatibility of the CAMLOG® Scanbody with suitable dental CAD systems see www.camlog.com/Products/CAMLOG/Digital Technology.

CAMLOG® ScanPosts for Sirona Scanbody, for digital recording of the CAMLOG® Implant or lab analog position, incl. CAMLOG® Abutment screw

K2620.3306		3.3	–	Titanium alloy
K2620.3806		3.8	–	
K2620.4306		4.3	–	
K2620.5006		5.0	–	
K2620.6006		6.0	–	

ACCESSORIES FOR CAMLOG® ABUTMENTS

CAMLOG® Bonding aids, for securing CAMLOG® Abutments and CAMLOG® Titanium bases CAD/CAM on the working model and for protecting the screw channel, white (2 units)

J4009.1600		3.3	Thread M 1.6	POM
		3.8		
		4.3		
J4009.2000		5.0	Thread M 2.0	
		6.0		

CAMLOG® Abutment screws, hex, for definitive screw retention of abutments into the implant

J4005.1601		3.3	Thread M 1.6	Titanium alloy
		3.8		
		4.3		
J4005.2001		5.0	Thread M 2.0	
		6.0		

CAMLOG® Lab screws, hex, for the fixation of abutments on the working model, brown anodized

J4006.1601		3.3	Thread M 1.6	Titanium alloy
		3.8		
		4.3		
J4006.2001		5.0	Thread M 2.0	
		6.0		

Note: Lab screws be used on working models only.

POM: Polyoxymethylene
 PEEK: Poly ether ether ketone
 H: height in mm

CAMLOG® PROSTHETICS

CROWN, BRIDGE AND HYBRID RESTORATIONS


CAMLOG® VARIO SR PROSTHETIC COMPONENTS FOR OCCLUSALLY SCREW-RETAINED RESTORATIONS

Art. No.	Article	\varnothing in mm	GH in mm	Material
----------	---------	------------------------	-------------	----------


CAMLOG® Vario SR abutments, straight, incl. CAMLOG® Vario SR abutment screw, sterile

K2560.3808			3.8	0.8	Titanium alloy
K2560.4308			4.3	0.8	
K2560.5008			5.0	0.8	
K2560.6008			6.0	0.8	


CAMLOG® Vario SR abutments, 20° angled, incl. CAMLOG® Abutment screw, sterile


K2561.3800		H 6.3	3.8	3.1-1.8	Titanium alloy
K2561.4300		H 6.3	4.3	3.2-1.7	
K2561.5000		H 6.9	5.0	3.9-2.2	
K2561.6000		H 6.9	6.0	4.0-2.0	

CAMLOG® Vario SR abutments, 30° angled, incl. CAMLOG® Abutment screw, sterile

K2562.3800		H 6.1	3.8	3.1-1.2	Titanium alloy
K2562.4300		H 6.1	4.3	3.2-1.0	
K2562.5000		H 7	5.0	4.0-1.5	
K2562.6000		H 7	6.0	4.3-1.3	

Impression taking, open and closed tray

J2566.4300		Vario SR impression cap, open tray, incl. fixing screw,	3.8	–	Titanium alloy
J2566.6000			4.3	–	
J2565.4300			5.0	–	
J2565.6000			6.0	–	

J2565.4300		Vario SR impression cap, closed tray	3.8	–	Titanium alloy
J2565.6000			4.3	–	
J2567.4300			5.0	–	
J2567.6000			6.0	–	

Fabrication of the plaster model




J2567.4300		Vario SR analog	3.8	–	Titanium alloy
J2567.6000			4.3	–	
J2567.4300			5.0	–	
J2567.6000			6.0	–	

GH: gingiva height
H: height in mm

CAMLOG® PROSTHETICS


CROWN, BRIDGE AND HYBRID RESTORATIONS

CAMLOG® VARIO SR PROSTHETIC COMPONENTS FOR OCCLUSALLY SCREW-RETAINED RESTORATIONS

Art. No.	Article	Ø in mm	GH in mm	Material
Cast crown, bridge and bar restorations				
J2563.4302	 <p>Vario SR plastic coping, crown, with triple-surface antirotation, burn-out</p>	3.8	—	POM
		4.3		
J2563.6002		5.0		
		6.0		
J2563.4301	 <p>Vario SR plastic coping, bridge, burn-out (2 units)</p>	3.8	—	POM
		4.3		
J2563.6001		5.0		
		6.0		
J2563.4303	 <p>Vario SR plastic coping, crown, with single-surface antirotation, for angled Vario SR abutments, burn-out</p>	3.8	—	POM
		4.3		
J2563.6003		5.0		
		6.0		

POM: Polyoxymethylene


Temporary or final bridge restorations

J2564.4301	 <p>Vario SR titanium cap, bridge, incl. Vario SR prosthetic screw</p>	3.8	—	Titanium alloy
		4.3		
J2564.6001		5.0		
		6.0		

Laser-welded bar restorations

J2570.4300	 <p>Vario SR base for bar, laser-weldable, incl. Vario SR prosthetic screw</p>	3.8	—	Titanium Grade 4
		4.3		
J2570.6000		5.0		
		6.0		

Accessories for Vario SR












J2568.4300	 <p>Vario SR protection cap, sterile</p>	3.8	—	Titanium alloy
		4.3		
J2568.6000		5.0		
		6.0		

GH: gingiva height
H: height in mm
Ø: implant diameter

CAMLOG® PROSTHETICS

CROWN, BRIDGE AND HYBRID RESTORATIONS


CAMLOG® VARIO SR PROSTHETIC COMPONENTS FOR OCCLUSALLY SCREW-RETAINED RESTORATIONS

Art. No.	Article	∅ in mm	Dimension in mm	Material	
Accessories for Vario SR					
J2569.0001		Vario SR aligning tool 20° , for insertion post, sterile	3.8	–	Copolycarbonate
			4.3		
			5.0		
			6.0		
J2569.0002		Vario SR aligning tool 30° , for insertion post, sterile	3.8	–	Copolycarbonate
			4.3		
			5.0		
			6.0		
J4007.1600		CAMLOG® Vario SR abutment screw , hex, for CAMLOG® Vario SR abutment, straight	3.8	Thread M 1.6	Titanium alloy
			4.3		
J4007.2000		CAMLOG® Vario SR abutment screw , hex, for CAMLOG® Vario SR abutment, straight	5.0	Thread M 2.0	
			6.0		
J4005.1601		CAMLOG® Abutment screw , hex, for CAMLOG® Vario SR abutment, 20°/30° angled	3.8	Thread M 1.6	Titanium alloy
			4.3		
J4005.2001		CAMLOG® Abutment screw , hex, for CAMLOG® Vario SR abutment, 20°/30° angled	5.0	Thread M 2.0	
			6.0		
J4008.1600		CAMLOG® Vario SR lab screw , hex, brown anodized, for CAMLOG® Vario SR abutment, straight	3.8	Thread M 1.6	Titanium alloy
			4.3		
J4008.2000		CAMLOG® Vario SR lab screw , hex, brown anodized, for CAMLOG® Vario SR abutment, straight	5.0	Thread M 2.0	
			6.0		
J4006.1601		CAMLOG® Lab screw , hex, brown anodized, for CAMLOG® Vario SR abutment, 20°/30° angled	3.8	Thread M 1.6	Titanium alloy
			4.3		
J4006.2001		CAMLOG® Lab screw , hex, brown anodized, for CAMLOG® Vario SR abutment, 20°/30° angled	5.0	Thread M 2.0	
			6.0		
J4005.2004		Vario SR prosthetic screw , hex, yellow anodized	3.8	Thread M 2.0	Titanium alloy
			4.3		
			5.0		
			6.0		


CAMLOG® PROSTHETICS

HYBRID RESTORATIONS

BAR RESTORATIONS

Art. No.	Article	Ø in mm	GH in mm	Material
J2255.3305 J2255.3320		3.3	0.5	Titanium alloy
J2255.3805 J2255.3820 J2255.3840			2.0	
J2255.4305 J2255.4320 J2255.4340			4.0	
J2255.5005 J2255.5020 J2255.5040		5.0	0.5	
J2255.6005 J2255.6020 J2255.6040			2.0	
			4.0	

Impression posts for bar abutment

J2130.4300		H 6.5	3.3	-	Titanium alloy
		H 6.5	3.8		
		H 6.5	4.3		
J2130.6000		H 7	5.0	-	
		H 7	6.0		


Healing caps for bar abutment

J2030.4300			3.3	-	Titanium alloy
			3.8		
			4.3		
J2030.6000			5.0	-	
			6.0		

Soldering aids/bar lab analogs, for bar abutments

J3020.4300			3.3	-	Stainless steel
			3.8		
			4.3		
J3020.6000			5.0	-	
			6.0		

Screws, hex, for bar abutment, screws for bases for bar abutments for impression taking, open tray and for soldering aid

J4005.1610			3.3	Thread M 1.6	Stainless steel
			3.8		
			4.3		
J4005.2010			5.0	Thread M 2.0	
			6.0		

GH: gingiva height
H: height in mm


CAMLOG® PROSTHETICS

HYBRID RESTORATIONS

BAR RESTORATIONS

Art. No.	Article	∅ in mm	Dimension in mm	Material
----------	---------	------------	--------------------	----------

Bases for bar abutment, burn-out

J2257.3300	 H 14	3.3	–	POM
J2257.3800		3.8	–	
J2257.4300		4.3	–	
J2257.5000		5.0	–	
J2257.6000		6.0	–	

Bases for bar abutment, cast-on

J2263.4300	 H 14	3.3	0,48 g*	Cast-on gold alloy/POM
J2263.6000		3.8		
		4.3	0,70 g*	
		5.0		
		6.0		

* Noble metal weight approx.


Bases for bar abutment, solderable

J2258.4300	 H 5.3	3.3	–	Solderable gold alloy
J2258.6000		3.8		
		4.3		
		5.0		
		6.0		

Bases for bar abutment, titanium, laser-weldable

J2262.4300	 H 5.3	3.3	–	Titanium Grade 4
J2262.6000		3.8		
		4.3		
		5.0		
		6.0		

Titanium bonding bases for bar abutment, Passive-Fit


J2260.3300	 H 3.5	3.3	–	Titanium alloy
J2260.3800		3.8		
J2260.4300		4.3		
J2260.5000		5.0		
J2260.6000		6.0		

POM: Polyoxymethylene
H: height in mm


CAMLOG® PROSTHETICS

HYBRID RESTORATIONS

BAR RESTORATIONS

Art. No.	Article	Ø in mm	GH in mm	Material
Sleeves for titanium bonding base, burn-out, Passive-Fit				
J2261.3300		3.3	–	POM
J2261.3800		3.8	–	
J2261.4300		4.3	–	
J2261.5000		5.0	–	
J2261.6000		6.0	–	

Holding pins, for bar abutment/bar lab analog (4 units)


J2256.1600		3.3	Thread M 1.6	POM
		3.8		
		4.3		
J2256.2000		5.0	Thread M 2.0	
		6.0		

Prosthetic screws for bar abutments, hex, for bar bases/sleeves (also for Passive-Fit)

J4005.1602		3.3	Thread M 1.6	Titanium alloy
		3.8		
		4.3		
J4005.2002		5.0	Thread M 2.0	
		6.0		

BALL ABUTMENT ANCHORING SYSTEM

CAMLOG® Ball abutment sets, incl. male part and matrix CM Dalbo®-Plus,
red duplication aid/spacer, stabilizing ring and ball abutment analog

J2250.3315		3.3	1.5	Titanium alloy/ Titanium Grade 4/ Gold alloy/Brass/ Plastic
J2250.3330			3.0	
J2250.3815		3.8	1.5	
J2250.3830			3.0	
J2250.3845			4.5	
J2250.4315		4.3	1.5	
J2250.4330			3.0	
J2250.4345			4.5	
J2250.5015		5.0	1.5	
J2250.5030			3.0	
J2250.5045			4.5	


GH: gingiva height

POM: Polyoxymethylene
H: height in mm

CAMLOG® PROSTHETICS

HYBRID RESTORATIONS

BALL ABUTMENT ANCHORING SYSTEM

Art. No.	Article	Ø in mm	GH in mm	Material
J2249.3315 J2249.3330		3.3	1.5 3.0	Titanium alloy
J2249.3815 J2249.3830 J2249.3845		3.8	1.5 3.0 4.5	
J2249.4315 J2249.4330 J2249.4345		4.3	1.5 3.0 4.5	
J2249.5015 J2249.5030 J2249.5045		5.0	1.5 3.0 4.5	

Matrix CM Dalbo®-Plus, for ball abutment, incl. lamella retention insert


J2250.0005		3.3	-	Titanium Grade 4/ Gold alloy
		3.8		
		4.3		
		5.0		

Lamella retention insert, for matrix CM Dalbo®-Plus

J2250.0007		3.3	-	Gold alloy
		3.8		
		4.3		
		5.0		

Dalbo®-Plus is a registered trademark of Cendres + Métaux SA, Biel, Switzerland.

Ball abutment analogs incl. stabilizing ring


J3015.3300		3.3	-	Brass/Plastic
J3015.3800		3.8	-	
J3015.4300		4.3	-	
J3015.5000		5.0	-	

GH: gingiva height H: height in mm


CAMLOG® PROSTHETICS

HYBRID RESTORATIONS


LOCATOR® ANCHORING SYSTEM

Art. No.	Article	Ø in mm	GH in mm	Material
CAMLOG® Locator® Abutments				
J2253.3310 J2253.3320 J2253.3330 J2253.3340		3.3	1.0	Titanium alloy/TiN
			2.0	
			3.0	
			4.0	
J2253.3810 J2253.3820 J2253.3830 J2253.3840 J2253.3850		3.8	1.0	
			2.0	
			3.0	
			4.0	
			5.0	
J2253.4310 J2253.4320 J2253.4330 J2253.4340 J2253.4350		4.3	1.0	
			2.0	
			3.0	
			4.0	
			5.0	
J2253.5010 J2253.5020 J2253.5030 J2253.5040 J2253.5050		5.0	1.0	
			2.0	
			3.0	
			4.0	
			5.0	

Impression taking





J2253.0200		Locator® Impression cap (4 units)	3.3	–	Aluminum/ Polyethylene
			3.8		
			4.3		
			5.0		

Modellherstellung

J2253.0340		Locator® Analog (4 units)	3.3	–	Aluminum
			3.8		
			4.3		
J2253.0350			5.0	–	

GH: gingiva height TiN: Titanium nitride-coated
H: height in mm




CAMLOG® PROSTHETICS
HYBRID RESTORATIONS
LOCATOR® ANCHORING SYSTEM

Art. No.	Article	∅ in mm	Dimension in mm	Material	
Locator® Male processing packages					
J2253.0102		Locator® Male processing package (2 units), Content per package: 1 Titanium housing with processing replacement male 1 Block out spacer white 1 Replacement male clear 1 Replacement male pink 1 Replacement male blue	3.3	–	Titanium alloy/ Polyethylene/ Teflon/Nylon
			3.8		
			4.3		
			5.0		
J2253.0112		Locator® Male processing package for extended range (2 units), Content per package: 1 Titanium housing with processing replacement male 1 Block out spacer white 1 Replacement male green, 1 Replacement male orange, 1 Replacement male red	3.8	–	Titanium alloy/ Polyethylene/ Teflon/Nylon
			4.3		
			5.0		
Locator® Accessories					
J2253.0401		Locator® Block out spacer (20 units)	3.3	–	Teflon
			3.8		
			4.3		
			5.0		
J2253.0402		Locator® Processing replacement male (4 units)	3.3	–	Polyethylene
			3.8		
			4.3		
			5.0		





CAMLOG® PROSTHETICS

HYBRID RESTORATIONS

LOCATOR® ANCHORING SYSTEM

Art. No.		Article	∅ in mm	Dimension in mm	Material
J2253.1005		Locator® Replacement male, clear, STRONG, Div.: 0°-10° (4 units)	3.3	–	Nylon
			3.8		
			4.3		
			5.0		
J2253.1003		Locator® Replacement male, pink, MEDIUM, Div.: 0°-10° (4 units)	3.3	–	Nylon
			3.8		
			4.3		
			5.0		
J2253.1002		Locator® Replacement male, blue, LIGHT, Div.: 0°-10° (4 units)	3.3	–	Nylon
			3.8		
			4.3		
			5.0		

Locator® Replacement males for extended range

J2253.2004		Locator® Replacement male for extended range*, green, STRONG, Div.: 10°-20° (4 units)	3.8	–	Nylon
			4.3		
			5.0		
J2253.2003		Locator® Replacement male for extended range*, orange, MEDIUM, Div.: 10°-20° (4 units)	3.8	–	Nylon
			4.3		
			5.0		
J2253.2002		Locator® Replacement male for extended range*, red, LIGHT, Div.: 10°-20° (4 units)	3.8	–	Nylon
			4.3		
			5.0		
J2253.2000		Locator® Replacement male for extended range*, gray, NO RETENTION, Div.: 0°-20° (4 units)	3.8	–	Nylon
			4.3		
			5.0		

* nonlicensed for implant diameter 3.3 mm


Manufacturer Locator®:
Zest Anchors LLC
Escondido, CA 92029, USA

Locator® is a registered trademark of Zest Anchors LLC

CAMLOG® PROSTHETICS

HYBRID RESTORATIONS

DOUBLE CROWN RESTORATIONS WITH CAMLOG® UNIVERSAL AND TELESCOPE ABUTMENTS

Art. No.	Article	∅ in mm	Dimension in mm	Material
CAMLOG® Universal abutments for double crown restorations, preparable, incl. CAMLOG® Abutment screw				
K2211.3800	 H 11		3.8	Titanium alloy
K2211.4300			4.3	
K2211.5000			5.0	
K2211.6000			6.0	

CAMLOG® Universal abutments PS for double crown restorations, for Platform Switching, preparable, incl. CAMLOG® Abutment screw

K2201.3800	 H 11			3.8	Titanium alloy
K2201.4300				4.3	
K2201.5000				5.0	
K2201.6000				6.0	

Note: CAMLOG® Universal abutments PS should only be used on CAMLOG® Implants with K article number!



CAMLOG® Telescope abutments for double crown restorations, preparable, incl. CAMLOG® Abutment screw

K2212.3800	 H 12		3.8	Titanium alloy
K2212.4300			4.3	
K2212.5000			5.0	
K2212.6000			6.0	



H: height in mm

ACCESSORIES FOR CAMLOG® ABUTMENTS

Abutment screws for the definitive screwing of abutments into the implant

J4005.1601		CAMLOG® Abutment screw, hex	3.3	Thread M 1.6	Titanium alloy
			3.8		
J4005.2001			4.3	Thread M 2.0	
			5.0		
			6.0		

Laborschrauben für die Befestigung auf dem Arbeitsmodell

J4006.1601		CAMLOG® Lab screw, hex, brown anodized	3.3	Thread M 1.6	Titanium alloy
			3.8		
			4.3		
J4006.2001			5.0	Thread M 2.0	
			6.0		

Note: Lab screws be used on working models only.

CAMLOG® PROSTHETICS

INSTRUMENTS FOR DENTAL TECHNICIANS

Art. No.	Article	∅ in mm	Material
----------	---------	------------	----------

Universal holders

J3709.0010	Universal holder, incl. 2 CAMLOG® Lab screws, hex, and 1 each CAMLOG® Abutment collet ∅ 3.3/3.8/4.3/5.0/6.0 mm		Stainless steel/ Titanium alloy
------------	--	--	------------------------------------




J3709.0015	Universal holder		Stainless steel
------------	-------------------------	--	-----------------




CAMLOG® Abutment collets, for universal holder, for grinding CAMLOG® Abutments

J3709.3300		3.3	Titanium alloy
J3709.3800		3.8	
J3709.4300		4.3	
J3709.5000		5.0	
J3709.6000		6.0	

Collets for zirconium oxide sleeve, for universal holder

J3712.4300		3.3	PEEK
		3.8	
		4.3	
J3712.6000		5.0	
		6.0	



Reamers for dilating the plaster model, for universal holder, incl. color-coded guide pin

J3706.3300		3.3	Stainless steel/ Titanium alloy
J3706.3800		3.8	
J3706.4300		4.3	
J3706.5000		5.0	
J3706.6000		6.0	

PEEK: Poly ether ether ketone

CAMLOG® PROSTHETICS

INSTRUMENTS FOR DENTAL TECHNICIANS

Art. No.	Article	∅ in mm	Material
Reworking reamers			
J3711.0010	Reworking reamer, for base for bar abutment, plane surface/cone seat, burn-out	3.3	Stainless steel
		3.8	
		4.3	
J3711.0015		5.0	
		6.0	
		3.3	
J3711.0020	Reworking reamer, for base for bar abutment, screw seat, burn-out	3.3	Stainless steel
		3.8	
		4.3	
J3711.0025		5.0	
		6.0	

CAMLOG® PROSTHETICS

CAMLOG® SELECTION ABUTMENTS

Art. No.	Article	∅ in mm	GH in mm	Material
----------	---------	------------	-------------	----------

K8011.1000



CAMLOG® Selection abutment kit,

Content (2 units each):

CAMLOG® Esthomic® Selection abutment, straight	3.8	1.0-1.8	POM
CAMLOG® Esthomic® Selection abutment, straight	3.8	3.0-4.5	
CAMLOG® Esthomic® Selection abutment, straight	4.3	1.0-1.8	
CAMLOG® Esthomic® Selection abutment, straight	4.3	3.0-4.5	
CAMLOG® Esthomic® Selection abutment, straight	5.0	1.0-1.8	
CAMLOG® Esthomic® Selection abutment, straight	5.0	3.0-4.5	
CAMLOG® Esthomic® Selection abutment, 15° angled, type A	3.8	1.0-1.8	
CAMLOG® Esthomic® Selection abutment, 15° angled, type A	4.3	1.0-1.8	
CAMLOG® Esthomic® Selection abutment, 15° angled, type A	5.0	1.0-1.8	
CAMLOG® Esthomic® Selection abutment, 15° angled, type B	3.8	1.0-1.8	
CAMLOG® Esthomic® Selection abutment, 15° angled, type B	4.3	1.0-1.8	
CAMLOG® Esthomic® Selection abutment, 15° angled, type B	5.0	1.0-1.8	
CAMLOG® Esthomic® Selection abutment, 20° angled, type A	3.8	1.0-1.8	
CAMLOG® Esthomic® Selection abutment, 20° angled, type A	4.3	1.0-1.8	
CAMLOG® Esthomic® Selection abutment, 20° angled, type A	5.0	1.0-1.8	
CAMLOG® Esthomic® Selection abutment, 20° angled, type B	3.8	1.0-1.8	
CAMLOG® Esthomic® Selection abutment, 20° angled, type B	4.3	1.0-1.8	
CAMLOG® Esthomic® Selection abutment, 20° angled, type B	5.0	1.0-1.8	
CAMLOG® Vario SR selection abutment, straight	3.8	0.8	
CAMLOG® Vario SR selection abutment, straight	4.3	0.8	
CAMLOG® Vario SR selection abutment, straight	5.0	0.8	
CAMLOG® Vario SR selection abutment, 20° angled	3.8	3.1-1.8	
CAMLOG® Vario SR selection abutment, 20° angled	4.3	3.2-1.7	
CAMLOG® Vario SR selection abutment, 20° angled	5.0	3.9-2.2	
CAMLOG® Vario SR selection abutment, 30° angled	3.8	3.1-1.2	
CAMLOG® Vario SR selection abutment, 30° angled	4.3	3.2-1.0	
CAMLOG® Vario SR selection abutment, 30° angled	5.0	4.0-1.5	

GH: gingiva height POM: Polyoxymethylene

Attention, do not use selection abutments on patients!





AUXILIARY ARTICLE

CONTENT

AUXILIARY ARTICLE	73
IMPLANTS FOR PRACTICE	74
DEMONSTRATION MODELS	74
MACRO MODEL	74
CAMLOG LITERATURE	75




AUXILIARY ARTICLE

IMPLANTS FOR PRACTICE

Art. No.		Article	∅ in mm	Length in mm	Material
K1049.3813		CAMLOG® SCREW-LINE Implant for practice, incl. insertion post and cover screw, yellow anodized	3.8	13	Titanium alloy
K1049.4313-01		CAMLOG® SCREW-LINE Implant for practice, incl. insertion post and cover screw, red anodized	4.3	13	Titanium alloy
K1039.3813		CAMLOG® ROOT-LINE 2 Implant for practice, incl. insertion post and cover screw, yellow anodized	3.8	13	Titanium alloy
K1039.4313		CAMLOG® ROOT-LINE 2 Implant for practice, incl. insertion post and cover screw, red anodized	4.3	13	Titanium alloy


Attention, do not use implants for practice on patients!

DEMONSTRATION MODELS

K8070.1020		CAMLOG® Demonstration model, acrylic glass, upper jaw, 4 CAMLOG® SCREW-LINE Implants, 4 x ∅ 4.3 mm			Acrylic glass/ Titanium
K8050.1040		CAMLOG® Demonstration model, acrylic glass, lower jaw, 4 CAMLOG® SCREW-LINE Implants, 4 x ∅ 4.3 mm			Acrylic glass/ Titanium
J8070.2050		Edentulous mandible incl. mounting plate			Plastic

AUXILIARY ARTICLE


MACRO MODEL

Art. No.	Article	Material
K8010.1010	 <p>CAMLOG® SCREW-LINE Macro model, Scale 3:1 Content:</p> <ul style="list-style-type: none"> - 1 CAMLOG® SCREW-LINE Implant - 1 CAMLOG® Esthomic® Abutment, straight - 1 CAMLOG® Abutment screw, hex - 1 Screwdriver, hex - 1 Premolar, suitable for CAMLOG® Esthomic® Abutment, straight - 1 Acrylic socket 	Plastic/ Stainless steel
K8010.1011	 <p>CAMLOG® ROOT-LINE 2 Macro model, Scale 3:1 Content:</p> <ul style="list-style-type: none"> - 1 CAMLOG® ROOT-LINE 2 Implant - 1 CAMLOG® Esthomic® Abutment, straight - 1 CAMLOG® Abutment screw, hex - 1 Screwdriver, hex - 1 Premolar, suitable for CAMLOG® Esthomic® Abutment, straight - 1 Acrylic socket 	Plastic/ Stainless steel

CAMLOG LITERATURE



Patient brochure
Questions and answers to dental implants




Implant pass
Patient-specific documentation of implant restoration
Packaging units: 10 units

AUXILIARY ARTICLE

CAMLOG LITERATURE

Art. No.

Article



Patient advice sheets

Set á 4 sheets, A4




Presentation folder

A4, laminated



Poster

Format: 50 x 70 cm



Appointment pad

50 sheets/pad, A7

Packaging units: 5 units

B2012.0100



IMPLANT PROSTHETICS

DVD compendium

Four teams – their concepts and solutions, Volume 1-4

A. Kirsch, K. L. Ackermann, G. Neuendorff,

A. Happe, A. Nolte, S. Wolfart, V. Weber, F. Beuer,

M. Stimmelmayer, J. Schweiger

2012 Quintessence Publishing Co, Ltd

INFORMATION CONTENT

INFORMATION	77
MATERIALS	78

INFORMATION

MATERIALS

Titanium Grade 4

Properties (ASTM F67):

Chemical structure (in %):	O	≤ 0.4
	Fe	≤ 0.5
	C	≤ 0.08
	N	≤ 0.05
	H	≤ 0.015
	Ti	Rest
Mechanical properties:	Tensile strength	≥ 550 MPa
	Elongation at break	≥ 15 %

Titanium alloy Ti6Al4V ELI

Properties (ASTM F136):

Chemical structure (in %):	Al	5.5 - 6.5
	V	3.5 - 4.5
	Fe	≤ 0.25
	C	≤ 0.08
	N	≤ 0.05
	O	≤ 0.13
	H	≤ 0.012
	Ti	Rest
Mechanical properties:	Tensile strength	≥ 860 MPa
	Elongation at break	≥ 10 %

Cast-on gold alloy CAMLOG® Gold-plastic abutment

Properties:

Chemical structure (in %):	Au	60
	Pd	20
	Pt	19
	Ir	1
Physical properties:	Melting range	1400 - 1490 °C
	Density	17.5 g/cm ³
	E-Modul	136 GPa
	Coefficient of thermal expansion (25-500°C)	11.9 µm/m·°C
	Coefficient of thermal expansion (25-600°C)	12.2 µm/m·°C
	Color	white
Mechanical properties:	Color	drawn
	Hardness HV5	> 215
	Tensile strength (Rm)	> 750 MPa
	0.2% Elongation limit (Rp 0.2%)	> 650 MPa
	Elongation at break	> 2%

Cast-on gold alloy
Base for bar abutment

Properties:

Chemical structure (in %):	Au	60
	Pt	19
	Pd	20
	Ir	1
Mechanical properties:	Density	17.5 g/cm ³
	Color	white
	Liquidus	1490 °C
	Solidus	1400 °C
	Coefficient of thermal expansion (25-500°C)	12.5 µm/m·°C
	Coefficient of thermal expansion (25-600°C)	12.6 µm/m·°C
	E-Modul	136.000 GPa
	hardened	700 °C / 30 min.
	Hardness HV5	210
	0.2 % Elongation limit	450-570 MPa
	Elongation at break	min 10 %
	Tensile strength MPa	530-650

Solderable gold alloy
Base for bar abutment

Properties:

Chemical structure (in %):	Au	70.00
	Pt	8.50
	Ag	13.40
	Pd	-
	Cu	7.50
	Zn	0.50
	Ir	0.10
	Rh	-
	Ru	-
	Mechanical properties:	Color
Melting range		895 - 1010 °C
	Hardness	
	annealed HV5	170
	hardened HV5	295
	self hardened HV5	280

Zirconium oxide

Properties:

Chemical structure (in %):	ZrO ₂ + HfO ₂ + Y ₂ O ₃	> 99.0
	Y ₂ O ₃	4.5 - 5.4
	HfO ₂	< 5
	Al ₂ O ₃	< 0.5
	other oxides	< 0.5
Mechanical properties:	Density	> 6.0 g/cm ³
	Porosity, open	0.00 %
	Microstructure:	
	Mean Linear intercept size	< 0.6 µm
	3 pt. transversal strength	≥ 800 MPa

INDEX	81
ALPHABETICAL	82
ARTICLE NUMBERS	90

INDEX

ALPHABETICAL

Article Article No. Page

A

Adapter for screw implants, long

for CAMLOG® SCREW-LINE and ROOT-LINE 2 Implants

Ø 3.3 mm	K5302.3310	37
Ø 3.8 mm	K5302.3810	37
Ø 4.3 mm	K5302.4310	37

Adapter,

ISO shaft for angled hand piece

	J5002.0011	37
--	------------	----

ALTApin applicator, angled 90°

	M5100.0030	35
--	------------	----

ALTApin applicator, straight

	M5100.0010	35
--	------------	----

ALTApin applicator, straight, work element

	M5200.0010	35
--	------------	----

ALTApin magazine

7 titanium pins, sterile packaging, 1 unit

	M1000.0050	35
--	------------	----

7 titanium pins, sterile packaging, 3 units

	M1000.0100	35
--	------------	----

ALTApin membrane fixator

	M5100.0070	35
--	------------	----

ALTApin pricker

	M5100.0050	35
--	------------	----

ALTApin pricker, insert

	M5200.0055	35
--	------------	----

ALTApin set

	M5600.0110	35
--	------------	----

ALTApin single patient drill, ISO shaft

	M5500.0050	35
--	------------	----

ALTApin surgery mallet

	M5100.0100	35
--	------------	----

ALTApin-Tray

	M5600.0210	35
--	------------	----

B

Ball abutment analogs

Ø 3.3 mm	J3015.3300	65
Ø 3.8 mm	J3015.3800	65
Ø 4.3 mm	J3015.4300	65
Ø 5.0 mm	J3015.5000	65

Bases for bar abutment, burn-out

Ø 3.3 mm	J2257.3300	63
Ø 3.8 mm	J2257.3800	63
Ø 4.3 mm	J2257.4300	63
Ø 5.0 mm	J2257.5000	63
Ø 6.0 mm	J2257.6000	63

Bases for bar abutment, cast-on

Ø 3.3/3.8/4.3 mm	J2263.4300	63
Ø 5.0/6.0 mm	J2263.6000	63

Bases for bar abutment, laser-weldable

Ø 3.3/3.8/4.3 mm	J2262.4300	63
Ø 5.0/6.0 mm	J2262.6000	63

Bases for bar abutment, solderable

Ø 3.3/3.8/4.3 mm	J2258.4300	63
Ø 5.0/6.0 mm	J2258.6000	63

Bite registration caps (5 units)

Ø 3.3 mm	J2112.3300	51
Ø 3.8 mm	J2112.3800	51
Ø 4.3 mm	J2112.4300	51
Ø 5.0 mm	J2112.5000	51
Ø 6.0 mm	J2112.6000	51

Bite registration caps (5 units)

Ø 3.3 mm	J2112.3300	51
Ø 3.8 mm	J2112.3800	51
Ø 4.3 mm	J2112.4300	51
Ø 5.0 mm	J2112.5000	51
Ø 6.0 mm	J2112.6000	51

C

CAMLOG® Abutment collets, for universal holder

Ø 3.3 mm	J3709.3300	70
Ø 3.8 mm	J3709.3800	70
Ø 4.3 mm	J3709.4300	70
Ø 5.0 mm	J3709.5000	70
Ø 6.0 mm	J3709.6000	70

Article Article No. Page

CAMLOG® Abutment screws, hex

Ø 3.3/3.8/4.3 mm, thread M 1.6	J4005.1601	58, 61, 69
Ø 5.0/6.0 mm, thread M 2.0	J4005.2001	58, 61, 69

CAMLOG® Ball abutment sets,

incl. male part and matrix CM Dalbo®-Plus

Ø 3.3 mm, GH 1.5 mm	J2250.3315	64
Ø 3.3 mm, GH 3.0 mm	J2250.3330	64
Ø 3.8 mm, GH 1.5 mm	J2250.3815	64
Ø 3.8 mm, GH 3.0 mm	J2250.3830	64
Ø 3.8 mm, GH 4.5 mm	J2250.3845	64
Ø 4.3 mm, GH 1.5 mm	J2250.4315	64
Ø 4.3 mm, GH 3.0 mm	J2250.4330	64
Ø 4.3 mm, GH 4.5 mm	J2250.4345	64
Ø 5.0 mm, GH 1.5 mm	J2250.5015	64
Ø 5.0 mm, GH 3.0 mm	J2250.5030	64
Ø 5.0 mm, GH 4.5 mm	J2250.5045	64

CAMLOG® Ball abutments, male part

Ø 3.3 mm, GH 1.5 mm	J2249.3315	65
Ø 3.3 mm, GH 3.0 mm	J2249.3330	65
Ø 3.8 mm, GH 1.5 mm	J2249.3815	65
Ø 3.8 mm, GH 3.0 mm	J2249.3830	65
Ø 3.8 mm, GH 4.5 mm	J2249.3845	65
Ø 4.3 mm, GH 1.5 mm	J2249.4315	65
Ø 4.3 mm, GH 3.0 mm	J2249.4330	65
Ø 4.3 mm, GH 4.5 mm	J2249.4345	65
Ø 5.0 mm, GH 1.5 mm	J2249.5015	65
Ø 5.0 mm, GH 3.0 mm	J2249.5030	65
Ø 5.0 mm, GH 4.5 mm	J2249.5045	65

CAMLOG® Bar abutments

Ø 3.3 mm, GH 0.5 mm	J2255.3305	62
Ø 3.3 mm, GH 2.0 mm	J2255.3320	62
Ø 3.8 mm, GH 0.5 mm	J2255.3805	62
Ø 3.8 mm, GH 2.0 mm	J2255.3820	62
Ø 3.8 mm, GH 4.0 mm	J2255.3840	62
Ø 4.3 mm, GH 0.5 mm	J2255.4305	62
Ø 4.3 mm, GH 2.0 mm	J2255.4320	62
Ø 4.3 mm, GH 4.0 mm	J2255.4340	62
Ø 5.0 mm, GH 0.5 mm	J2255.5005	62
Ø 5.0 mm, GH 2.0 mm	J2255.5020	62
Ø 5.0 mm, GH 4.0 mm	J2255.5040	62
Ø 6.0 mm, GH 0.5 mm	J2255.6005	62
Ø 6.0 mm, GH 2.0 mm	J2255.6020	62
Ø 6.0 mm, GH 4.0 mm	J2255.6040	62

CAMLOG® Bite registration posts

Ø 3.3 mm	J2140.3300	51
Ø 3.8 mm	J2140.3800	51
Ø 4.3 mm	J2140.4300	51
Ø 5.0 mm	J2140.5000	51
Ø 6.0 mm	J2140.6000	51

CAMLOG® Bonding aids

Ø 3.3/3.8/4.3 mm, thread M 1.6	J4009.1600	58
Ø 5.0/6.0 mm, thread M 2.0	J4009.2000	58

CAMLOG® Ceramic abutments, 2-parts

Ø 3.3 mm	K2242.3340	55
Ø 3.8 mm	K2242.3840	55
Ø 4.3 mm	K2242.4340	55
Ø 5.0 mm	K2242.5040	55
Ø 6.0 mm	K2242.6040	55

CAMLOG® Demonstration model, acrylic glass

upper jaw, CAMLOG® SCREW-LINE, Ø 4.3 mm	K8070.1020	74
lower jaw, CAMLOG® SCREW-LINE, Ø 4.3 mm	K8050.1040	74

CAMLOG® Esthomic® Abutments PS, 15° angled, type A

Ø 3.8 mm, GH 1.5-2.5 mm	K2203.3815	54
Ø 4.3 mm, GH 1.5-2.5 mm	K2203.4315	54
Ø 5.0 mm, GH 1.5-2.5 mm	K2203.5015	54
Ø 6.0 mm, GH 1.5-2.5 mm	K2203.6015	54

INDEX

ALPHABETICAL

Article	Article No.	Page
CAMLOG® Esthomic® Abutments PS, 15° angled, type B		
∅ 3.8 mm, GH 1.5-2.5 mm	K2204.3815	54
∅ 4.3 mm, GH 1.5-2.5 mm	K2204.4315	54
∅ 5.0 mm, GH 1.5-2.5 mm	K2204.5015	54
∅ 6.0 mm, GH 1.5-2.5 mm	K2204.6015	54
CAMLOG® Esthomic® Abutments PS, straight		
∅ 3.8 mm, GH 1.5-2.5 mm	K2202.3815	54
∅ 4.3 mm, GH 1.5-2.5 mm	K2202.4315	54
∅ 5.0 mm, GH 1.5-2.5 mm	K2202.5015	54
∅ 6.0 mm, GH 1.5-2.5 mm	K2202.6015	54
CAMLOG® Esthomic® Abutments, 15° angled, type A		
∅ 3.8 mm, GH 1.0-1.8 mm	K2227.3810	52
∅ 3.8 mm, GH 3.0-4.5 mm	K2227.3830	52
∅ 4.3 mm, GH 1.0-1.8 mm	K2227.4310	52
∅ 4.3 mm, GH 3.0-4.5 mm	K2227.4330	52
∅ 5.0 mm, GH 1.0-1.8 mm	K2227.5010	52
∅ 5.0 mm, GH 3.0-4.5 mm	K2227.5030	52
∅ 6.0 mm, GH 1.0-1.8 mm	K2227.6010	52
∅ 6.0 mm, GH 3.0-4.5 mm	K2227.6030	52
CAMLOG® Esthomic® Abutments, 15° angled, type B		
∅ 3.8 mm, GH 1.0-1.8 mm	K2228.3810	53
∅ 3.8 mm, GH 3.0-4.5 mm	K2228.3830	53
∅ 4.3 mm, GH 1.0-1.8 mm	K2228.4310	53
∅ 4.3 mm, GH 3.0-4.5 mm	K2228.4330	53
∅ 5.0 mm, GH 1.0-1.8 mm	K2228.5010	53
∅ 5.0 mm, GH 3.0-4.5 mm	K2228.5030	53
∅ 6.0 mm, GH 1.0-1.8 mm	K2228.6010	53
∅ 6.0 mm, GH 3.0-4.5 mm	K2228.6030	53
CAMLOG® Esthomic® Abutments, 20° angled, type A		
∅ 3.8 mm, GH 1.0-1.8 mm	K2231.3810	53
∅ 3.8 mm, GH 3.0-4.5 mm	K2231.3830	53
∅ 4.3 mm, GH 1.0-1.8 mm	K2231.4310	53
∅ 4.3 mm, GH 3.0-4.5 mm	K2231.4330	53
∅ 5.0 mm, GH 1.0-1.8 mm	K2231.5010	53
∅ 5.0 mm, GH 3.0-4.5 mm	K2231.5030	53
∅ 6.0 mm, GH 1.0-1.8 mm	K2231.6010	53
∅ 6.0 mm, GH 3.0-4.5 mm	K2231.6030	53
CAMLOG® Esthomic® Abutments, 20° angled, type B		
∅ 3.8 mm, GH 1.0-1.8 mm	K2232.3810	53
∅ 3.8 mm, GH 3.0-4.5 mm	K2232.3830	53
∅ 4.3 mm, GH 1.0-1.8 mm	K2232.4310	53
∅ 4.3 mm, GH 3.0-4.5 mm	K2232.4330	53
∅ 5.0 mm, GH 1.0-1.8 mm	K2232.5010	53
∅ 5.0 mm, GH 3.0-4.5 mm	K2232.5030	53
∅ 6.0 mm, GH 1.0-1.8 mm	K2232.6010	53
∅ 6.0 mm, GH 3.0-4.5 mm	K2232.6030	53
CAMLOG® Esthomic® Abutments, straight		
∅ 3.8 mm, GH 1.0-1.8 mm	K2226.3810	52
∅ 3.8 mm, GH 3.0-4.5 mm	K2226.3830	52
∅ 4.3 mm, GH 1.0-1.8 mm	K2226.4310	52
∅ 4.3 mm, GH 3.0-4.5 mm	K2226.4330	52
∅ 5.0 mm, GH 1.0-1.8 mm	K2226.5010	52
∅ 5.0 mm, GH 3.0-4.5 mm	K2226.5030	52
∅ 6.0 mm, GH 1.0-1.8 mm	K2226.6010	52
∅ 6.0 mm, GH 3.0-4.5 mm	K2226.6030	52
CAMLOG® Esthomic® Abutments, Inset		
∅ 3.3 mm, GH 1.5-2.8 mm	K2235.3315	53
∅ 3.8 mm, GH 1.5-2.8 mm	K2235.3815	53
∅ 4.3 mm, GH 1.5-2.8 mm	K2235.4315	53
∅ 5.0 mm, GH 1.5-2.8 mm	K2235.5015	53
∅ 6.0 mm, GH 1.5-2.8 mm	K2235.6015	53
CAMLOG® Gold-plastic abutments		
∅ 3.3 mm	K2246.3300	55
∅ 3.8 mm	K2246.3800	55
∅ 4.3 mm	K2246.4300	55
∅ 5.0 mm	K2246.5000	55
∅ 6.0 mm	K2246.6000	55

Article	Article No.	Page
CAMLOG® Healing cap PS, bottleneck		
∅ 3.8 mm, GH 4.0 mm	K2001.3840	34
∅ 3.8 mm, GH 6.0 mm	K2001.3860	34
∅ 4.3 mm, GH 4.0 mm	K2001.4340	34
∅ 4.3 mm, GH 6.0 mm	K2001.4360	34
∅ 5.0 mm, GH 4.0 mm	K2001.5040	34
∅ 5.0 mm, GH 6.0 mm	K2001.5060	34
∅ 6.0 mm, GH 4.0 mm	K2001.6040	34
∅ 6.0 mm, GH 6.0 mm	K2001.6060	34
CAMLOG® Healing cap PS, cylindrical		
∅ 3.8 mm, GH 2.0 mm	K2005.3820	34
∅ 3.8 mm, GH 4.0 mm	K2005.3840	34
∅ 3.8 mm, GH 6.0 mm	K2005.3860	34
∅ 4.3 mm, GH 2.0 mm	K2005.4320	34
∅ 4.3 mm, GH 4.0 mm	K2005.4340	34
∅ 4.3 mm, GH 6.0 mm	K2005.4360	34
∅ 5.0 mm, GH 2.0 mm	K2005.5020	34
∅ 5.0 mm, GH 4.0 mm	K2005.5040	34
∅ 5.0 mm, GH 6.0 mm	K2005.5060	34
∅ 6.0 mm, GH 2.0 mm	K2005.6020	34
∅ 6.0 mm, GH 4.0 mm	K2005.6040	34
∅ 6.0 mm, GH 6.0 mm	K2005.6060	34
CAMLOG® Healing cap PS, wide body		
∅ 3.8 mm, GH 4.0 mm	K2004.3840	34
∅ 3.8 mm, GH 6.0 mm	K2004.3860	34
∅ 4.3 mm, GH 4.0 mm	K2004.4340	34
∅ 4.3 mm, GH 6.0 mm	K2004.4360	34
∅ 5.0 mm, GH 4.0 mm	K2004.5040	34
∅ 5.0 mm, GH 6.0 mm	K2004.5060	34
∅ 6.0 mm, GH 4.0 mm	K2004.6040	34
∅ 6.0 mm, GH 6.0 mm	K2004.6060	34
CAMLOG® Healing cap, bottleneck		
∅ 3.3 mm, GH 4.0 mm	J2011.3340	34
∅ 3.8 mm, GH 4.0 mm	J2011.3840	34
∅ 3.8 mm, GH 6.0 mm	J2011.3860	34
∅ 4.3 mm, GH 4.0 mm	J2011.4340	34
∅ 4.3 mm, GH 6.0 mm	J2011.4360	34
∅ 5.0 mm, GH 4.0 mm	J2011.5040	34
∅ 5.0 mm, GH 6.0 mm	J2011.5060	34
∅ 6.0 mm, GH 4.0 mm	J2011.6040	34
∅ 6.0 mm, GH 6.0 mm	J2011.6060	34
CAMLOG® Healing cap, cylindrical		
∅ 3.3 mm, GH 2.0 mm	J2015.3320	34
∅ 3.3 mm, GH 4.0 mm	J2015.3340	34
∅ 3.8 mm, GH 2.0 mm	J2015.3820	34
∅ 3.8 mm, GH 4.0 mm	J2015.3840	34
∅ 3.8 mm, GH 6.0 mm	J2015.3860	34
∅ 4.3 mm, GH 2.0 mm	J2015.4320	34
∅ 4.3 mm, GH 4.0 mm	J2015.4340	34
∅ 4.3 mm, GH 6.0 mm	J2015.4360	34
∅ 5.0 mm, GH 2.0 mm	J2015.5020	34
∅ 5.0 mm, GH 4.0 mm	J2015.5040	34
∅ 5.0 mm, GH 6.0 mm	J2015.5060	34
∅ 6.0 mm, GH 2.0 mm	J2015.6020	34
∅ 6.0 mm, GH 4.0 mm	J2015.6040	34
∅ 6.0 mm, GH 6.0 mm	J2015.6060	34
CAMLOG® Healing cap, wide body		
∅ 3.3 mm, GH 2.0 mm	J2014.3320	34
∅ 3.3 mm, GH 4.0 mm	J2014.3340	34
∅ 3.8 mm, GH 2.0 mm	J2014.3820	34
∅ 3.8 mm, GH 4.0 mm	J2014.3840	34
∅ 3.8 mm, GH 6.0 mm	J2014.3860	34
∅ 4.3 mm, GH 2.0 mm	J2014.4320	34
∅ 4.3 mm, GH 4.0 mm	J2014.4340	34
∅ 4.3 mm, GH 6.0 mm	J2014.4360	34
∅ 5.0 mm, GH 2.0 mm	J2014.5020	34

INDEX

ALPHABETICAL

Article	Article No.	Page
CAMLOG® Healing cap, wide body		
∅ 5.0 mm, GH 4.0 mm	J2014.5040	34
∅ 5.0 mm, GH 6.0 mm	J2014.5060	34
∅ 6.0 mm, GH 2.0 mm	J2014.6020	34
∅ 6.0 mm, GH 4.0 mm	J2014.6040	34
∅ 6.0 mm, GH 6.0 mm	J2014.6060	34
CAMLOG® Impression posts PS, closed tray		
∅ 3.8 mm	K2109.3800	50
∅ 4.3 mm	K2109.4300	50
∅ 5.0 mm	K2109.5000	50
∅ 6.0 mm	K2109.6000	50
CAMLOG® Impression posts PS, open tray		
∅ 3.8 mm	K2119.3800	50
∅ 4.3 mm	K2119.4300	50
∅ 5.0 mm	K2119.5000	50
∅ 6.0 mm	K2119.6000	50
CAMLOG® Impression posts, closed tray		
∅ 3.3 mm	K2110.3300	50
∅ 3.8 mm	K2110.3800	50
∅ 4.3 mm	K2110.4300	50
∅ 5.0 mm	K2110.5000	50
∅ 6.0 mm	K2110.6000	50
CAMLOG® Impression posts, open tray		
∅ 3.3 mm	K2121.3300	50
∅ 3.8 mm	K2121.3800	50
∅ 4.3 mm	K2121.4300	50
∅ 5.0 mm	K2121.5000	50
∅ 6.0 mm	K2121.6000	50
CAMLOG® Lab analogs		
∅ 3.3 mm	K3010.3300	51
∅ 3.8 mm	K3010.3800	51
∅ 4.3 mm	K3010.4300	51
∅ 5.0 mm	K3010.5000	51
∅ 6.0 mm	K3010.6000	51
CAMLOG® Lab screws, hex, brown anodized		
∅ 3.3/3.8/4.3 mm, thread M 1.6	J4006.1601	58, 61, 69
∅ 5.0/6.0 mm, thread M 2.0	J4006.2001	58, 61, 69
CAMLOG® Locator® Abutments		
∅ 3.3 mm, GH 1.0 mm	J2253.3310	66
∅ 3.3 mm, GH 2.0 mm	J2253.3320	66
∅ 3.3 mm, GH 3.0 mm	J2253.3330	66
∅ 3.3 mm, GH 4.0 mm	J2253.3340	66
∅ 3.8 mm, GH 1.0 mm	J2253.3810	66
∅ 3.8 mm, GH 2.0 mm	J2253.3820	66
∅ 3.8 mm, GH 3.0 mm	J2253.3830	66
∅ 3.8 mm, GH 4.0 mm	J2253.3840	66
∅ 3.8 mm, GH 5.0 mm	J2253.3850	66
∅ 4.3 mm, GH 1.0 mm	J2253.4310	66
∅ 4.3 mm, GH 2.0 mm	J2253.4320	66
∅ 4.3 mm, GH 3.0 mm	J2253.4330	66
∅ 4.3 mm, GH 4.0 mm	J2253.4340	66
∅ 4.3 mm, GH 5.0 mm	J2253.4350	66
∅ 5.0 mm, GH 1.0 mm	J2253.5010	66
∅ 5.0 mm, GH 2.0 mm	J2253.5020	66
∅ 5.0 mm, GH 3.0 mm	J2253.5030	66
∅ 5.0 mm, GH 4.0 mm	J2253.5040	66
∅ 5.0 mm, GH 5.0 mm	J2253.5050	66
CAMLOG® Logfit® Abutments		
∅ 3.8 mm, GH 0.8 mm	K2550.3808	56
∅ 3.8 mm, GH 1.5 mm	K2550.3815	56
∅ 4.3 mm, GH 0.8 mm	K2550.4308	56
∅ 4.3 mm, GH 1.5 mm	K2550.4315	56
∅ 5.0 mm, GH 0.8 mm	K2550.5008	56
∅ 5.0 mm, GH 1.5 mm	K2550.5015	56
∅ 6.0 mm, GH 0.8 mm	K2550.6008	56
∅ 6.0 mm, GH 1.5 mm	K2550.6015	56

Article	Article No.	Page
CAMLOG® Modeling aids		
for CAMLOG® Titanium bases CAD/CAM, burn-out		
∅ 3.3 mm	J2244.3302	57
∅ 3.8 mm	J2244.3802	57
∅ 4.3 mm	J2244.4302	57
∅ 5.0 mm	J2244.5002	57
∅ 6.0 mm	J2244.6002	57
CAMLOG® ROOT-LINE 2 Implant, Promote® plus		
∅ 3.3 mm, L 11 mm	K1032.3311	30
∅ 3.3 mm, L 13 mm	K1032.3313	30
∅ 3.3 mm, L 16 mm	K1032.3316	30
∅ 3.8 mm, L 9 mm	K1032.3809	30
∅ 3.8 mm, L 11 mm	K1032.3811	30
∅ 3.8 mm, L 13 mm	K1032.3813	30
∅ 3.8 mm, L 16 mm	K1032.3816	30
∅ 4.3 mm, L 9 mm	K1032.4309	30
∅ 4.3 mm, L 11 mm	K1032.4311	30
∅ 4.3 mm, L 13 mm	K1032.4313	30
∅ 4.3 mm, L 16 mm	K1032.4316	30
∅ 5.0 mm, L 9 mm	K1032.5009	30
∅ 5.0 mm, L 11 mm	K1032.5011	30
∅ 5.0 mm, L 13 mm	K1032.5013	30
∅ 5.0 mm, L 16 mm	K1032.5016	30
∅ 6.0 mm, L 9 mm	K1032.6009	30
∅ 6.0 mm, L 11 mm	K1032.6011	30
∅ 6.0 mm, L 13 mm	K1032.6013	30
∅ 6.0 mm, L 16 mm	K1032.6016	30
CAMLOG® ROOT-LINE 2 Macro model		
Scale 3:1	K8010.1011	75
CAMLOG® ROOT-LINE 2 Implant for practice		
∅ 3.8 mm	K1039.3813	74
∅ 4.3 mm	K1039.4313	74
CAMLOG® Scanbodies, incl. CAMLOG® Abutment screw		
∅ 3.3 mm	K2610.3310	58
∅ 3.8 mm	K2610.3810	58
∅ 4.3 mm	K2610.4310	58
∅ 5.0/6.0 mm	K2610.6010	58
CAMLOG® ScanPosts, incl. CAMLOG® Abutment screw		
∅ 3.3 mm	K2620.3306	58
∅ 3.8 mm	K2620.3806	58
∅ 4.3 mm	K2620.4306	58
∅ 5.0 mm	K2620.5006	58
∅ 6.0 mm	K2620.6006	58
CAMLOG® SCREW-LINE Implant for practice		
∅ 3.8 mm	K1049.3813	74
∅ 4.3 mm	K1049.4313-01	74
CAMLOG® SCREW-LINE Implant, Promote® plus		
∅ 3.3 mm, L 11 mm	K1052.3311	17
∅ 3.3 mm, L 13 mm	K1052.3313	17
∅ 3.3 mm, L 16 mm	K1052.3316	17
∅ 3.8 mm, L 9 mm	K1052.3809	17
∅ 3.8 mm, L 11 mm	K1052.3811	17
∅ 3.8 mm, L 13 mm	K1052.3813	17
∅ 3.8 mm, L 16 mm	K1052.3816	17
∅ 4.3 mm, L 9 mm	K1052.4309	17
∅ 4.3 mm, L 11 mm	K1052.4311	17
∅ 4.3 mm, L 13 mm	K1052.4313	17
∅ 4.3 mm, L 16 mm	K1052.4316	17
∅ 5.0 mm, L 9 mm	K1052.5009	17
∅ 5.0 mm, L 11 mm	K1052.5011	17
∅ 5.0 mm, L 13 mm	K1052.5013	17
∅ 5.0 mm, L 16 mm	K1052.5016	17
∅ 6.0 mm, L 9 mm	K1052.6009	17
∅ 6.0 mm, L 11 mm	K1052.6011	17

Article	Article No.	Page
CAMLOG® SCREW-LINE Implant, Promote® plus		
∅ 6.0 mm, L 13 mm.....	K1052.6013	17
∅ 6.0 mm, L 16 mm.....	K1052.6016	17
CAMLOG® SCREW-LINE Implant, Promote®		
∅ 3.3 mm, L 11 mm.....	K1042.3311	16
∅ 3.3 mm, L 13 mm.....	K1042.3313	16
∅ 3.3 mm, L 16 mm.....	K1042.3316	16
∅ 3.8 mm, L 9 mm.....	K1042.3809	16
∅ 3.8 mm, L 11 mm.....	K1042.3811	16
∅ 3.8 mm, L 13 mm.....	K1042.3813	16
∅ 3.8 mm, L 16 mm.....	K1042.3816	16
∅ 4.3 mm, L 9 mm.....	K1042.4309	16
∅ 4.3 mm, L 11 mm.....	K1042.4311	16
∅ 4.3 mm, L 13 mm.....	K1042.4313	16
∅ 4.3 mm, L 16 mm.....	K1042.4316	16
∅ 5.0 mm, L 9 mm.....	K1042.5009	16
∅ 5.0 mm, L 11 mm.....	K1042.5011	16
∅ 5.0 mm, L 13 mm.....	K1042.5013	16
∅ 5.0 mm, L 16 mm.....	K1042.5016	16
∅ 6.0 mm, L 9 mm.....	K1042.6009	16
∅ 6.0 mm, L 11 mm.....	K1042.6011	16
∅ 6.0 mm, L 13 mm.....	K1042.6013	16
∅ 6.0 mm, L 16 mm.....	K1042.6016	16
CAMLOG® SCREW-LINE Makro model,		
Scale 3:1.....	K8010.1010	75
CAMLOG® Selection abutment kit	K8011.1000	72
CAMLOG® Telescope abutments		
∅ 3.8 mm.....	K2212.3800	69
∅ 4.3 mm.....	K2212.4300	69
∅ 5.0 mm.....	K2212.5000	69
∅ 6.0 mm.....	K2212.6000	69
CAMLOG® Temporary abutments PS		
∅ 3.8 mm.....	K2208.3800	52
∅ 4.3 mm.....	K2208.4300	52
∅ 5.0 mm.....	K2208.5000	52
∅ 6.0 mm.....	K2208.6000	52
CAMLOG® Temporary abutments		
∅ 3.8 mm.....	K2241.3800	52
∅ 4.3 mm.....	K2241.4300	52
∅ 5.0 mm.....	K2241.5000	52
∅ 6.0 mm.....	K2241.6000	52
CAMLOG® Titanium bases CAD/CAM		
∅ 3.3 mm.....	K2244.3348	57
∅ 3.8 mm.....	K2244.3848	57
∅ 4.3 mm.....	K2244.4348	57
∅ 5.0 mm.....	K2244.5048	57
∅ 6.0 mm.....	K2244.6048	57
CAMLOG® Titanium bases,		
for CAMLOG® Ceramic abutment		
∅ 3.3 mm.....	K2242.3342	56
∅ 3.8 mm.....	K2242.3842	56
∅ 4.3 mm.....	K2242.4342	56
∅ 5.0 mm.....	K2242.5042	56
∅ 6.0 mm.....	K2242.6042	56
CAMLOG® Universal abutments PS		
∅ 3.8 mm.....	K2201.3800	55, 69
∅ 4.3 mm.....	K2201.4300	55, 69
∅ 5.0 mm.....	K2201.5000	55, 69
∅ 6.0 mm.....	K2201.6000	55, 69
CAMLOG® Universal abutments		
∅ 3.3 mm.....	K2211.3300	55, 69
∅ 3.8 mm.....	K2211.3800	55, 69
∅ 4.3 mm.....	K2211.4300	55, 69
∅ 5.0 mm.....	K2211.5000	55, 69
∅ 6.0 mm.....	K2211.6000	55, 69

Article	Article No.	Page
CAMLOG® Vario SR abutment screws		
∅ 3.8/4.3 mm, hex, thread M 1.6.....	J4007.1600	61
∅ 5.0/6.0 mm, hex, thread M 2.0.....	J4007.2000	61
CAMLOG® Vario SR abutments, 20° angled,		
incl. CAMLOG® Abutment screw		
∅ 3.8 mm.....	K2561.3800	59
∅ 4.3 mm.....	K2561.4300	59
∅ 5.0 mm.....	K2561.5000	59
∅ 6.0 mm.....	K2561.6000	59
CAMLOG® Vario SR abutments, 30° angled,		
incl. CAMLOG® Abutment screw		
∅ 3.8 mm.....	K2562.3800	59
∅ 4.3 mm.....	K2562.4300	59
∅ 5.0 mm.....	K2562.5000	59
∅ 6.0 mm.....	K2562.6000	59
CAMLOG® Vario SR abutments, straight,		
incl. CAMLOG® Vario SR abutment screw		
∅ 3.8 mm.....	K2560.3808	59
∅ 4.3 mm.....	K2560.4308	59
∅ 5.0 mm.....	K2560.5008	59
∅ 6.0 mm.....	K2560.6008	59
CAMLOG® Vario SR lab screws, hex		
∅ 3.8/4.3 mm.....	J4008.1600	61
∅ 5.0/6.0 mm.....	J4008.2000	61
Cardanic driver (30°)	J5300.0010	37
Cleaning cannula		
for drills with internal irrigation.....	J5002.0020	37
Cleaning needle		
for drills with internal irrigation.....	J5002.0012	37
Collets for zirconium oxide sleeve		
for universal holder		
∅ 3.3/3.8/4.3 mm.....	J3712.4300	70
∅ 5.0/6.0 mm.....	J3712.6000	70
CT-tube for drill ∅ 2.0 mm		
internal diameter 2.1 mm.....	A2002.2000	13
CT-tube for drill ∅ 2.2 mm		
internal diameter 2.3 mm.....	A2222.2200	13

D

Depth stop for form drills SCREW-LINE and ROOT-LINE 2,		
with reduced coil		
∅ 3.3 mm.....	J5015.3300	20, 33
∅ 3.8 mm.....	J5015.3800	20, 33
∅ 4.3 mm.....	J5015.4300	20, 33
∅ 5.0 mm.....	J5015.5000	20, 33
∅ 6.0 mm.....	J5015.6000	20, 33
Depth stop SCREW-LINE		
for pilot drill (J5051.2000) and pre-drill (J5051.2800)		
L 9 mm.....	J5015.0009	19, 32
L 11 mm.....	J5015.0011	19, 32
L 13 mm.....	J5015.0013	19, 32
Drill extension, ISO shaft		
L 26.6 mm, for drills with internal irrigation.....	J5002.0005	29
L 26.5 mm.....	J5002.0006	36
Drill for CT-tube		
(for A2002.2000), ∅ 2.6 mm.....	A2050.2600	13
(for A2222.2200), ∅ 2.8 mm.....	A2050.2800	13
Driver for ball abutment,		
manual/wrench L 18.3 mm.....	J5300.0011	39
Driver for bar abutment		
∅ 3.3/3.8/4.3 mm, L 18.6 mm.....	J5300.0020	39
∅ 5.0/6.0 mm, L 18.6 mm.....	J5300.0025	39

INDEX

ALPHABETICAL

Article	Article No.	Page
Driver for impression post and healing cap for bar abutment		
Ø 3.3/3.8/4.3 mm, L 19.1 mm	J5300.0027	39
Ø 5.0/6.0 mm, L 19.1 mm	J5300.0028	39
Driver for Locator®, manual/wrench, L 24.3 mm	J2253.0001	39
Driver for screw implants, with ISO shaft for angled hand piece L 27.5 mm	J5300.0007	36
Driver, long for screw implants, manual/wrench, L 27.0 mm	J5300.0009	36
Driver, short for screw implants, manual/wrench, L 18.0 mm	J5300.0008	36

E

Edentulous mandible incl. mounting plate	J8070.2050	74
---	------------	----

F

Form drill ROOT-LINE 2

Ø 3.3 mm, L 9 mm	J5055.3309	33
Ø 3.3 mm, L 11 mm	J5055.3311	33
Ø 3.3 mm, L 13 mm	J5055.3313	33
Ø 3.3 mm, L 16 mm	J5055.3316	33
Ø 3.8 mm, L 9 mm	J5055.3809	33
Ø 3.8 mm, L 11 mm	J5055.3811	33
Ø 3.8 mm, L 13 mm	J5055.3813	33
Ø 3.8 mm, L 16 mm	J5055.3816	33
Ø 4.3 mm, L 9 mm	J5055.4309	33
Ø 4.3 mm, L 11 mm	J5055.4311	33
Ø 4.3 mm, L 13 mm	J5055.4313	33
Ø 4.3 mm, L 16 mm	J5055.4316	33
Ø 5.0 mm, L 9 mm	J5055.5009	33
Ø 5.0 mm, L 11 mm	J5055.5011	33
Ø 5.0 mm, L 13 mm	J5055.5013	33
Ø 5.0 mm, L 16 mm	J5055.5016	33
Ø 6.0 mm, L 9 mm	J5055.6009	33
Ø 6.0 mm, L 11 mm	J5055.6011	33
Ø 6.0 mm, L 13 mm	J5055.6013	33
Ø 6.0 mm, L 16 mm	J5055.6016	33

Form drill SCREW-LINE, Cortical bone

Ø 3.3 mm	J5053.3316	21
Ø 3.8 mm	J5053.3816	21
Ø 4.3 mm	J5053.4316	21
Ø 5.0 mm	J5053.5016	21
Ø 6.0 mm	J5053.6016	21

Form drill SCREW-LINE, with reduced coil

Ø 3.3 mm, L 9 mm	J5052.3309	20
Ø 3.3 mm, L 11 mm	J5052.3311	20
Ø 3.3 mm, L 13 mm	J5052.3313	20
Ø 3.3 mm, L 16 mm	J5052.3316	20
Ø 3.8 mm, L 9 mm	J5052.3809	20
Ø 3.8 mm, L 11 mm	J5052.3811	20

Article	Article No.	Page
Form drill SCREW-LINE, with reduced coil		
Ø 3.8 mm, L 13 mm	J5052.3813	20
Ø 3.8 mm, L 16 mm	J5052.3816	20
Ø 4.3 mm, L 9 mm	J5052.4309	20
Ø 4.3 mm, L 11 mm	J5052.4311	20
Ø 4.3 mm, L 13 mm	J5052.4313	20
Ø 4.3 mm, L 16 mm	J5052.4316	20
Ø 5.0 mm, L 9 mm	J5052.5009	20
Ø 5.0 mm, L 11 mm	J5052.5011	20
Ø 5.0 mm, L 13 mm	J5052.5013	20
Ø 5.0 mm, L 16 mm	J5052.5016	20
Ø 6.0 mm, L 9 mm	J5052.6009	20
Ø 6.0 mm, L 11 mm	J5052.6011	20
Ø 6.0 mm, L 13 mm	J5052.6013	20
Ø 6.0 mm, L 16 mm	J5052.6016	20

G

Guide System CAMLOG® Insertion post

Ø 3.3 mm	K2026.3300	29
Ø 3.8 mm	K2026.3800	29
Ø 4.3 mm	K2026.4300	29

Guide System CAMLOG® SCREW-LINE Implant,

Promote® plus

Ø 3.3 mm, L 11 mm	K1053.3311	26
Ø 3.3 mm, L 13 mm	K1053.3313	26
Ø 3.3 mm, L 16 mm	K1053.3316	26
Ø 3.8 mm, L 9 mm	K1053.3809	26
Ø 3.8 mm, L 11 mm	K1053.3811	26
Ø 3.8 mm, L 13 mm	K1053.3813	26
Ø 3.8 mm, L 16 mm	K1053.3816	26
Ø 4.3 mm, L 9 mm	K1053.4309	26
Ø 4.3 mm, L 11 mm	K1053.4311	26
Ø 4.3 mm, L 13 mm	K1053.4313	26
Ø 4.3 mm, L 16 mm	K1053.4316	26

Guide System Check-up pin

Ø 3.3 mm	J5301.3300	29
Ø 3.8/4.3 mm	J5301.4300	29

Guide System Driver,

with ISO shaft for angled hand piece

Ø 3.3/3.8/4.3 mm	J5304.4300	29
------------------------	------------	----

Guide System Form drill, Cortical bone

Ø 3.3 mm, L 11 mm	J5048.3311	28
Ø 3.3 mm, L 13 mm	J5048.3313	28
Ø 3.3 mm, L 16 mm	J5048.3316	28
Ø 3.8 mm, L 9 mm	J5048.3809	28
Ø 3.8 mm, L 11 mm	J5048.3811	28
Ø 3.8 mm, L 13 mm	J5048.3813	28
Ø 3.8 mm, L 16 mm	J5048.3816	28
Ø 4.3 mm, L 9 mm	J5048.4309	28
Ø 4.3 mm, L 11 mm	J5048.4311	28
Ø 4.3 mm, L 13 mm	J5048.4313	28
Ø 4.3 mm, L 16 mm	J5048.4316	28

Guide System Form drill, SCREW-LINE

Ø 3.3 mm, L 16 mm	J5046.3316	27
Ø 3.8 mm, L 16 mm	J5046.3816	27
Ø 4.3 mm, L 16 mm	J5046.4316	27

INDEX

ALPHABETICAL

Article	Article No.	Page
Guide System Gingiva punches, sterile		
Ø 3.3 mm	J5041.3300	28
Ø 3.8 mm	J5041.3800	28
Ø 4.3 mm	J5041.4300	28
Guide System Driver, manual/wrench		
Ø 3.3/3.8/4.3 mm	J5303.4300	29
Guide System Guiding sleeves		
Ø 3.3 mm	J3714.3303	28
Ø 3.8 mm	J3714.3803	28
Ø 4.3 mm	J3714.4303	28
Guide System Pilot drill		
Ø 3.3 mm, L 16 mm	J5044.3316	26
Ø 3.8/4.3 mm, L 16 mm	J5044.4316	26
Guide System Pilot drill set		
Ø 3.3 mm, L 11 mm	J5043.3311	26
Ø 3.3 mm, L 13 mm	J5043.3313	26
Ø 3.8/4.3 mm, L 9 mm	J5043.4309	26
Ø 3.8/4.3 mm, L 11 mm	J5043.4311	26
Ø 3.8/4.3 mm, L 13 mm	J5043.4313	26
Guide System Seating tool		
Ø 3.3 mm	J3716.3300	29
Ø 3.8/4.3 mm	J3716.4300	29
Guide System Surgery set, SCREW-LINE		
Ø 3.3 mm, L 11 mm	J5045.3311	27
Ø 3.3 mm, L 13 mm	J5045.3313	27
Ø 3.8 mm, L 9 mm	J5045.3809	27
Ø 3.8 mm, L 11 mm	J5045.3811	27
Ø 3.8 mm, L 13 mm	J5045.3813	37
Ø 4.3 mm, L 9 mm	J5045.4309	27
Ø 4.3 mm, L 11 mm	J5045.4311	27
Ø 4.3 mm, L 13 mm	J5045.4313	27
Guide System Template drill		
Ø 3.3 mm	J3713.3300	29
Ø 3.8/4.3 mm	J3713.4300	29
H		
Healing caps for bar abutment		
Ø 3.3/3.8/4.3 mm	J2030.4300	62
Ø 5.0/6.0 mm	J2030.6000	62
Holding key for insertion post	J5302.0010	37
Holding pins, for bar abutment/bar lab analog, yellow, for thread M 1.6		
Ø 3.3/3.8/4.3 mm	J2256.1600	64
Holding pins, for bar abutment/bar lab analog, blue, for thread M 2.0		
Ø 5.0/6.0 mm	J2256.2000	64
Holding sleeve for screw implants, color-coded		
Ø 3.3 mm	J5302.3300	37
Ø 3.8 mm	J5302.3800	37
Ø 4.3 mm	J5302.4300	37
I		
Implant Prosthetics, DVD compendium		
	B2012.0100	76
Implant pass		75

Article	Article No.	Page
Impression caps (5 units)		
Ø 3.3 mm	J2111.3300	51
Ø 3.8 mm	J2111.3800	51
Ø 4.3 mm	J2111.4300	51
Ø 5.0 mm	J2111.5000	51
Ø 6.0 mm	J2111.6000	51
Impression posts for bar abutment		
Ø 3.3/3.8/4.3 mm	J2130.4300	62
Ø 5.0/6.0 mm	J2130.6000	62
L		
Lamella retention insert, for matrix CM Dalbo®-Plus		
Ø 3.3/3.8/4.3/5.0 mm	J2250.0007	65
Locator® Analog		
Ø 3.3/3.8/4.3 mm	J2253.0340	66
Ø 5.0 mm	J2253.0350	66
Locator® Angle measurement guide		
	J2253.0003	39
Locator® Block out spacer		
Ø 3.3/3.8/4.3/5.0 mm	J2253.0401	67
Locator® Impression cap		
Ø 3.3/3.8/4.3/5.0 mm	J2253.0200	66
Locator® Instrument, threepart, L 83 mm		
	J2253.0002	39
Locator® Male processing package for extended range		
Ø 3.8/4.3/5.0 mm	J2253.0112	67
Locator® Replacement male for extended range, gray		
Ø 3.8/4.3/5.0 mm	J2253.2000	68
Locator® Replacement male for extended range, green		
Ø 3.8/4.3/5.0 mm	J2253.2004	68
Locator® Replacement male for extended range, orange		
Ø 3.8/4.3/5.0 mm	J2253.2003	68
Locator® Replacement male for extended range, red		
Ø 3.8/4.3/5.0 mm	J2253.2002	68
Locator® Male processing package		
Ø 3.3/3.8/4.3/5.0 mm	J2253.0102	67
Locator® Parallel post		
	J2253.0004	39
Locator® Processing replacement male		
Ø 3.3/3.8/4.3/5.0 mm	J2253.0402	67
Locator® Replacement male, blue		
Ø 3.3/3.8/4.3/5.0 mm	J2253.1002	68
Locator® Replacement male, clear		
Ø 3.3/3.8/4.3/5.0 mm	J2253.1005	68
Locator® Replacement male, pink		
Ø 3.3/3.8/4.3/5.0 mm	J2253.1003	68
Logfit® Analogs		
Ø 3.8/4.3 mm	J2552.4300	56
Ø 5.0/6.0 mm	J2552.6000	56
Logfit® Impression caps		
Ø 3.8/4.3 mm	J2551.4300	56
Ø 5.0/6.0 mm	J2551.6000	56
Logfit® Plastic copings bridge		
Ø 3.8/4.3 mm	J2553.4301	57
Ø 5.0/6.0 mm	J2553.6001	57
Logfit® Plastic copings crown		
Ø 3.8/4.3 mm	J2553.4302	57
Ø 5.0/6.0 mm	J2553.6002	57

INDEX

ALPHABETICAL

Article Article No. Page

M

Matrix CM Dalbo®-Plus, for ball abutment
 Ø 3.3/3.8/4.3/5.0 mm J2250.0005 **65**

O

Osteotome SCREW-LINE, angled concave
 Ø 3.3 mm J5420.3310 **25**
 Ø 3.8 mm J5420.3810 **25**
 Ø 4.3 mm J5420.4310 **25**
 Ø 5.0 mm J5420.5010 **25**
 Ø 6.0 mm J5420.6010 **25**

Osteotome SCREW-LINE, angled convex
 Ø 3.3 mm J5418.3310 **23**
 Ø 3.8 mm J5418.3810 **23**
 Ø 4.3 mm J5418.4310 **23**
 Ø 5.0 mm J5418.5010 **23**
 Ø 6.0 mm J5418.6010 **23**

Osteotome SCREW-LINE, straight concave
 Ø 3.3 mm J5420.3300 **24**
 Ø 3.8 mm J5420.3800 **24**
 Ø 4.3 mm J5420.4300 **24**
 Ø 5.0 mm J5420.5000 **24**
 Ø 6.0 mm J5420.6000 **24**

Osteotome SCREW-LINE, straight convex
 Ø 3.3 mm J5418.3300 **22**
 Ø 3.8 mm J5418.3800 **22**
 Ø 4.3 mm J5418.4300 **22**
 Ø 5.0 mm J5418.5000 **22**
 Ø 6.0 mm J5418.6000 **22**

Osteotomy set CAMLOG®/CONELOG® SCREW-LINE
 angled concave J5420.0030 **25**
 angled convex J5418.0030 **23**
 straight concave J5420.0020 **24**
 straight convex J5418.0020 **22**

P

Paralleling pin SCREW-LINE
 Ø 1.7-2.8/2.0 mm J5300.2028 **36**

Patient brochure **75**

PickUp instrument
 holder for carrying implants J5300.0030 **37**

Pilot drill without coil, resterilizable
 Ø 2.0 mm J5051.2003 **19, 32**

Pilot drill SCREW-LINE, reduced coil
 Ø 2.0 mm J5051.2000 **19**

Pre-drill SCREW-LINE
 Ø 1.7-2.8 mm J5051.2800 **19, 32**

Pre-Osteotome SCREW-LINE, straight concave
 Ø 1.7-2.8 mm J5419.2800 **24, 25**

Pre-Osteotome SCREW-LINE, straight convex
 Ø 1.7-2.8 mm J5417.2800 **22, 23**

Prosthetic screws, for bar abutments, hex
 Ø 3.3/3.8/4.3 mm, thread M 1.6 J4005.1602 **64**
 Ø 5.0/6.0 mm, thread M 2.0 J4005.2002 **64**

Prosthetic set J5330.8600 **38**

Prosthetic tray (without content) J5330.8500 **38**

Article Article No. Page

R

Reamers for dilating the plaster model, for universal holder, incl. color-coded guide pin
 Ø 3.3 mm J3706.3300 **70**
 Ø 3.8 mm J3706.3800 **70**
 Ø 4.3 mm J3706.4300 **70**
 Ø 5.0 mm J3706.5000 **70**
 Ø 6.0 mm J3706.6000 **70**

Reworking reamer, for base for bar abutment, plane surface/cone seat, burn-out
 Ø 3.3/3.8/4.3 mm J3711.0010 **71**
 Ø 5.0/6.0 mm J3711.0015 **71**

Reworking reamer, for base for bar abutment, screw seat, burn-out
 Ø 3.3/3.8/4.3 mm J3711.0020 **71**
 Ø 5.0/6.0 mm J3711.0025 **71**

Round bur
 Ø 2.3 mm J5050.2300 **19, 32**
 Ø 3.5 mm J5050.3500 **19, 32**

S

Screws, hex, for bar abutment
 Ø 3.3/3.8/4.3 mm, thread M 1.6 J4005.1610 **62**
 Ø 5.0/6.0 mm, thread M 2.0 J4005.2010 **62**

Screwdriver
 Activator, for ball abutment matrix CM Dalbo®-Plus J5315.0005 **39**

Screwdriver
 hex, extra short, manual/wrench L 14.5 mm J5316.0510 **38**
 hex, long, ISO shaft L 26.0 mm J5316.0503 **38**
 hex, long, manual/wrench L 30.3 mm J5316.0502 **38**
 hex, short, ISO shaft L 18.0 mm J5316.0504 **38**
 hex, short, manual/wrench L 22.5 mm J5316.0501 **38**

Sleeves for titanium bonding base, burn-out, Passive-Fit
 Ø 3.3 mm J2261.3300 **64**
 Ø 3.8 mm J2261.3800 **64**
 Ø 4.3 mm J2261.4300 **64**
 Ø 5.0 mm J2261.5000 **64**
 Ø 6.0 mm J2261.6000 **64**

Soldering aids/bar lab analogs
 Ø 3.3/3.8/4.3 mm J3020.4300 **62**
 Ø 5.0/6.0 mm J3020.6000 **62**

Surgery set CAMLOG®/CONELOG® SCREW-LINE J5300.0057 **18**

Surgery set CAMLOG® ROOT-LINE 2 J5300.0059 **31**

Surgery tray CAMLOG® ROOT-LINE 2 (without content) J5300.8915 **31**

T

Tap adapter
 for tap SCREW-LINE
 short L 18.0 mm J5322.0010 **36**
 long L 23.0 mm J5322.0011 **36**

Tap ROOT-LINE 2
 Ø 3.3 mm J5056.3309 **33**
 Ø 3.8 mm J5056.3809 **33**
 Ø 4.3 mm J5056.4309 **33**
 Ø 5.0 mm J5056.5009 **33**
 Ø 6.0 mm J5056.6009 **33**

Article	Article No.	Page
Tap SCREW-LINE, with hexagon		
Ø 3.3 mm	J5054.3309	21
Ø 3.8 mm	J5054.3809	21
Ø 4.3 mm	J5054.4309	21
Ø 5.0 mm	J5054.5009	21
Ø 6.0 mm	J5054.6009	21
Titanium bonding bases for bar abutment,		
Passive-Fit		
Ø 3.3 mm	J2260.3300	63
Ø 3.8 mm	J2260.3800	63
Ø 4.3 mm	J2260.4300	63
Ø 5.0 mm	J2260.5000	63
Ø 6.0 mm	J2260.6000	63
Torque wrench	J5320.1030	38
U		
Universal holder	J3709.0015	70
Universal holder, incl. CAMLOG® Abutment collet		
Ø 3.3/3.8/4.3/5.0/6.0 mm	J3709.0010	70
V		
Vario SR aligning tool,		
for insertion posts, Ø 3.8/4.3/5.0/6.0 mm		
20°	J2569.0001	61
30°	J2569.0002	61
Vario SR analog		
Ø 3.8/4.3 mm	J2567.4300	59
Ø 5.0/6.0 mm	J2567.6000	59
Vario SR base for bar, laser-weldable		
Ø 3.8/4.3 mm	J2570.4300	60
Ø 5.0/6.0 mm	J2570.6000	60
Vario SR impression cap, closed tray		
Ø 3.8/4.3 mm	J2565.4300	59
Ø 5.0/6.0 mm	J2565.6000	59
Vario SR impression cap, open tray,		
incl. fixing screw		
Ø 3.8/4.3 mm	J2566.4300	59
Ø 5.0/6.0 mm	J2566.6000	59
Vario SR plastic coping, bridge, burn-out,		
Ø 3.8/4.3 mm	J2563.4301	60
Ø 5.0/6.0 mm	J2563.6001	60
Vario SR plastic coping, crown,		
with single-surface antirotation,		
for angled Vario SR abutments, burn-out		
Ø 3.8/4.3 mm	J2563.4303	60
Ø 5.0/6.0 mm	J2563.6003	60
Vario SR plastic coping, crown,		
with triple-surface antirotation, burn-out		
Ø 3.8/4.3 mm	J2563.4302	60
Ø 5.0/6.0 mm	J2563.6002	60
Vario SR prosthetic screw		
Ø 3.8/4.3/5.0/6.0 mm, thread M 2.0	J4005.2004	61
Vario SR protection cap		
Ø 3.8/4.3 mm	J2568.4300	60
Ø 5.0/6.0 mm	J2568.6000	60
Vario SR titanium cap, bridge		
Ø 3.8/4.3 mm	J2564.4301	60
Ø 5.0/6.0 mm	J2564.6001	60

Article	Article No.	Page
X		
X-Ray Planning foil 1.25:1		
CAMLOG® ROOT-LINE 2 Implants	K5300.9012	12
CAMLOG® SCREW-LINE Implants	K5300.9010	12
X-Ray Planning foil 1.4:1		
CAMLOG® ROOT-LINE 2 Implants	K5300.9013	12
CAMLOG® SCREW-LINE Implants	K5300.9011	12
X-Ray Transfer pictures 1.25:1		
CAMLOG® ROOT-LINE 2 Implants		
planning slide, self-adhesive		
Ø 3.3 mm	K5300.9070	12
Ø 3.8 mm	K5300.9071	12
Ø 4.3 mm	K5300.9072	12
Ø 5.0 mm	K5300.9073	12
Ø 6.0 mm	K5300.9074	12
X-Ray Transfer pictures 1.25:1		
CAMLOG® SCREW-LINE Implants		
planning slide, self-adhesive		
Ø 3.3 mm	K5300.9080	12
Ø 3.8 mm	K5300.9081	12
Ø 4.3 mm	K5300.9082	12
Ø 5.0 mm	K5300.9083	12
Ø 6.0 mm	K5300.9084	12
Z		
Zirconium oxide sleeves, for CAMLOG® Ceramic abutment		
Ø 3.3 mm	J2242.3341	56
Ø 3.8 mm	J2242.3841	56
Ø 4.3 mm	J2242.4341	56
Ø 5.0 mm	J2242.5041	56
Ø 6.0 mm	J2242.6041	56

INDEX

ARTICLE NUMBERS

Article No.	Article	Page	Article No.	Article	Page
A2002.2000	CT-tube for drill \varnothing 2.0 mm internal diameter 2.1 mm	13	J2130.4300	Impression posts for bar abutment \varnothing 3.3/3.8/4.3 mm	62
A2050.2600	Drill for CT-tube \varnothing 2.6 mm	13	J2130.6000	\varnothing 5.0/6.0 mm	62
A2050.2800	\varnothing 2.8 mm	13	J2140.3300	CAMLOG® Bite registration posts \varnothing 3.3 mm	51
A2222.2200	CT-tube for drill \varnothing 2.2 mm internal diameter 2.3 mm	13	J2140.3800	\varnothing 3.8 mm	51
B2012.0100	Implant Prosthetics , DVD compendium	76	J2140.4300	\varnothing 4.3 mm	51
J2011.3340	CAMLOG® Healing cap , bottleneck \varnothing 3.3 mm, GH 4.0 mm	34	J2140.5000	\varnothing 5.0 mm	51
J2011.3840	\varnothing 3.8 mm, GH 4.0 mm	34	J2140.6000	\varnothing 6.0 mm	51
J2011.3860	\varnothing 3.8 mm, GH 6.0 mm	34	J2242.3341	Zirconium oxide sleeves , for CAMLOG® Ceramic abutment \varnothing 3.3 mm	56
J2011.4340	\varnothing 4.3 mm, GH 4.0 mm	34	J2242.3841	\varnothing 3.8 mm	56
J2011.4360	\varnothing 4.3 mm, GH 6.0 mm	34	J2242.4341	\varnothing 4.3 mm	56
J2011.5040	\varnothing 5.0 mm, GH 4.0 mm	34	J2242.5041	\varnothing 5.0 mm	56
J2011.5060	\varnothing 5.0 mm, GH 6.0 mm	34	J2242.6041	\varnothing 6.0 mm	56
J2011.6040	\varnothing 6.0 mm, GH 4.0 mm	34	J2244.3302	CAMLOG® Modeling aids for CAMLOG® Titanium bases CAD/CAM , burn-out \varnothing 3.3 mm	57
J2011.6060	\varnothing 6.0 mm, GH 6.0 mm	34	J2244.3802	\varnothing 3.8 mm	57
J2014.3320	CAMLOG® Healing cap , wide body \varnothing 3.3 mm, GH 2.0 mm	34	J2244.4302	\varnothing 4.3 mm	57
J2014.3340	\varnothing 3.3 mm, GH 4.0 mm	34	J2244.5002	\varnothing 5.0 mm	57
J2014.3820	\varnothing 3.8 mm, GH 2.0 mm	34	J2244.6002	\varnothing 6.0 mm	57
J2014.3840	\varnothing 3.8 mm, GH 4.0 mm	34	J2249.3315	CAMLOG® Ball abutments, male part \varnothing 3.3 mm, GH 1.5 mm	65
J2014.3860	\varnothing 3.8 mm, GH 6.0 mm	34	J2249.3330	\varnothing 3.3 mm, GH 3.0 mm	65
J2014.4320	\varnothing 4.3 mm, GH 2.0 mm	34	J2249.3815	\varnothing 3.8 mm, GH 1.5 mm	65
J2014.4340	\varnothing 4.3 mm, GH 4.0 mm	34	J2249.3830	\varnothing 3.8 mm, GH 3.0 mm	65
J2014.4360	\varnothing 4.3 mm, GH 6.0 mm	34	J2249.3845	\varnothing 3.8 mm, GH 4.5 mm	65
J2014.5020	\varnothing 5.0 mm, GH 2.0 mm	34	J2249.4315	\varnothing 4.3 mm, GH 1.5 mm	65
J2014.5040	\varnothing 5.0 mm, GH 4.0 mm	34	J2249.4330	\varnothing 4.3 mm, GH 3.0 mm	65
J2014.5060	\varnothing 5.0 mm, GH 6.0 mm	34	J2249.4345	\varnothing 4.3 mm, GH 4.5 mm	65
J2014.6020	\varnothing 6.0 mm, GH 2.0 mm	34	J2249.5015	\varnothing 5.0 mm, GH 1.5 mm	65
J2014.6040	\varnothing 6.0 mm, GH 4.0 mm	34	J2249.5030	\varnothing 5.0 mm, GH 3.0 mm	65
J2014.6060	\varnothing 6.0 mm, GH 6.0 mm	34	J2249.5045	\varnothing 5.0 mm, GH 4.5 mm	65
J2015.3320	CAMLOG® Healing cap , cylindrical \varnothing 3.3 mm, GH 2.0 mm	34	J2250.0005	Matrix CM Dalbo®-Plus , for ball abutment \varnothing 3.3/3.8/4.3/5.0 mm	65
J2015.3340	\varnothing 3.3 mm, GH 4.0 mm	34	J2250.0007	Lamella retention insert , for matrix CM Dalbo®-Plus \varnothing 3.3/3.8/4.3/5.0 mm	65
J2015.3820	\varnothing 3.8 mm, GH 2.0 mm	34	J2250.0007	\varnothing 3.3/3.8/4.3/5.0 mm	65
J2015.3840	\varnothing 3.8 mm, GH 4.0 mm	34	J2250.3315	CAMLOG® Ball abutment sets , incl. male part and matrix CM Dalbo®-Plus \varnothing 3.3 mm, GH 1.5 mm	64
J2015.3860	\varnothing 3.8 mm, GH 6.0 mm	34	J2250.3330	\varnothing 3.3 mm, GH 3.0 mm	64
J2015.4320	\varnothing 4.3 mm, GH 2.0 mm	34	J2250.3815	\varnothing 3.8 mm, GH 1.5 mm	64
J2015.4340	\varnothing 4.3 mm, GH 4.0 mm	34	J2250.3830	\varnothing 3.8 mm, GH 3.0 mm	64
J2015.4360	\varnothing 4.3 mm, GH 6.0 mm	34	J2250.3845	\varnothing 3.8 mm, GH 4.5 mm	64
J2015.5020	\varnothing 5.0 mm, GH 2.0 mm	34	J2250.4315	\varnothing 4.3 mm, GH 1.5 mm	64
J2015.5040	\varnothing 5.0 mm, GH 4.0 mm	34	J2250.4330	\varnothing 4.3 mm, GH 3.0 mm	64
J2015.5060	\varnothing 5.0 mm, GH 6.0 mm	34	J2250.4345	\varnothing 4.3 mm, GH 4.5 mm	64
J2015.6020	\varnothing 6.0 mm, GH 2.0 mm	34	J2250.5015	\varnothing 5.0 mm, GH 1.5 mm	64
J2015.6040	\varnothing 6.0 mm, GH 4.0 mm	34	J2250.5030	\varnothing 5.0 mm, GH 3.0 mm	64
J2015.6060	\varnothing 6.0 mm, GH 6.0 mm	34	J2250.5045	\varnothing 5.0 mm, GH 4.5 mm	64
J2030.4300	Healing caps for bar abutment \varnothing 3.3/3.8/4.3 mm	62	J2253.0001	Driver for Locator® , manual/wrench L 24.3 mm	39
J2030.6000	\varnothing 5.0/6.0 mm	62	J2253.0002	Locator® Instrument , threepart.....	39
J2111.3300	Impression caps (5 units) \varnothing 3.3 mm	51	J2253.0003	Locator® Angle measurement guide	39
J2111.3800	\varnothing 3.8 mm	51	J2253.0004	Locator® Parallel post	39
J2111.4300	\varnothing 4.3 mm	51	J2253.0102	Locator® Male processing package \varnothing 3.3/3.8/4.3/5.0 mm	67
J2111.5000	\varnothing 5.0 mm	51	J2253.0112	Locator® Male processing package , for extended range \varnothing 3.8/4.3/5.0 mm	67
J2111.6000	\varnothing 6.0 mm	51	J2253.0200	Locator® Impression cap \varnothing 3.3/3.8/4.3/5.0 mm	66
J2112.3300	Bite registration caps (5 units) \varnothing 3.3 mm	51	J2253.0340	Locator® Analog \varnothing 3.3/3.8/4.3 mm	66
J2112.3800	\varnothing 3.8 mm	51	J2253.0350	\varnothing 5.0 mm	66
J2112.4300	\varnothing 4.3 mm	51			
J2112.5000	\varnothing 5.0 mm	51			
J2112.6000	\varnothing 6.0 mm	51			

INDEX

ARTICLE NUMBERS

Article No.	Article	Page	Article No.	Article	Page
	Locator® Block out spacer			Bases for bar abutment, burn-out	
J2253.0401	∅ 3.3/3.8/4.3/5.0 mm	67	J2257.3300	∅ 3.3 mm	63
	Locator® Processing replacement male		J2257.3800	∅ 3.8 mm	63
J2253.0402	∅ 3.3/3.8/4.3/5.0 mm	67	J2257.4300	∅ 4.3 mm	63
	Locator® Replacement male, blue		J2257.5000	∅ 5.0 mm	63
J2253.1002	∅ 3.3/3.8/4.3/5.0 mm	68	J2257.6000	∅ 6.0 mm	63
	Locator® Replacement male, pink			Bases for bar abutment, solderable	
J2253.1003	∅ 3.3/3.8/4.3/5.0 mm	68	J2258.4300	∅ 3.3/3.8/4.3 mm	63
	Locator® Replacement male, clear		J2258.6000	∅ 5.0/6.0 mm	63
J2253.1005	∅ 3.3/3.8/4.3/5.0 mm	68		Titanium bonding bases for bar abutment, Passive-Fit	
	Locator® Replacement male for extended range, gray		J2260.3300	∅ 3.3 mm	63
J2253.2000	∅ 3.8/4.3/5.0 mm	68	J2260.3800	∅ 3.8 mm	63
	Locator® Replacement male for extended range, red		J2260.4300	∅ 4.3 mm	63
J2253.2002	∅ 3.8/4.3/5.0 mm	68	J2260.5000	∅ 5.0 mm	63
	Locator® Replacement male for extended range, orange		J2260.6000	∅ 6.0 mm	63
J2253.2003	∅ 3.8/4.3/5.0 mm	68		Sleeves for titanium bonding base, burn-out Passive-Fit	
	Locator® Replacement male for extended range, green		J2261.3300	∅ 3.3 mm	64
J2253.2004	∅ 3.8/4.3/5.0 mm	68	J2261.3800	∅ 3.8 mm	64
	CAMLOG® Locator® Abutments		J2261.4300	∅ 4.3 mm	64
J2253.3310	∅ 3.3 mm, GH 1.0 mm	66	J2261.5000	∅ 5.0 mm	64
J2253.3320	∅ 3.3 mm, GH 2.0 mm	66	J2261.6000	∅ 6.0 mm	64
J2253.3330	∅ 3.3 mm, GH 3.0 mm	66		Bases for bar abutment, laser-weldable	
J2253.3340	∅ 3.3 mm, GH 4.0 mm	66	J2262.4300	∅ 3.3/3.8/4.3 mm	63
J2253.3810	∅ 3.8 mm, GH 1.0 mm	66	J2262.6000	∅ 5.0/6.0 mm	63
J2253.3820	∅ 3.8 mm, GH 2.0 mm	66		Bases for bar abutment, cast-on	
J2253.3830	∅ 3.8 mm, GH 3.0 mm	66	J2263.4300	∅ 3.3/3.8/4.3 mm	63
J2253.3840	∅ 3.8 mm, GH 4.0 mm	66	J2263.6000	∅ 5.0/6.0 mm	63
J2253.3850	∅ 3.8 mm, GH 5.0 mm	66		Logfit® Impression caps	
J2253.4310	∅ 4.3 mm, GH 1.0 mm	66	J2551.4300	∅ 3.8/4.3 mm	56
J2253.4320	∅ 4.3 mm, GH 2.0 mm	66	J2551.6000	∅ 5.0/6.0 mm	56
J2253.4330	∅ 4.3 mm, GH 3.0 mm	66		Logfit® Analogs	
J2253.4340	∅ 4.3 mm, GH 4.0 mm	66	J2552.4300	∅ 3.8/4.3 mm	56
J2253.4350	∅ 4.3 mm, GH 5.0 mm	66	J2552.6000	∅ 5.0/6.0 mm	56
J2253.5010	∅ 5.0 mm, GH 1.0 mm	66		Logfit® Plastic copings, bridge	
J2253.5020	∅ 5.0 mm, GH 2.0 mm	66	J2553.4301	∅ 3.8/4.3 mm	57
J2253.5030	∅ 5.0 mm, GH 3.0 mm	66	J2553.6001	∅ 5.0/6.0 mm	57
J2253.5040	∅ 5.0 mm, GH 4.0 mm	66		Logfit® Plastic copings, crown	
J2253.5050	∅ 5.0 mm, GH 5.0 mm	66	J2553.4302	∅ 3.8/4.3 mm	57
	CAMLOG® Bar abutments		J2553.6002	∅ 5.0/6.0 mm	57
J2255.3305	∅ 3.3 mm, GH 0.5 mm	62		Vario SR plastic coping, bridge, burn-out	
J2255.3320	∅ 3.3 mm, GH 2.0 mm	62	J2563.4301	∅ 3.8/4.3 mm	60
J2255.3805	∅ 3.8 mm, GH 0.5 mm	62	J2563.6001	∅ 5.0/6.0 mm	60
J2255.3820	∅ 3.8 mm, GH 2.0 mm	62		Vario SR plastic coping, crown, with triple-surface antirotation, burn-out	
J2255.3840	∅ 3.8 mm, GH 4.0 mm	62	J2563.4302	∅ 3.8/4.3 mm	60
J2255.4305	∅ 4.3 mm, GH 0.5 mm	62	J2563.6002	∅ 5.0/6.0 mm	60
J2255.4320	∅ 4.3 mm, GH 2.0 mm	62		Vario SR plastic coping, crown, with single-surface antirotation, burn-out	
J2255.4340	∅ 4.3 mm, GH 4.0 mm	62	J2563.4303	∅ 3.8/4.3 mm	60
J2255.5005	∅ 5.0 mm, GH 0.5 mm	62	J2563.6003	∅ 5.0/6.0 mm	60
J2255.5020	∅ 5.0 mm, GH 2.0 mm	62		Vario SR titanium cap, bridge	
J2255.5040	∅ 5.0 mm, GH 4.0 mm	62	J2564.4301	∅ 3.8/4.3 mm	60
J2255.6005	∅ 6.0 mm, GH 0.5 mm	62	J2564.6001	∅ 5.0/6.0 mm	60
J2255.6020	∅ 6.0 mm, GH 2.0 mm	62		Vario SR impression cap, closed tray	
J2255.6040	∅ 6.0 mm, GH 4.0 mm	62	J2565.4300	∅ 3.8/4.3 mm	59
	Holding pins, for bar abutment/bar lab analog, yellow, thread M 1.6		J2565.6000	∅ 5.0/6.0 mm	59
J2256.1600	∅ 3.3/3.8/4.3 mm	64		Vario SR impression cap, open tray, incl. fixing screw	
	Holding pins, for bar abutment/bar lab analog, blue, Thread M 2.0		J2566.4300	∅ 3.8/4.3 mm	59
J2256.2000	∅ 5.0/6.0 mm	64	J2566.6000	∅ 5.0/6.0 mm	59
				Vario SR analog	
			J2567.4300	∅ 3.8/4.3 mm	59
			J2567.6000	∅ 5.0/6.0 mm	59

INDEX

ARTICLE NUMBERS

Article No.	Article	Page	Article No.	Article	Page
	Vario SR protection cap			Screw , for bar abutment, hex	
J2568.4300	∅ 3.8/4.3 mm	60	J4005.1610	∅ 3.3/3.8/4.3 mm, thread M 1.6	62
J2568.6000	∅ 5.0/6.0 mm	60		Prosthetic screw , for bar abutment, hex	
	Vario SR aligning tool ,		J4005.2002	∅ 5.0/6.0 mm, thread M 2.0	64
	for insertion post, ∅ 3.8/4.3/5.0/6.0 mm			Vario SR prosthetic screw ,	
J2569.0001	20°	61	J4005.2004	∅ 3.8/4.3/5.0/6.0 mm, thread M 2.0	61
J2569.0002	30°	61		Screw , for bar abutment, hex	
	Vario SR base for bar, laser-weldable		J4005.2010	∅ 5.0/6.0 mm, thread M 2.0	62
J2570.4300	∅ 3.8/4.3 mm	60		CAMLOG® Lab screws, hex , brown anodized	
J2570.6000	∅ 5.0/6.0 mm	60	J4006.1601	∅ 3.3/3.8/4.3 mm, thread M 1.6	58, 61, 69
	Ball abutment analogs		J4006.2001	∅ 5.0/6.0 mm, thread M 2.0	58, 61, 69
J3015.3300	∅ 3.3 mm	65		CAMLOG® Vario SR abutment screws, hex	
J3015.3800	∅ 3.8 mm	65	J4007.1600	∅ 3.8/4.3 mm, thread M 1.6	61
J3015.4300	∅ 4.3 mm	65	J4007.2000	∅ 5.0/6.0 mm, thread M 2.0	61
J3015.5000	∅ 5.0 mm	65		CAMLOG® Vario SR lab screws, hex	
	Soldering aids/bar lab analogs ,		J4008.1600	∅ 3.8/4.3 mm, thread M 1.6	61
	for bar abutments		J4008.2000	∅ 5.0/6.0 mm, thread M 2.0	61
J3020.4300	∅ 3.3/3.8/4.3 mm	62		CAMLOG® Bonding aids, hex	
J3020.6000	∅ 5.0/6.0 mm	62	J4009.1600	∅ 3.3/3.8/4.3 mm, thread M 1.6	58
	Reamers for dilating the plaster model ,		J4009.2000	∅ 5.0/6.0 mm, thread M 2.0	58
	incl. color-coded guide pin			Drill extension, ISO shaft	
J3706.3300	∅ 3.3 mm	70	J5002.0005	L 26.6 mm, for drills with internal irrigation	29
J3706.3800	∅ 3.8 mm	70	J5002.0006	L 26.5 mm	36
J3706.4300	∅ 4.3 mm	70	J5002.0011	Adapter , ISO shaft for angled hand piece	37
J3706.5000	∅ 5.0 mm	70	J5002.0012	Cleaning needle for drills with internal irrigation...	37
J3706.6000	∅ 6.0 mm	70	J5002.0020	Cleaning cannula for drills with internal irrigation..	37
	Universal holder ,			Depth stop SCREW-LINE for pilot drill	
	incl. CAMLOG® Abutment collet			(J5051.2000) and pre-drill (J5051.2800)	
J3709.0010	∅ 3.3/3.8/4.3/5.0/6.0 mm	70	J5015.0009	L 9 mm	19, 32
J3709.0015	Universal holder	70	J5015.0011	L 11 mm	19, 32
	CAMLOG® Abutment collets,		J5015.0013	L 13 mm	19, 32
	for universal holder			Depth stop for form drills SCREW-LINE,	
J3709.3300	∅ 3.3 mm	70		and ROOT-LINE 2 , with reduced coil	
J3709.3800	∅ 3.8 mm	70	J5015.3300	∅ 3.3 mm	20, 33
J3709.4300	∅ 4.3 mm	70	J5015.3800	∅ 3.8 mm	20, 33
J3709.5000	∅ 5.0 mm	70	J5015.4300	∅ 4.3 mm	20, 33
J3709.6000	∅ 6.0 mm	70	J5015.5000	∅ 5.0 mm	20, 33
	Reworking reamer, for base for bar abutment ,		J5015.6000	∅ 6.0 mm	20, 33
	plane surface/cone seat, burn-out			Guide System Gingiva punches	
J3711.0010	∅ 3.3/3.8/4.3 mm	71	J5041.3300	∅ 3.3 mm	28
J3711.0015	∅ 5.0/6.0 mm	71	J5041.3800	∅ 3.8 mm	28
	Reworking reamer, for base for bar abutment ,		J5041.4300	∅ 4.3 mm	28
	screw seat, burn-out			Guide System Pilot drill set	
J3711.0020	∅ 3.3/3.8/4.3 mm	71	J5043.3311	∅ 3.3 mm, L 11 mm	26
J3711.0025	∅ 5.0/6.0 mm	71	J5043.3313	∅ 3.3 mm, L 13 mm	26
	Collets for zirconium oxide sleeve ,		J5043.4309	∅ 3.8/4.3 mm, L 9 mm	26
	for universal holder		J5043.4311	∅ 3.8/4.3 mm, L 11 mm	26
J3712.4300	∅ 3.3/3.8/4.3 mm	70	J5043.4313	∅ 3.8/4.3 mm, L 13 mm	26
J3712.6000	∅ 5.0/6.0 mm	70		Guide System Pilot drill	
	Guide System Template drill		J5044.3316	∅ 3.3 mm, L 16 mm	26
J3713.3300	∅ 3.3 mm	29	J5044.4316	∅ 3.8/4.3 mm, L 16 mm	26
J3713.4300	∅ 3.8/4.3 mm	29		Guide System Surgery set, SCREW-LINE	
	Guide System Guiding sleeves		J5045.3311	∅ 3.3 mm, L 11 mm	27
J3714.3303	∅ 3.3 mm	28	J5045.3313	∅ 3.3 mm, L 13 mm	27
J3714.3803	∅ 3.8 mm	28	J5045.3809	∅ 3.8 mm, L 9 mm	27
J3714.4303	∅ 4.3 mm	28	J5045.3811	∅ 3.8 mm, L 11 mm	27
	Guide System Seating tool		J5045.3813	∅ 3.8 mm, L 13 mm	27
J3716.3300	∅ 3.3 mm	29	J5045.4309	∅ 4.3 mm, L 9 mm	27
J3716.4300	∅ 3.8/4.3 mm	29	J5045.4311	∅ 4.3 mm, L 11 mm	27
	CAMLOG® Abutment screws, hex		J5045.4313	∅ 4.3 mm, L 13 mm	27
J4005.1601	∅ 3.3/3.8/4.3 mm, thread M 1.6	58, 61, 69			
J4005.2001	∅ 5.0/6.0 mm, thread M 2.0	58, 61, 69			
	Prosthetic screw , for bar abutment, hex				
J4005.1602	∅ 3.3/3.8/4.3 mm, thread M 1.6	64			

INDEX

ARTICLE NUMBERS

Article No.	Article	Page	Article No.	Article	Page
	Guide System Form drill, SCREW-LINE			Form drill ROOT-LINE 2, with reduced coil	
J5046.3316	∅ 3.3 mm, L 16 mm	27	J5055.3309	∅ 3.3 mm, L 9 mm	33
J5046.3816	∅ 3.8 mm, L 16 mm	27	J5055.3311	∅ 3.3 mm, L 11 mm	33
J5046.4316	∅ 4.3 mm, L 16 mm	27	J5055.3313	∅ 3.3 mm, L 13 mm	33
	Guide System Form drill, Cortical bone		J5055.3316	∅ 3.3 mm, L 16 mm	33
J5048.3311	∅ 3.3 mm, L 11 mm	28	J5055.3809	∅ 3.8 mm, L 9 mm	33
J5048.3313	∅ 3.3 mm, L 13 mm	28	J5055.3811	∅ 3.8 mm, L 11 mm	33
J5048.3316	∅ 3.3 mm, L 16 mm	28	J5055.3813	∅ 3.8 mm, L 13 mm	33
J5048.3809	∅ 3.8 mm, L 9 mm	28	J5055.3816	∅ 3.8 mm, L 16 mm	33
J5048.3811	∅ 3.8 mm, L 11 mm	28	J5055.4309	∅ 4.3 mm, L 9 mm	33
J5048.3813	∅ 3.8 mm, L 13 mm	28	J5055.4311	∅ 4.3 mm, L 11 mm	33
J5048.3816	∅ 3.8 mm, L 16 mm	28	J5055.4313	∅ 4.3 mm, L 13 mm	33
J5048.4309	∅ 4.3 mm, L 9 mm	28	J5055.4316	∅ 4.3 mm, L 16 mm	33
J5048.4311	∅ 4.3 mm, L 11 mm	28	J5055.5009	∅ 5.0 mm, L 9 mm	33
J5048.4313	∅ 4.3 mm, L 13 mm	28	J5055.5011	∅ 5.0 mm, L 11 mm	33
J5048.4316	∅ 4.3 mm, L 16 mm	28	J5055.5013	∅ 5.0 mm, L 13 mm	33
	Round bur		J5055.5016	∅ 5.0 mm, L 16 mm	33
J5050.2300	∅ 2.3 mm	19, 32	J5055.6009	∅ 6.0 mm, L 9 mm	33
J5050.3500	∅ 3.5 mm	19, 32	J5055.6011	∅ 6.0 mm, L 11 mm	33
	Pilot drill SCREW-LINE,		J5055.6013	∅ 6.0 mm, L 13 mm	33
	reduced coil		J5055.6016	∅ 6.0 mm, L 16 mm	33
J5051.2000	∅ 2.0 mm	19, 32		Tap ROOT-LINE 2, with hexagon	
	Pilot drill without coil		J5056.3309	∅ 3.3 mm	33
J5051.2003	∅ 2.0 mm	19, 32	J5056.3809	∅ 3.8 mm	33
	Pre-drill SCREW-LINE		J5056.4309	∅ 4.3 mm	33
J5051.2800	∅ 1.7-2.8 mm	19, 32	J5056.5009	∅ 5.0 mm	33
	Form drill SCREW-LINE,		J5056.6009	∅ 6.0 mm	33
	reduced coil			Driver for screw implants,	
J5052.3309	∅ 3.3 mm, L 9 mm	20		with ISO shaft for angled hand piece	
J5052.3311	∅ 3.3 mm, L 11 mm	20	J5300.0007	L 27.5 mm	36
J5052.3313	∅ 3.3 mm, L 13 mm	20		Driver, short, for screw implants,	
J5052.3316	∅ 3.3 mm, L 16 mm	20	J5300.0008	L 18.0 mm	36
J5052.3809	∅ 3.8 mm, L 9 mm	20		Driver, long, for screw implants,	
J5052.3811	∅ 3.8 mm, L 11 mm	20	J5300.0009	L 27.0 mm	36
J5052.3813	∅ 3.8 mm, L 13 mm	20	J5300.0010	Cardanic driver (30°)	37
J5052.3816	∅ 3.8 mm, L 16 mm	20		Driver for ball abutment,	
J5052.4309	∅ 4.3 mm, L 9 mm	20	J5300.0011	L 18.3 mm	39
J5052.4311	∅ 4.3 mm, L 11 mm	20		Driver for bar abutment	
J5052.4313	∅ 4.3 mm, L 13 mm	20	J5300.0020	∅ 3.3/3.8/4.3 mm, L 18.6 mm	39
J5052.4316	∅ 4.3 mm, L 16 mm	20	J5300.0025	∅ 5.0/6.0 mm, L 18.6 mm	39
J5052.5009	∅ 5.0 mm, L 9 mm	20		Driver for impression post and healing cap	
J5052.5011	∅ 5.0 mm, L 11 mm	20		for bar abutment	
J5052.5013	∅ 5.0 mm, L 13 mm	20	J5300.0027	∅ 3.3/3.8/4.3 mm, L 19.1 mm	39
J5052.5016	∅ 5.0 mm, L 16 mm	20	J5300.0028	∅ 5.0/6.0 mm, L 19.1 mm	39
J5052.6009	∅ 6.0 mm, L 9 mm	20		PickUp instrument	
J5052.6011	∅ 6.0 mm, L 11 mm	20	J5300.0030	holder for carrying implants	37
J5052.6013	∅ 6.0 mm, L 13 mm	20	J5300.0057	Surgery set CAMLOG®/CONOLOG® SCREW-LINE ..	18
J5052.6016	∅ 6.0 mm, L 16 mm	20	J5300.0059	Surgery set CAMLOG® ROOT-LINE 2	31
	Form drill SCREW-LINE, Cortical bone			Paralleling pin SCREW-LINE	
J5053.3316	∅ 3.3 mm	21	J5300.2028	∅ 1.7-2.8/2.0 mm	36
J5053.3816	∅ 3.8 mm	21	J5300.8915	Surgery tray CAMLOG® ROOT-LINE 2 (without content)	31
J5053.4316	∅ 4.3 mm	21		Guide System Check-up pin	
J5053.5016	∅ 5.0 mm	21	J5301.3300	∅ 3.3 mm	29
J5053.6016	∅ 6.0 mm	21	J5301.4300	∅ 3.8/4.3 mm	29
	Tap SCREW-LINE, with hexagon		J5302.0010	Holding key for insertion post	37
J5054.3309	∅ 3.3 mm	21		Holding sleeve for screw implants, color-coded	
J5054.3809	∅ 3.8 mm	21	J5302.3300	∅ 3.3 mm	37
J5054.4309	∅ 4.3 mm	21	J5302.3800	∅ 3.8 mm	37
J5054.5009	∅ 5.0 mm	21	J5302.4300	∅ 4.3 mm	37
J5054.6009	∅ 6.0 mm	21			

INDEX

ARTICLE NUMBERS

Article No.	Article	Page
	Guide System Driver, manual/wrench	
J5303.4300	3.3/3.8/4.3 mm.....	29
	Guide System Driver, with ISO shaft for angled hand piece	
J5304.4300	3.3/3.8/4.3 mm.....	29
	Screwdriver Activator, for ball abutment matrix CM Dalbo®-Plus	39
	Screwdriver, hex	
J5316.0501	short, manual/wrench, L 22.5 mm	38
J5316.0502	long, manual/wrench, L 30.3 mm	38
J5316.0503	long, ISO shaft, L 26.0 mm	38
J5316.0504	short, ISO shaft, L 18.0 mm	38
J5316.0510	extra short, manual/wrench, L 14.5 mm	38
J5320.1030	Torque wrench, with continuous torque adjustment until maximal 30 Ncm	38
	Tap adapter, short for tap SCREW-LINE L 18.0 mm	36
J5322.0010		
	Tap adapter, long for tap SCREW-LINE L 23.0 mm	36
J5322.0011		
J5330.8500	Prosthetic tray (without content).....	38
J5330.8600	Prosthetic set	38
	Pre-Osteotome SCREW-LINE, straight convex	
J5417.2800	∅ 1.7-2.8 mm.....	22, 23
	Osteotomy set CAMLOG®/CONELOG® SCREW-LINE,	
J5418.0020	straight convex.....	22
J5418.0030	angled convex.....	23
J5420.0020	straight concave.....	24
J5420.0030	angled concave.....	25
	Osteotome SCREW-LINE, straight convex	
J5418.3300	∅ 3.3 mm	22
J5418.3800	∅ 3.8 mm	22
J5418.4300	∅ 4.3 mm	22
J5418.5000	∅ 5.0 mm	22
J5418.6000	∅ 6.0 mm	22
	Osteotome SCREW-LINE, angled convex	
J5418.3310	∅ 3.3 mm	23
J5418.3810	∅ 3.8 mm	23
J5418.4310	∅ 4.3 mm	23
J5418.5010	∅ 5.0 mm	23
J5418.6010	∅ 6.0 mm	23
	Pre-Osteotome SCREW-LINE, straight concave	
J5419.2800	∅ 1.7-2.8 mm.....	24, 25
	Osteotome SCREW-LINE, straight concave	
J5420.3300	∅ 3.3 mm	24
J5420.3800	∅ 3.8 mm	24
J5420.4300	∅ 4.3 mm	24
J5420.5000	∅ 5.0 mm	24
J5420.6000	∅ 6.0 mm	24
	Osteotome SCREW-LINE, angled concave	
J5420.3310	∅ 3.3 mm	25
J5420.3810	∅ 3.8 mm	25
J5420.4310	∅ 4.3 mm	25
J5420.5010	∅ 5.0 mm	25
J5420.6010	∅ 6.0 mm	25
J8070.2050	Edentulous mandible incl. mounting plate	74

Article No.	Article	Page
	CAMLOG® ROOT-LINE 2 Implant, Promote® plus	
K1032.3311	∅ 3.3 mm, L 11 mm	30
K1032.3313	∅ 3.3 mm, L 13 mm	30
K1032.3316	∅ 3.3 mm, L 16 mm	30
K1032.3809	∅ 3.8 mm, L 9 mm	30
K1032.3811	∅ 3.8 mm, L 11 mm	30
K1032.3813	∅ 3.8 mm, L 13 mm	30
K1032.3816	∅ 3.8 mm, L 16 mm	30
K1032.4309	∅ 4.3 mm, L 9 mm	30
K1032.4311	∅ 4.3 mm, L 11 mm	30
K1032.4313	∅ 4.3 mm, L 13 mm	30
K1032.4316	∅ 4.3 mm, L 16 mm	30
K1032.5009	∅ 5.0 mm, L 9 mm	30
K1032.5011	∅ 5.0 mm, L 11 mm	30
K1032.5013	∅ 5.0 mm, L 13 mm	30
K1032.5016	∅ 5.0 mm, L 16 mm	30
K1032.6009	∅ 6.0 mm, L 9 mm	30
K1032.6011	∅ 6.0 mm, L 11 mm	30
K1032.6013	∅ 6.0 mm, L 13 mm	30
K1032.6016	∅ 6.0 mm, L 16 mm	30
	CAMLOG® ROOT-LINE 2 Implant for practice	
K1039.3813	∅ 3.8 mm	74
K1039.4313	∅ 4.3 mm	74
	CAMLOG® SCREW-LINE Implant, Promote®	
K1042.3311	∅ 3.3 mm, L 11 mm	16
K1042.3313	∅ 3.3 mm, L 13 mm	16
K1042.3316	∅ 3.3 mm, L 16 mm	16
K1042.3809	∅ 3.8 mm, L 9 mm	16
K1042.3811	∅ 3.8 mm, L 11 mm	16
K1042.3813	∅ 3.8 mm, L 13 mm	16
K1042.3816	∅ 3.8 mm, L 16 mm	16
K1042.4309	∅ 4.3 mm, L 9 mm	16
K1042.4311	∅ 4.3 mm, L 11 mm	16
K1042.4313	∅ 4.3 mm, L 13 mm	16
K1042.4316	∅ 4.3 mm, L 16 mm	16
K1042.5009	∅ 5.0 mm, L 9 mm	16
K1042.5011	∅ 5.0 mm, L 11 mm	16
K1042.5013	∅ 5.0 mm, L 13 mm	16
K1042.5016	∅ 5.0 mm, L 16 mm	16
K1042.6009	∅ 6.0 mm, L 9 mm	16
K1042.6011	∅ 6.0 mm, L 11 mm	16
K1042.6013	∅ 6.0 mm, L 13 mm	16
K1042.6016	∅ 6.0 mm, L 16 mm	16
	CAMLOG® SCREW-LINE Implant for practice	
K1049.3813	∅ 3.8 mm	74
K1049.4313-01	∅ 4.3 mm	74
	CAMLOG® SCREW-LINE Implant, Promote® plus	
K1052.3311	∅ 3.3 mm, L 11 mm	17
K1052.3313	∅ 3.3 mm, L 13 mm	17
K1052.3316	∅ 3.3 mm, L 16 mm	17
K1052.3809	∅ 3.8 mm, L 9 mm	17
K1052.3811	∅ 3.8 mm, L 11 mm	17
K1052.3813	∅ 3.8 mm, L 13 mm	17
K1052.3816	∅ 3.8 mm, L 16 mm	17
K1052.4309	∅ 4.3 mm, L 9 mm	17
K1052.4311	∅ 4.3 mm, L 11 mm	17
K1052.4313	∅ 4.3 mm, L 13 mm	17
K1052.4316	∅ 4.3 mm, L 16 mm	17
K1052.5009	∅ 5.0 mm, L 9 mm	17
K1052.5011	∅ 5.0 mm, L 11 mm	17
K1052.5013	∅ 5.0 mm, L 13 mm	17
K1052.5016	∅ 5.0 mm, L 16 mm	17
K1052.6009	∅ 6.0 mm, L 9 mm	17
K1052.6011	∅ 6.0 mm, L 11 mm	17
K1052.6013	∅ 6.0 mm, L 13 mm	17
K1052.6016	∅ 6.0 mm, L 16 mm	17

INDEX

ARTICLE NUMBERS

Article No.	Article	Page	Article No.	Article	Page
Guide System CAMLOG® SCREW-LINE Implant, Promote® plus			CAMLOG® Impression posts, open tray		
K1053.3311	∅ 3.3 mm, L 11 mm	26	K2121.3300	∅ 3.3 mm	50
K1053.3313	∅ 3.3 mm, L 13 mm	26	K2121.3800	∅ 3.8 mm	50
K1053.3316	∅ 3.3 mm, L 16 mm	26	K2121.4300	∅ 4.3 mm	50
K1053.3809	∅ 3.8 mm, L 9 mm	26	K2121.5000	∅ 5.0 mm	50
K1053.3811	∅ 3.8 mm, L 11 mm	26	K2121.6000	∅ 6.0 mm	50
K1053.3813	∅ 3.8 mm, L 13 mm	26	CAMLOG® Universal abutments PS		
K1053.3816	∅ 3.8 mm, L 16 mm	26	K2201.3800	∅ 3.8 mm	55, 69
K1053.4309	∅ 4.3 mm, L 9 mm	26	K2201.4300	∅ 4.3 mm	55, 69
K1053.4311	∅ 4.3 mm, L 11 mm	26	K2201.5000	∅ 5.0 mm	55, 69
K1053.4313	∅ 4.3 mm, L 13 mm	26	K2201.6000	∅ 6.0 mm	55, 69
K1053.4316	∅ 4.3 mm, L 16 mm	26	CAMLOG® Esthomic® Abutments PS, straight		
CAMLOG® Healing cap PS, bottleneck			K2202.3815	∅ 3.8 mm, GH 1.5-2.5 mm	54
K2001.3840	∅ 3.8 mm, GH 4.0 mm	34	K2202.4315	∅ 4.3 mm, GH 1.5-2.5 mm	54
K2001.3860	∅ 3.8 mm, GH 6.0 mm	34	K2202.5015	∅ 5.0 mm, GH 1.5-2.5 mm	54
K2001.4340	∅ 4.3 mm, GH 4.0 mm	34	K2202.6015	∅ 6.0 mm, GH 1.5-2.5 mm	54
K2001.4360	∅ 4.3 mm, GH 6.0 mm	34	CAMLOG® Esthomic® Abutments PS, 15° angled, type A		
K2001.5040	∅ 5.0 mm, GH 4.0 mm	34	K2203.3815	∅ 3.8 mm, GH 1.5-2.5 mm	54
K2001.5060	∅ 5.0 mm, GH 6.0 mm	34	K2203.4315	∅ 4.3 mm, GH 1.5-2.5 mm	54
K2001.6040	∅ 6.0 mm, GH 4.0 mm	34	K2203.5015	∅ 5.0 mm, GH 1.5-2.5 mm	54
K2001.6060	∅ 6.0 mm, GH 6.0 mm	34	K2203.6015	∅ 6.0 mm, GH 1.5-2.5 mm	54
CAMLOG® Healing cap PS, wide body			CAMLOG® Esthomic® Abutments PS, 15° angled, type B		
K2004.3840	∅ 3.8 mm, GH 4.0 mm	34	K2204.3815	∅ 3.8 mm, GH 1.5-2.5 mm	54
K2004.3860	∅ 3.8 mm, GH 6.0 mm	34	K2204.4315	∅ 4.3 mm, GH 1.5-2.5 mm	54
K2004.4340	∅ 4.3 mm, GH 4.0 mm	34	K2204.5015	∅ 5.0 mm, GH 1.5-2.5 mm	54
K2004.4360	∅ 4.3 mm, GH 6.0 mm	34	K2204.6015	∅ 6.0 mm, GH 1.5-2.5 mm	54
K2004.5040	∅ 5.0 mm, GH 4.0 mm	34	CAMLOG® Temporary abutments PS		
K2004.5060	∅ 5.0 mm, GH 6.0 mm	34	K2208.3800	∅ 3.8 mm	52
K2004.6040	∅ 6.0 mm, GH 4.0 mm	34	K2208.4300	∅ 4.3 mm	52
K2004.6060	∅ 6.0 mm, GH 6.0 mm	34	K2208.5000	∅ 5.0 mm	52
CAMLOG® Healing cap PS, cylindrical			K2208.6000	∅ 6.0 mm	52
K2005.3820	∅ 3.8 mm, GH 2.0 mm	34	CAMLOG® Universal abutments		
K2005.3840	∅ 3.8 mm, GH 4.0 mm	34	K2211.3300	∅ 3.3 mm	55
K2005.3860	∅ 3.8 mm, GH 6.0 mm	34	K2211.3800	∅ 3.8 mm	55, 69
K2005.4320	∅ 4.3 mm, GH 2.0 mm	34	K2211.4300	∅ 4.3 mm	55, 69
K2005.4340	∅ 4.3 mm, GH 4.0 mm	34	K2211.5000	∅ 5.0 mm	55, 69
K2005.4360	∅ 4.3 mm, GH 6.0 mm	34	K2211.6000	∅ 6.0 mm	55, 69
K2005.5020	∅ 5.0 mm, GH 2.0 mm	34	CAMLOG® Telescope abutments		
K2005.5040	∅ 5.0 mm, GH 4.0 mm	34	K2212.3800	∅ 3.8 mm	69
K2005.5060	∅ 5.0 mm, GH 6.0 mm	34	K2212.4300	∅ 4.3 mm	69
K2005.6020	∅ 6.0 mm, GH 2.0 mm	34	K2212.5000	∅ 5.0 mm	69
K2005.6040	∅ 6.0 mm, GH 4.0 mm	34	K2212.6000	∅ 6.0 mm	69
K2005.6060	∅ 6.0 mm, GH 6.0 mm	34	CAMLOG® Esthomic® Abutments, straight		
Guide System CAMLOG® Insertion post			K2226.3810	∅ 3.8 mm, GH 1.0-1.8 mm	52
K2026.3300	∅ 3.3 mm	29	K2226.3830	∅ 3.8 mm, GH 3.0-4.5 mm	52
K2026.3800	∅ 3.8 mm	29	K2226.4310	∅ 4.3 mm, GH 1.0-1.8 mm	52
K2026.4300	∅ 4.3 mm	29	K2226.4330	∅ 4.3 mm, GH 3.0-4.5 mm	52
CAMLOG® Impression posts PS, closed tray			K2226.5010	∅ 5.0 mm, GH 1.0-1.8 mm	52
K2109.3800	∅ 3.8 mm	50	K2226.5030	∅ 5.0 mm, GH 3.0-4.5 mm	52
K2109.4300	∅ 4.3 mm	50	K2226.6010	∅ 6.0 mm, GH 1.0-1.8 mm	52
K2109.5000	∅ 5.0 mm	50	K2226.6030	∅ 6.0 mm, GH 3.0-4.5 mm	52
K2109.6000	∅ 6.0 mm	50	CAMLOG® Esthomic® Abutments, 15° angled, type A		
CAMLOG® Impression posts, closed tray			K2227.3810	∅ 3.8 mm, GH 1.0-1.8 mm	52
K2110.3300	∅ 3.3 mm	50	K2227.3830	∅ 3.8 mm, GH 3.0-4.5 mm	52
K2110.3800	∅ 3.8 mm	50	K2227.4310	∅ 4.3 mm, GH 1.0-1.8 mm	52
K2110.4300	∅ 4.3 mm	50	K2227.4330	∅ 4.3 mm, GH 3.0-4.5 mm	52
K2110.5000	∅ 5.0 mm	50	K2227.5010	∅ 5.0 mm, GH 1.0-1.8 mm	52
K2110.6000	∅ 6.0 mm	50	K2227.5030	∅ 5.0 mm, GH 3.0-4.5 mm	52
CAMLOG® Impression posts PS, open tray			K2227.6010	∅ 6.0 mm, GH 1.0-1.8 mm	52
K2119.3800	∅ 3.8 mm	50	K2227.6030	∅ 6.0 mm, GH 3.0-4.5 mm	52
K2119.4300	∅ 4.3 mm	50			
K2119.5000	∅ 5.0 mm	50			
K2119.6000	∅ 6.0 mm	50			

INDEX

ARTICLE NUMBERS

Article No.	Article	Page	Article No.	Article	Page
	CAMLOG® Esthomic® Abutments, 15° angled, type B			CAMLOG® Logfit® Abutments	
K2228.3810	∅ 3.8 mm, GH 1.0-1.8 mm	53	K2550.3808	∅ 3.8 mm, GH 0.8 mm	56
K2228.3830	∅ 3.8 mm, GH 3.0-4.5 mm	53	K2550.3815	∅ 3.8 mm, GH 1.5 mm	56
K2228.4310	∅ 4.3 mm, GH 1.0-1.8 mm	53	K2550.4308	∅ 4.3 mm, GH 0.8 mm	56
K2228.4330	∅ 4.3 mm, GH 3.0-4.5 mm	53	K2550.4315	∅ 4.3 mm, GH 1.5 mm	56
K2228.5010	∅ 5.0 mm, GH 1.0-1.8 mm	53	K2550.5008	∅ 5.0 mm, GH 0.8 mm	56
K2228.5030	∅ 5.0 mm, GH 3.0-4.5 mm	53	K2550.5015	∅ 5.0 mm, GH 1.5 mm	56
K2228.6010	∅ 6.0 mm, GH 1.0-1.8 mm	53	K2550.6008	∅ 6.0 mm, GH 0.8 mm	56
K2228.6030	∅ 6.0 mm, GH 3.0-4.5 mm	53	K2550.6015	∅ 6.0 mm, GH 1.5 mm	56
	CAMLOG® Esthomic® Abutments, 20° angled, type A			CAMLOG® Vario SR abutments, straight, incl. CAMLOG® Vario SR abutment screw	
K2231.3810	∅ 3.8 mm, GH 1.0-1.8 mm	53	K2560.3808	∅ 3.8 mm, GH 0.8 mm	59
K2231.3830	∅ 3.8 mm, GH 3.0-4.5 mm	53	K2560.4308	∅ 4.3 mm, GH 0.8 mm	59
K2231.4310	∅ 4.3 mm, GH 1.0-1.8 mm	53	K2560.5008	∅ 5.0 mm, GH 0.8 mm	59
K2231.4330	∅ 4.3 mm, GH 3.0-4.5 mm	53	K2560.6008	∅ 6.0 mm, GH 0.8 mm	59
K2231.5010	∅ 5.0 mm, GH 1.0-1.8 mm	53		CAMLOG® Vario SR abutments, 20° angled, incl. CAMLOG® Abutment screw	
K2231.5030	∅ 5.0 mm, GH 3.0-4.5 mm	53	K2561.3800	∅ 3.8 mm	59
K2231.6010	∅ 6.0 mm, GH 1.0-1.8 mm	53	K2561.4300	∅ 4.3 mm	59
K2231.6030	∅ 6.0 mm, GH 3.0-4.5 mm	53	K2561.5000	∅ 5.0 mm	59
	CAMLOG® Esthomic® Abutments, 20° angled, type B		K2561.6000	∅ 6.0 mm	59
K2232.3810	∅ 3.8 mm, GH 1.0-1.8 mm	53		CAMLOG® Vario SR abutments, 30° angled, incl. CAMLOG® Abutment screw	
K2232.3830	∅ 3.8 mm, GH 3.0-4.5 mm	53	K2562.3800	∅ 3.8 mm	59
K2232.4310	∅ 4.3 mm, GH 1.0-1.8 mm	53	K2562.4300	∅ 4.3 mm	59
K2232.4330	∅ 4.3 mm, GH 3.0-4.5 mm	53	K2562.5000	∅ 5.0 mm	59
K2232.5010	∅ 5.0 mm, GH 1.0-1.8 mm	53	K2562.6000	∅ 6.0 mm	59
K2232.5030	∅ 5.0 mm, GH 3.0-4.5 mm	53		CAMLOG® Scanbodies, incl. CAMLOG® Abutment screw	
K2232.6010	∅ 6.0 mm, GH 1.0-1.8 mm	53	K2610.3310	∅ 3.3 mm	58
K2232.6030	∅ 6.0 mm, GH 3.0-4.5 mm	53	K2610.3810	∅ 3.8 mm	58
	CAMLOG® Esthomic® Abutments, Inset		K2610.4310	∅ 4.3 mm	58
K2235.3315	∅ 3.3 mm, GH 1.5-2.8 mm	53	K2610.6010	∅ 5.0/6.0 mm	58
K2235.3815	∅ 3.8 mm, GH 1.5-2.8 mm	53		CAMLOG® ScanPosts incl. CAMLOG® Abutment screw	
K2235.4315	∅ 4.3 mm, GH 1.5-2.8 mm	53	K2620.3306	∅ 3.3 mm	58
K2235.5015	∅ 5.0 mm, GH 1.5-2.8 mm	53	K2620.3806	∅ 3.8 mm	58
K2235.6015	∅ 6.0 mm, GH 1.5-2.8 mm	53	K2620.4306	∅ 4.3 mm	58
	CAMLOG® Temporary abutments		K2620.5006	∅ 5.0 mm	58
K2241.3800	∅ 3.8 mm	52	K2620.6006	∅ 6.0 mm	58
K2241.4300	∅ 4.3 mm	52		CAMLOG® Lab analogs	
K2241.5000	∅ 5.0 mm	52	K3010.3300	∅ 3.3 mm	51
K2241.6000	∅ 6.0 mm	52	K3010.3800	∅ 3.8 mm	51
	CAMLOG® Ceramic abutments, 2-parts		K3010.4300	∅ 4.3 mm	51
K2242.3340	∅ 3.3 mm	55	K3010.5000	∅ 5.0 mm	51
K2242.3840	∅ 3.8 mm	55	K3010.6000	∅ 6.0 mm	51
K2242.4340	∅ 4.3 mm	55		K5300.9010 X-Ray Planning foil 1.25:1 CAMLOG® SCREW-LINE Implants.....	12
K2242.5040	∅ 5.0 mm	55		K5300.9011 X-Ray Planning foil 1.4:1 CAMLOG® SCREW-LINE Implants.....	12
K2242.6040	∅ 6.0 mm	55		K5300.9012 X-Ray Planning foil 1.25:1 CAMLOG® ROOT-LINE 2 Implants	12
	CAMLOG® Titanium bases, for CAMLOG® Ceramic abutment			K5300.9013 X-Ray Planning foil 1.4:1 CAMLOG® ROOT-LINE 2 Implants	12
K2242.3342	∅ 3.3 mm	56		X-Ray Transfer pictures 1.25:1 CAMLOG® SCREW-LINE Implants	
K2242.3842	∅ 3.8 mm	56	K5300.9080	∅ 3.3 mm	12
K2242.4342	∅ 4.3 mm	56	K5300.9081	∅ 3.8 mm	12
K2242.5042	∅ 5.0 mm	56	K5300.9082	∅ 4.3 mm	12
K2242.6042	∅ 6.0 mm	56	K5300.9083	∅ 5.0 mm	12
	CAMLOG® Titanium bases CAD/CAM		K5300.9084	∅ 6.0 mm	12
K2244.3348	∅ 3.3 mm	57			
K2244.3848	∅ 3.8 mm	57			
K2244.4348	∅ 4.3 mm	57			
K2244.5048	∅ 5.0 mm	57			
K2244.6048	∅ 6.0 mm	57			
	CAMLOG® Gold-plastic abutments				
K2246.3300	∅ 3.3 mm	55			
K2246.3800	∅ 3.8 mm	55			
K2246.4300	∅ 4.3 mm	55			
K2246.5000	∅ 5.0 mm	55			
K2246.6000	∅ 6.0 mm	55			

Article No.	Article	Page
	X-Ray Transfer pictures 1.25:1	
	CAMLOG® ROOT-LINE 2 Implants	
K5300.9070	∅ 3.3 mm	12
K5300.9071	∅ 3.8 mm	12
K5300.9072	∅ 4.3 mm	12
K5300.9073	∅ 5.0 mm	12
K5300.9074	∅ 6.0 mm	12
	Adapter for screw implants, long, for CAMLOG®	
	SCREW-LINE and ROOT-LINE 2 Implants	
K5302.3310	∅ 3.3 mm	37
K5302.3810	∅ 3.8 mm	37
K5302.4310	∅ 4.3 mm	37
	CAMLOG® SCREW-LINE Macro model	
K8010.1010	Maßstab 3:1	75
	CAMLOG® ROOT-LINE 2 Macro model	
K8010.1011	Maßstab 3:1	75
K8011.1000	CAMLOG® Selection abutment kit	72
	CAMLOG® Demonstration model, acrylic glass	
K8050.1040	lower jaw, 4 CAMLOG® SCREW-LINE Implants	
	∅ 4.3 mm	74
	CAMLOG® Demonstration model, acrylic glass	
K8070.1020	upper jaw, 4 CAMLOG® SCREW-LINE Implants	
	∅ 4.3 mm	74
	ALTApin magazine	
M1000.0050	7 titanium pins, 1 unit	35
M1000.0100	7 titanium pins, 3 units.....	35
M5100.0010	ALTApin applicator , straight.....	35
M5100.0030	ALTApin applicator , angled 90°	35
M5100.0050	ALTApin pricker	35
M5100.0070	ALTApin membrane fixator	35
M5100.0100	ALTApin surgery mallet	35
M5200.0010	ALTApin applicator , straight, work element.....	35
M5200.0055	ALTApin pricker , insert.....	35
M5500.0050	ALTApin single patient drill , ISO shaft	35
M5600.0110	ALTApin set, Membrane fixation system	35
M5600.0210	ALTApin-Tray	35

Adress/Stamp

Date/Signature

Your Customer no.

Order Form

Delivery

normal express

Quantity	Article number	Description	Price

We thank you for your order.

CE0123

Art. No. J8001.0003 Rev. 3 09/2014



HEADQUARTERS

CAMLOG Biotechnologies AG | Margarethenstrasse 38 | CH - 4053 Basel
Telefon +41 61 565 41 00 | Fax +41 61 565 41 01 | info@camlog.com | www.camlog.com

Manufacturer of CAMLOG®/CONELOG® Products: ALTATEC GmbH, Maybachstraße 5, D-71299 Wimsheim

camlog