


CAMLOG®
SYSTEM



PRODUCT CATALOG CAMLOG® IMPLANT SYSTEM

Valid from March 2017

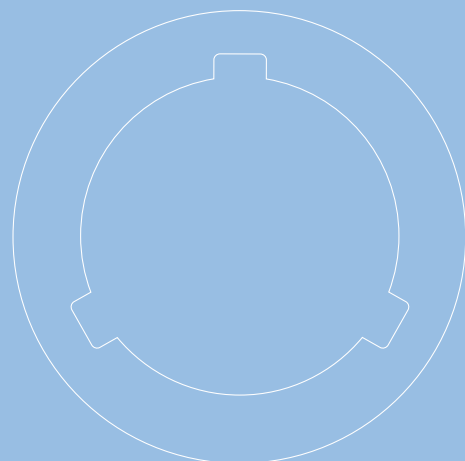

a perfect fit™

camlog

SYSTEM INFORMATION

The CAMLOG® Implant System	2
----------------------------	---

SURGERY

Planning	14
SCREW-LINE implants and instruments	17
SCREW-LINE guide system Implants and instruments	22
ROOT-LINE 2 implants and instruments	27
General surgery instruments	32
Osteotomy set	39
ALTApin set	43
Healing caps	46

PROSTHETICS

Impression taking	50
Bite registration	51
Fabrication of the plaster model	51
Temporary abutments	52
Esthomic® Abutments	52
Universal abutments	54
Gold-plastic abutment	54
Ceramic abutment	54
Logfit® Prosthetic system	55
CAD/CAM prosthetics	56
COMFOUR™ System	60
Ball abutment anchoring system	64
Locator® Anchoring system	65
Double crown restorations	68
Prosthetic instruments	70
Instruments for dental technicians	74
Selection abutments	75

AUXILIARY ARTICLE

Implants for practice	78
Demonstration models	78
Macro models	79
Literature	80

AUXILIARY INFORMATION

Indication overview	82
Implant overview	85
Prosthetics overview	86
Screw overview	92
Overview torque wrench settings	96
Materials	98

INDEX

Alphabetical	100
Article numbers	105

THE CAMLOG® IMPLANT SYSTEM



The CAMLOG® Implant System is based on years of clinical and laboratory experience and is a user-friendly, consistent prosthetically oriented implant system.

All CAMLOG® Products are manufactured with the latest state-of-the-art technology. The CAMLOG® Implant System is continuously being developed by the company's research and development team in collaboration with clinics, universities and dental technicians and therefore stays abreast of the latest technology.

The CAMLOG® and CONELOG® Implant Systems are well documented scientifically. Studies* support this with respect to a great many parameters including the implant surface, time of implantation and/or implant loading, primary stability, and the connection design. The long-term results of the Promote® Surface are convincing.

The descriptions that follow are not adequate to permit immediate use of the CAMLOG® Implant System.

Instruction by a surgeon experienced in using the system is strongly recommended. CAMLOG® Products should only be used by dentists, doctors, surgeons and dental technicians who have been trained in using the system. Appropriate courses and training sessions are regularly offered by CAMLOG.

Methodological errors in treatment can result in loss of the implant and significant loss of peri-implant bone.

Not all products are available in all countries.

Packaging units: unless described otherwise, each pack contains one product.

* see «Further documentation» on page 115

CAMLOG® SCREW-LINE IMPLANTS

SCREW-LINE implants represent conical screw implants and are available both with Promote® Surface (1.4 mm machined implant neck portion) and Promote® Plus surface (0.4 mm machined implant neck portion).

Both implant versions are fitted with three square grooves in the Tube-in-Tube® inner configuration and can be used for the Platform Switching option.

The implants are not only suitable for late, but also for immediate or delayed immediate implantation. The implant is easily inserted because the taper of the external implant body of 3° to 9° (depending on lengths and diameters) induces self-centering. The self-tapping thread provides continuous contact with the bone and high primary stability. Rounding of the apical geometry ensures gentle insertion of the SCREW-LINE implants into the bone.

CAMLOG® SCREW-LINE implants are supplied in sterile packaging, pre-mounted on an insertion post which is color-coded according to the diameter.



IMPLANT DIAMETERS



IMPLANT LENGTHS



CAMLOG® ROOT-LINE 2 IMPLANTS

CAMLOG® ROOT-LINE 2 implants are root-shaped screw implants. The geometry of the implant body allows its use at limited apical bone and is easy to insert due to self-centering.

The implants are available with the Promote® plus surface (0.4 mm machined implant neck portion). They are fitted with the proven Tube-in-Tube® Implant-abutment connection and the three angular grooves and can be used for the Platform Switching option.

CAMLOG® ROOT-LINE 2 implants are supplied in sterile packaging, pre-mounted on an insertion post which is color-coded according to the diameter.

IMPLANT DIAMETERS



IMPLANT LENGTHS



The option of Platform Switching may only be used with CAMLOG® Implants with K article numbers.

PROMOTE® SURFACE

CAMLOG® Implants are available with the Promote® surface. For the CAMLOG® SCREW-LINE implants Promote®, the abrasive-blasted, acid-etched surface extends up to 1.4 mm below the implant shoulder and the Promote® plus surface up to 0.4 mm under the shoulder. For CAMLOG® ROOT-LINE 2 implants this reaches up to 0.4 mm below the implant shoulder (Promote® plus). The surface is based on current scientific knowledge and supports rapid osseointegration. Scientific results from studies with cell cultures, osteohistology and in pull-out trials illustrate this impressively.



CAMLOG® TUBE-IN-TUBE® IMPLANT-ABUTMENT CONNECTION

The very heart of the CAMLOG® Implant System is the Tube-in-Tube® Implant-abutment connection. The special geometric principle with the three short cams of the abutments, together with the precision of the connection, ensure optimal distribution of force and torque between the individual components. The CAMLOG® Implant-abutment connection is predominantly form-fitting and was biomechanically optimized by applying elaborate finite element analyses. This has proven itself over many years and in several million implant insertions. The groove/cam geometry makes the system distinctive.

The CAMLOG® Tube-in-Tube® Connection is a 5.4 mm deep implant-abutment connection with antirotational locking mechanism. The three symmetrically arranged grooves are located in the 1.9 mm deep cylindrical drill hole in the coronal region. This region leads apically to an upper thread. This is followed by a thinner and longish cylindrical threaded bore. The abutment screw of the two-piece abutment engages in this lower inner thread. The CAMLOG® Tube-in-Tube® Connection has undergone extensive scientific studies and achieved above average good results for tightness and precision fit.

ADVANTAGES AND BENEFITS OF THE TUBE-IN-TUBE® CONNECTION


- Three possible positions of the abutment
- Fast and uncomplicated insertion and alignment without the need for aids
- Efficiency through time-saving handling
- Virtually perfect transfer through excellent fit
- Only slight torque necessary for the abutment screw
- High long-term stability

For optimal positioning of the abutments, the implant should be aligned in the bone so that one of the three grooves points in vestibular direction. With the CAMLOG® SCREW-LINE and ROOT-LINE 2 implants, the insertion tools include markings that correspond to the three grooves of the implant's inner configuration.

CAMLOG® BALL, LOCATOR® AND STRAIGHT BAR ABUTMENTS

Ball, Locator® and straight bar abutments are available for the CAMLOG® Implant System. These differ from the abutments with abutment screws in the apical region through different connection designs. Ball, Locator® and straight bar abutments are manufactured as single pieces with a thread in the apical region which engages with the upper inner thread of the CAMLOG® Implant. These abutments are screwed into the CAMLOG® Implant using the corresponding insertion tools.



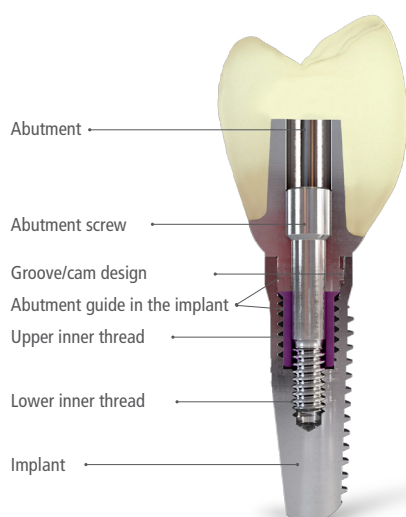

PRODUCTION PRECISION

The inner and outer geometry of the CAMLOG® Implants and abutments are rotary machined for the most part. The tolerances can therefore be kept very low. The result is excellent part precision without impacting the material structure. The Tube-in-Tube® Implant-abutment connection thus ensures a very precise, stable and rotation-locked connection to the prosthetic components.

EFFECT OF THE PLATFORM SWITCHING DESIGN

Platform Switching option is used to support the hard and soft tissue in the peri-implant esthetic region. The distance between the implant-abutment interface and the alveolar crest is to be increased to reduce the effect of inflammatory cell infiltrates on bone resorption. The option of Platform Switching may only be used with CAMLOG® Implants with K article numbers.

CAMLOG® HEALING CAPS PS FOR PLATFORM SWITCHING

The CAMLOG® Healing caps PS (cylindrical, wide body, bottleneck) are tapered in diameter at the shoulder support making it possible to adapt soft tissue over the implant shoulder.



CAMLOG® IMPRESSION POSTS PS, OPEN AND CLOSED TRAY FOR PLATFORM SWITCHING


Due to the adaptation of the soft tissue over the implant shoulder, the use of the CAMLOG® Healing caps PS necessitates the use of the CAMLOG® Impression post PS for Platform Switching.

CAMLOG® TEMPORARY ABUTMENTS PS, CAMLOG® ESTHOMIC® ABUTMENTS PS AND CAMLOG® UNIVERSAL ABUTMENTS PS FOR PLATFORM SWITCHING

The CAMLOG® Abutments PS are also tapered in diameter in the area of the shoulder support and thus allow adapting soft tissue over the implant shoulder during prosthetic restoration.



Short cam geometry



CAMLOG® ABUTMENTS WITH K ARTICLE NUMBERS

The abutments are extended apically in tubular shape (5.4 mm) and include three short cams in the upper section that correspond to the three grooves in the implant.

When inserting the abutments, their tubular extension towards the apex affects the simple, easy and safe orientation in the longitudinal axis of the implant before the three cams lock into the grooves of the implant shoulder. The abutment is rotated until tactile engagement of the cams in the grooves of the implant. The abutment is then in the final position.

The implant-abutment connection of the CAMLOG® Implant System is predominantly a form-fitting connection. The connection with the cam geometry was optimally designed in terms of biomechanics by applying elaborate finite element analyses. The image displays the distribution of the von Mises tension in the implant-abutment connection in accordance with ISO 14801 at a load of 200 N.

CAMLOG® HEALING CAPS

The various healing caps are used according to indication for single and two-stage procedures. The CAMLOG® Healing caps are available in three geometries (cylindrical, wide body and bottleneck), both for the standard connections as well as for the Platform Switching option (PS). They are not rotation-locked and are screw-retained in the upper inner thread of the implants.



CAMLOG® IMPRESSION TAKING

Impression-taking of the CAMLOG® Implants is possible with impression posts, open or closed tray. Impression posts for Platform Switching (PS) are also an option. All impression-taking components are color-coded based on the implant diameter. High-precision components ensure correct transfer of the intraoral situation. The antirotational mechanism is ensured by the CAMLOG® groove/cam geometry.



CAMLOG® PROSTHETIC COMPONENTS

The CAMLOG® Implants can be provided with a wide range of flexible, anatomically adapted prosthetic components. CAMLOG® Abutments are color-coded according to the implant diameters.



CAMLOG® TEMPORARY ABUTMENTS

Various abutments are available for the CAMLOG® Implant System for temporary prosthetic restorations. CAMLOG® Temporary abutments made of titanium alloy (Ti6Al4V ELI) are available in crown and bridge versions.


As an option, temporary restoration on CAMLOG® Implants can also be performed with temporary abutments made of PEEK (poly ether ether ketone). Also as option for Platform Switching (PS). The abutments can be used in immediate implantations or after exposing the gingiva.

CAMLOG® ESTHOMIC® ABUTMENTS

Anatomically preformed abutments allow for optimal stump design. The CAMLOG® Esthomic® Abutments are available both straight and angled with various gingival heights and with an oval anatomically pre-shaped shoulder profile. The angled Esthomic® Abutments are available in A and B versions differentiated by a cam offset of 60°. This results in six prosthetic-oriented rotating positions and allows perfect prosthetic alignment of the axes.



CAMLOG® Esthomic® Abutment cam alignment

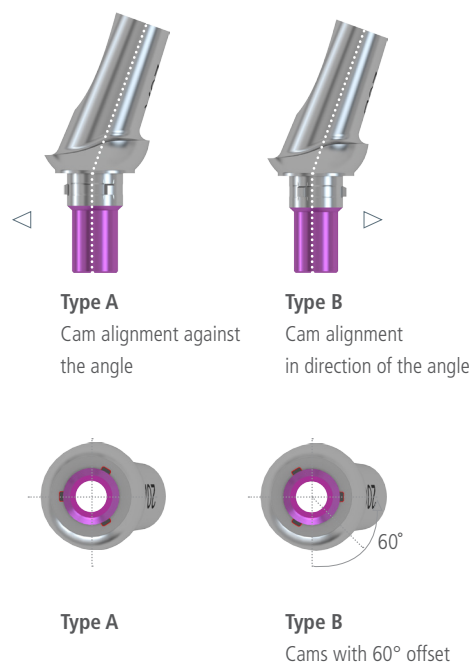

CAMLOG® GOLD-PLASTIC ABUTMENT

The CAMLOG® Gold-plastic abutment can be used with the cast-on technique to fabricate a multitude of customized implant restorations, such as single crowns, mesostructures for cementable bridge restorations and primary abutments for bridging implant axis divergences in the double crown technique.



CAMLOG® TITANIUM BASES CAD/CAM

CAMLOG® Titanium bases CAD/CAM act as a bonding basis for customized, implant-supported dental restorations made of suitable materials. Reconstructions are fabricated with the aid of CAD/CAM techniques. CAMLOG® Titanium bases CAD/CAM are available in crown and bridge versions.

CAMLOG® LOGFIT® ABUTMENTS

The CAMLOG® Logfit® Prosthetic System enables the fabrication of cementable crown and bridge restorations. The Logfit® Prosthetic System consists of prefabricated components precisely matched to one another and thus standardizes the clinical and technical procedure. The result is a lower workload for the practice and the dental laboratory.



CAMLOG® UNIVERSAL AND TELESCOPE ABUTMENTS


CAMLOG® Universal and telescope abutments can be used for individually fabricated cementable crown and bridge restorations and for double crown restorations. The universal abutment is also available for optional Platform Switching (PS). The abutments are made of titanium alloy and can be custom trimmed.



COMFOUR™ SYSTEM

Occlusally screw-retained restorations are state-of-the-art. With the COMFOUR™ System, edentulous patients are given the option of immediate, comfortable and permanent dentures based on four or six implants as a rule – and thus a considerable gain in quality of life. But clinicians too can look forward to considerably greater comfort and freedom. COMFOUR™ offers several treatment concepts. In addition to occlusally screw-retained crowns and bridges for immediate and delayed restorations, the multi-optional system also permits bar restorations on straight and angled bar abutments. COMFOUR™ offers a wide

range of options to master the challenges in practice routine easier and with less time in future. Next to its versatility, the COMFOUR™ prosthetic system excels through its slim design in particular. All components are of delicate and low design, which simplifies prosthetic restorations considerably for dentists and dental technicians. In addition, a number of technical highlights ensure that COMFOUR™ is not simply just a name, but also a program – for users and patients alike.

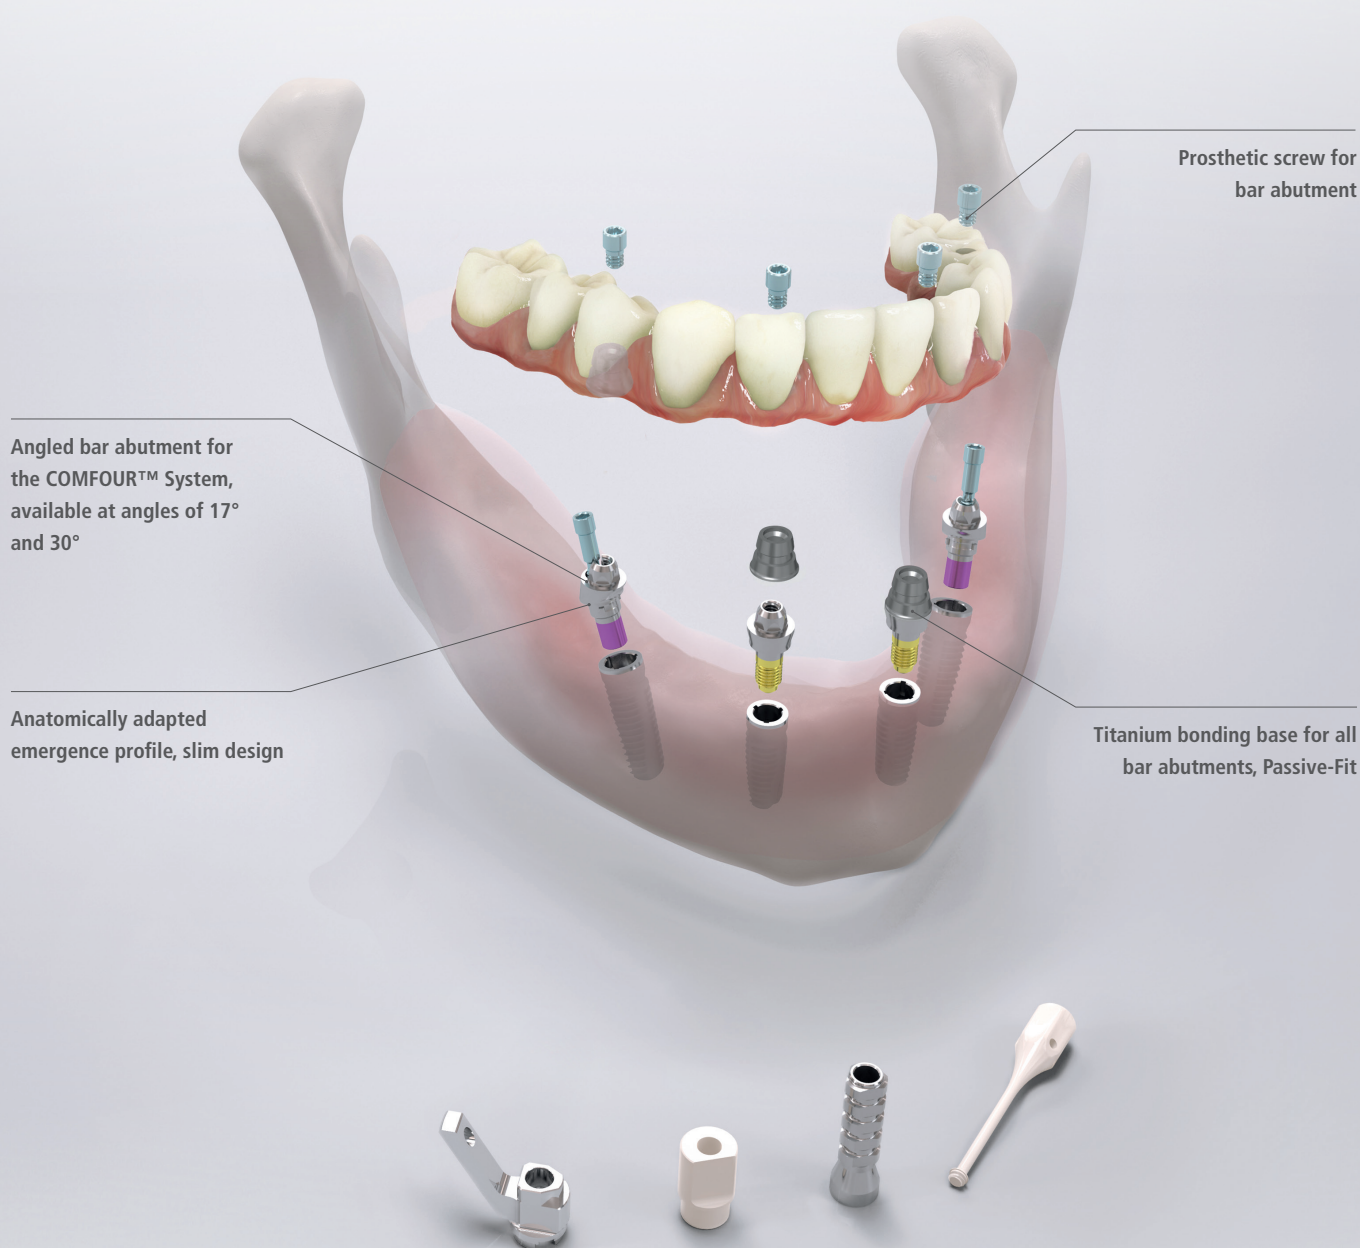

COMFOUR™ offers a large selection of options to manage the requirements of your practice. Easier and more time-saving.

COLOR CODING OF THE SURGICAL AND PROSTHETIC CAMLOG® PRODUCTS



EXPLANATION OF SYMBOLS

	Sterilized using irradiation
	Non-sterile
	Caution, observe the warning notices
	Use-by date
	Do not re-use
	Article number
	Lot number
	Manufacture
	Date of manufacture
	Temperature limit
	Consult instructions for use
	Do not use if package is damaged
	Do not re-sterilize

EXPLANATION OF ABBREVIATIONS

	Diameter
	Apical diameter
	Gingival diameter
	Prosthetic platform diameter
	Length
	Gingival height
	Poly ether ether ketone
	Polyoxymethylene
	Platform Switching

GENERAL SAFETY INSTRUCTIONS AND WARNINGS

The descriptions in this product catalog are not sufficient to allow immediate use of the CAMLOG® Implant System. Instruction by a surgeon experienced in using the CAMLOG® Implant System is strongly recommended.

SECONDARY PACKAGING

Sealed, folding box with color-coded product label

INNER IMPLANT PACKAGING (PRIMARY PACKAGING)

Sealed, color-coded

EXAMPLE OF PRODUCT LABEL FOR OUTER IMPLANT PACKAGING










PLANNING – X-RAY PLANNING FOILS AND X-RAY TRANSFER PICTURE

	Article	Art.-No.	Ø
<p>X-RAY PLANNING FOIL 1.25:1 CAMLOG® SCREW-LINE IMPLANT, K-SCREWS</p> <p>ACTUAL SIZE</p> <p>25% MAGNIFICATION</p>	X-Ray Planning foil 1.25:1 CAMLOG® SCREW-LINE Implants Magnification 25%	K5300.9010	-
	X-Ray Planning foil 1.25:1 CAMLOG® ROOT-LINE 2 Implants Magnification 25%	K5300.9012	-
<p>X-RAY PLANNING FOIL 1.4:1 CAMLOG® SCREW-LINE IMPLANT, K-SCREWS</p> <p>ACTUAL SIZE</p> <p>40% MAGNIFICATION</p>	X-Ray Planning foil 1.4:1 CAMLOG® SCREW-LINE Implants Magnification 40%	K5300.9011	-
	X-Ray Planning foil 1.4:1 CAMLOG® ROOT-LINE 2 Implants Magnification 40%	K5300.9013	-
<p>X-RAY TRANSFER PICTURES CAMLOG® SCREW-LINE IMPLANTS Ø 3.3 mm K-SCREWS</p>	X-Ray Transfer pictures 1.25:1 CAMLOG® SCREW-LINE Implants Planning foils, self-adhesive Magnification 25%	K5300.9080	3.3 mm
		K5300.9081	3.8 mm
		K5300.9082	4.3 mm
		K5300.9083	5.0 mm
		K5300.9084	6.0 mm
<p>X-RAY TRANSFER PICTURES CAMLOG® ROOT-LINE 2 IMPLANTS Ø 3.3 mm K-SCREWS</p>	X-Ray Transfer pictures 1.25:1 CAMLOG® ROOT-LINE 2 Implants Planning foils, self-adhesive Magnification 25%	K5300.9070	3.3 mm
		K5300.9071	3.8 mm
		K5300.9072	4.3 mm
		K5300.9073	5.0 mm
		K5300.9074	6.0 mm

CT-PLANNING – FOR 3-D X-RAY PLANNING AND DRILLING TEMPLATE

	Article	Art.-No.	L
	CT-tube for drill Ø 2.0 mm, corrugated tubing pack of 10 internal diameter 2.1 mm external diameter 2.5 mm Material Titanium alloy	A2002.2000	4.0 mm 10.0 mm
	CT-tube for drill Ø 2.2 mm, corrugated tubing pack of 10 internal diameter 2.3 mm external diameter 2.7 mm Material Titanium alloy	A2222.2200	4.0 mm 10.0 mm
	Drill for CT-tube (for A2002.2000) Ø 2.6 mm Material Stainless steel	A2050.2600	-
	Drill for CT-tube (for A2222.2200) Ø 2.8 mm Material Stainless steel	A2050.2800	-

* for pilot drills J5051.2003 and pilot drills SCREW-LINE J5051.2000

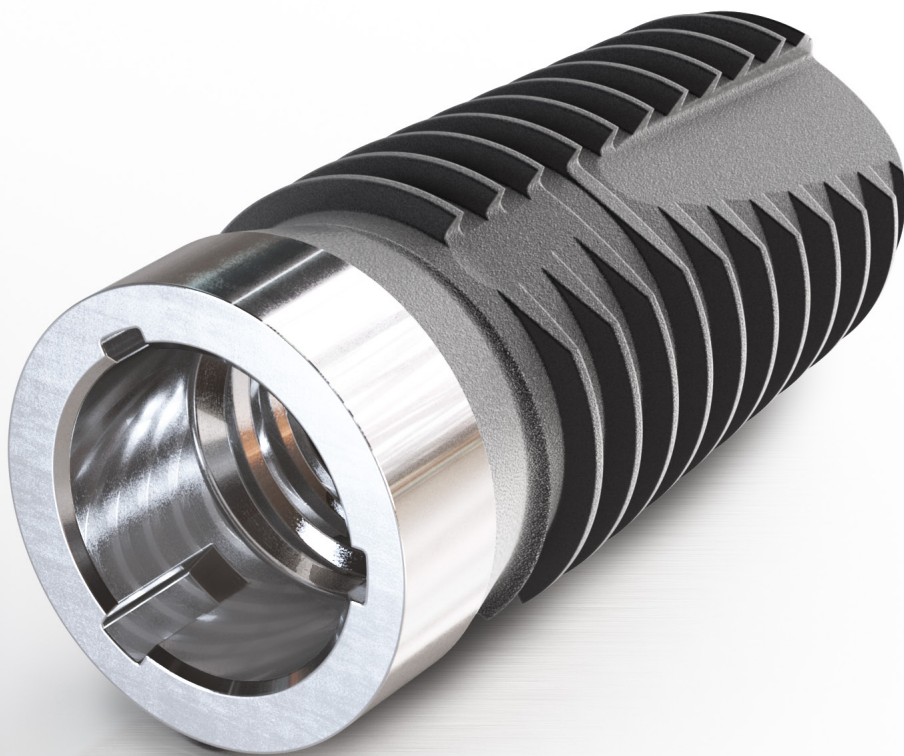

SCREW-LINE – IMPLANTS


	Article	Art.-No.	Ø	L	A Ø
	CAMLOG® SCREW-LINE Implant, Promote® incl. insertion post and cover screw, sterile Material Titanium Grade 4	K1044.3311	3.3 mm	11 mm	2.7 mm
		K1044.3313		13 mm	
		K1044.3316		16 mm	
		K1044.3809	3.8 mm	9 mm	3.5 mm
		K1044.3811		11 mm	
		K1044.3813		13 mm	
		K1044.3816		16 mm	
		K1044.4309	4.3 mm	9 mm	3.9 mm
		K1044.4311		11 mm	
		K1044.4313		13 mm	
		K1044.4316		16 mm	
		K1044.5009	5.0 mm	9 mm	4.6 mm
		K1044.5011		11 mm	
		K1044.5013		13 mm	
		K1044.5016		16 mm	
		K1044.6009	6.0 mm	9 mm	5.5 mm
		K1044.6011		11 mm	
		K1044.6013		13 mm	
		K1044.6016		16 mm	
	CAMLOG® SCREW-LINE Implant, Promote® plus incl. insertion post and cover screw, sterile Material Titanium Grade 4	K1054.3311	3.3 mm	11 mm	2.7 mm
		K1054.3313		13 mm	
		K1054.3316		16 mm	
		K1054.3809	3.8 mm	9 mm	3.5 mm
		K1054.3811		11 mm	
		K1054.3813		13 mm	
		K1054.3816		16 mm	
		K1054.4309	4.3 mm	9 mm	3.9 mm
		K1054.4311		11 mm	
		K1054.4313		13 mm	
		K1054.4316		16 mm	
		K1054.5009	5.0 mm	9 mm	4.6 mm
		K1054.5011		11 mm	
		K1054.5013		13 mm	
		K1054.5016		16 mm	
		K1054.6009	6.0 mm	9 mm	5.5 mm
		K1054.6011		11 mm	
		K1054.6013		13 mm	
		K1054.6016		16 mm	

NOTES


- CAMLOG® SCREW-LINE implants, Promote®, with Art. No. K1044.xxxx are available from June 2017.
- CAMLOG® SCREW-LINE implants, Promote® plus, with Art. No. K1054.xxxx are available from September 2017.
- CAMLOG® SCREW-LINE implants Promote® with Art. No. K1044.xxxx and CAMLOG® SCREW-LINE implants Promote® plus with Art. No. K1054.xxxx can be used exclusively with the new optimized drivers (Art. No. J5300.0031, J5300.0032, J5300.0033, J5300.0034 or J5300.0035).

With CAMLOG® SCREW-LINE Implants with the diameters 3.8/4.3/5.0/6.0 mm, the option of Platform Switching is possible.




SCREW-LINE – SURGERY SET CAMLOG®/CONELOG®

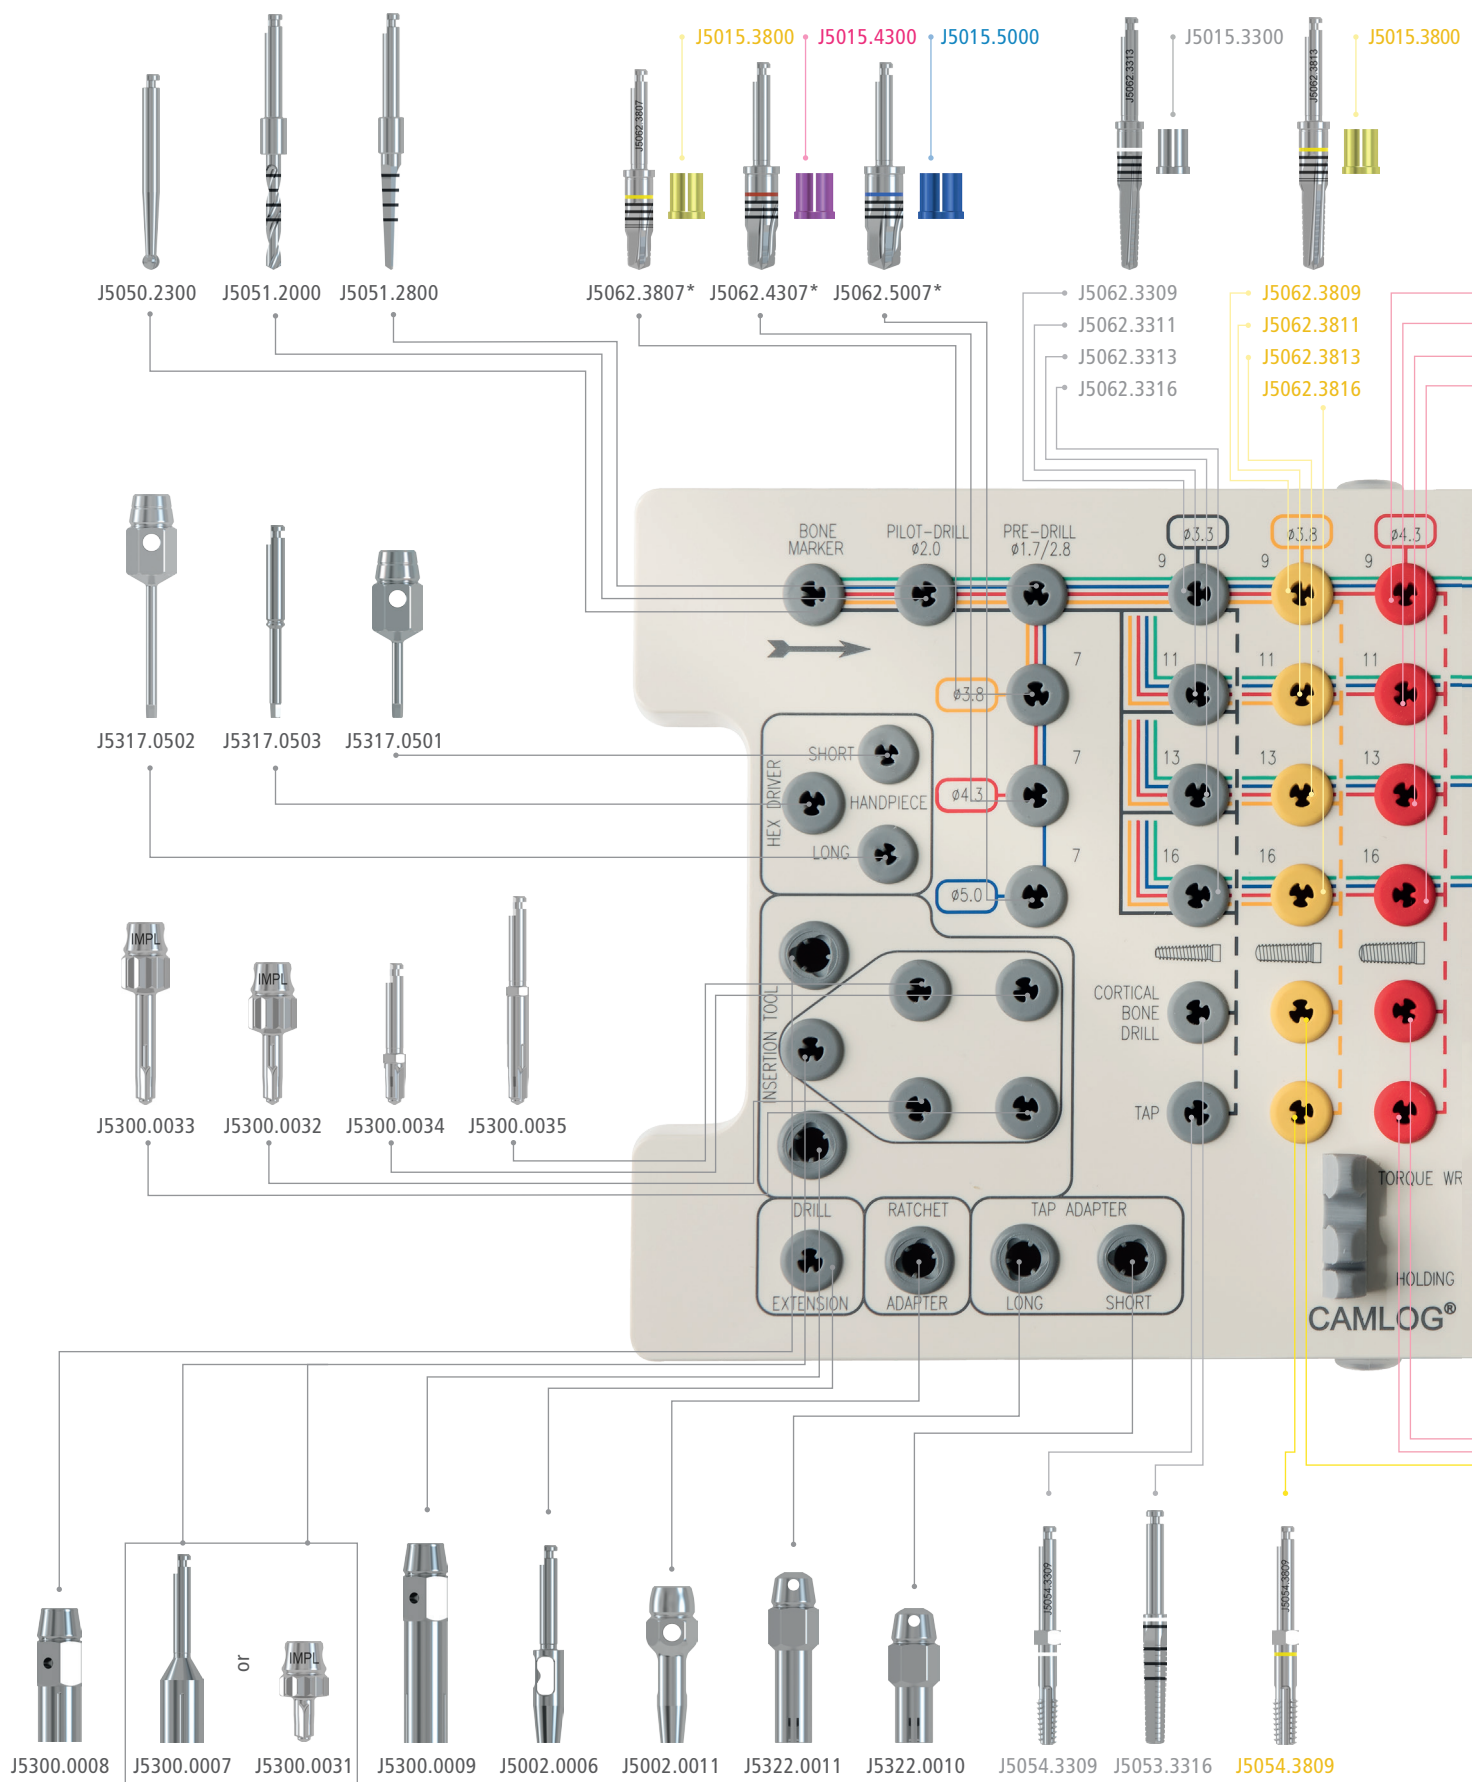

* only for CONELOG® SCREW-LINE implants length 7 mm

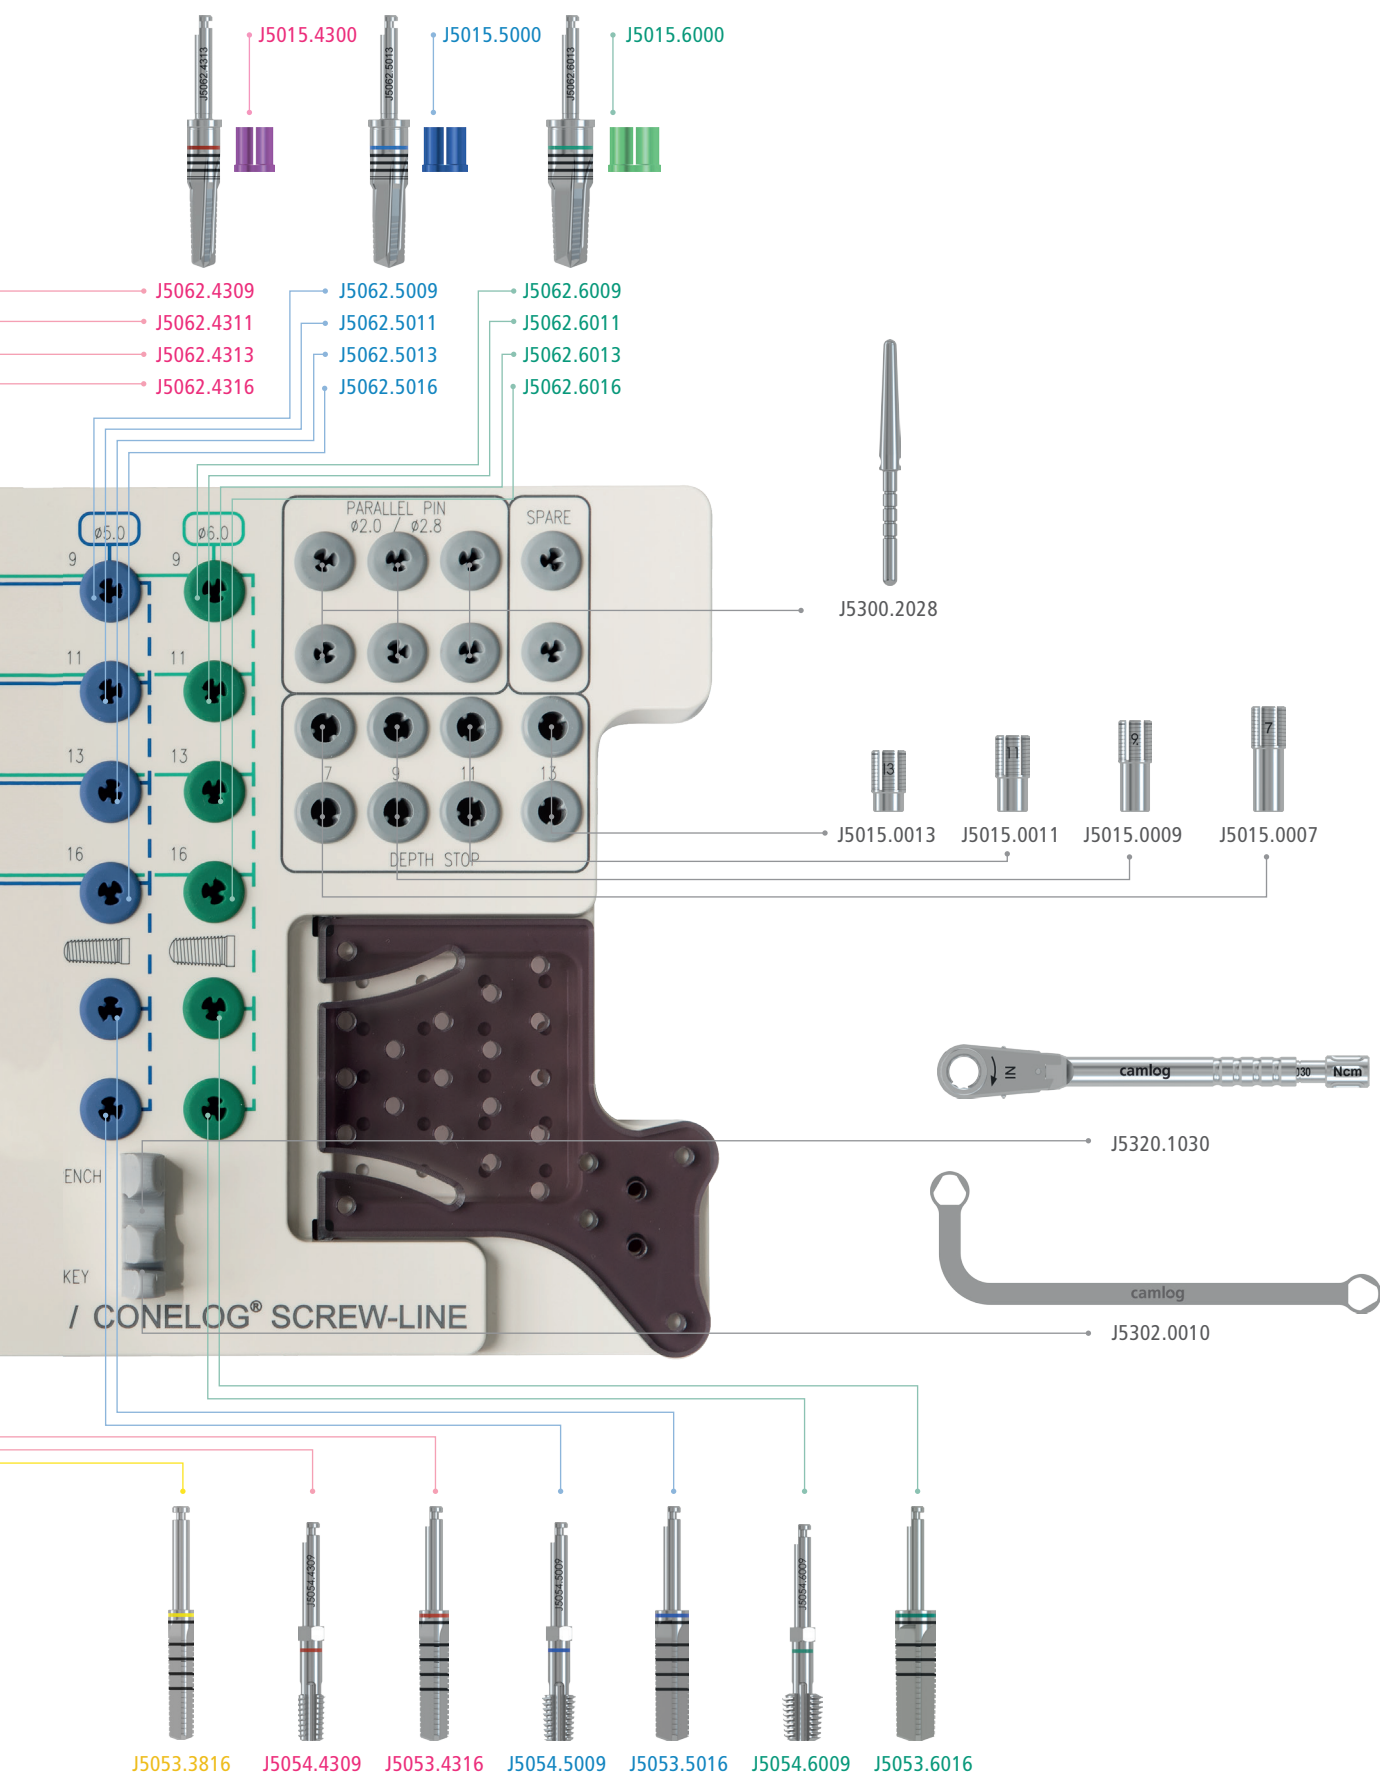



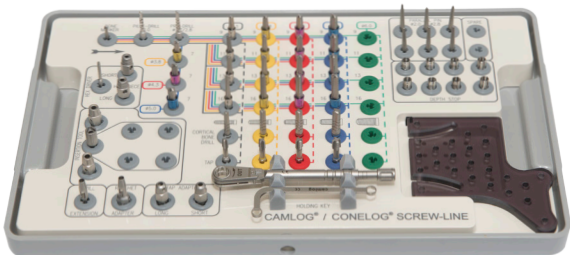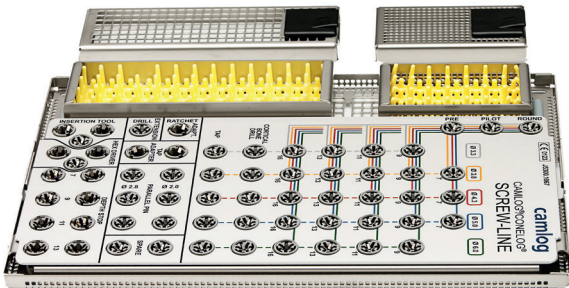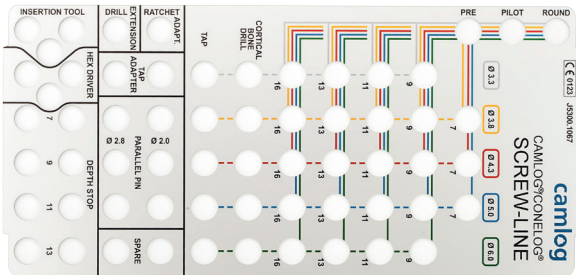

SCREW-LINE – SURGERY SET

	Article	Art.-No.
	<p>Surgery set CAMLOG®/CONELOG® SCREW-LINE Contains all necessary color-code ordered surgical instruments, incl. torque wrench and holding key for insertion post (drills and taps for Ø 6.0 mm are not included)</p>	J5300.0061
	<p>Surgery wash tray CAMLOG®/CONELOG® SCREW-LINE incl. pattern, without content</p>	J5300.8967
	<p>Pattern for surgery wash tray CAMLOG®/CONELOG® SCREW-LINE</p>	J5300.1067

Preparation of the implant bed for CAMLOG® SCREW-LINE implants and for CONELOG® SCREW-LINE implants is performed with identical instruments.

SCREW-LINE – SURGICAL INSTRUMENTS

	Article	Art.-No.	Ø	L
	Form drill SCREW-LINE resterilizable Material Stainless steel	J5062.3309	3.3 mm	9 mm
		J5062.3311		11 mm
		J5062.3313		13 mm
		J5062.3316		16 mm
		J5062.3809	3.8 mm	9 mm
		J5062.3811		11 mm
		J5062.3813		13 mm
		J5062.3816		16 mm
		J5062.4309	4.3 mm	9 mm
		J5062.4311		11 mm
		J5062.4313		13 mm
		J5062.4316		16 mm
		J5062.5009	5.0 mm	9 mm
		J5062.5011		11 mm
		J5062.5013		13 mm
		J5062.5016		16 mm
		J5062.6009	6.0 mm	9 mm
		J5062.6011		11 mm
		J5062.6013		13 mm
		J5062.6016		16 mm
	Depth stop for form drills SCREW-LINE and ROOT-LINE 2 resterilizable Material Titanium alloy	J5015.3300	3.3 mm	-
		J5015.3800	3.8 mm	
		J5015.4300	4.3 mm	
		J5015.5000	5.0 mm	
		J5015.6000	6.0 mm	
	Form drill SCREW-LINE Cortical bone resterilizable Material Stainless steel	J5053.3316	3.3 mm	-
		J5053.3816	3.8 mm	
		J5053.4316	4.3 mm	
		J5053.5016	5.0 mm	
		J5053.6016	6.0 mm	
	Tap SCREW-LINE with hexagon, resterilizable Material Stainless steel	J5054.3309	3.3 mm	-
		J5054.3809	3.8 mm	
		J5054.4309	4.3 mm	
		J5054.5009	5.0 mm	
		J5054.6009	6.0 mm	





SCREW-LINE – GUIDE SYSTEM

	Article	Art.-No.	Ø	L	A Ø		
	<p>Guide System CAMLOG® SCREW-LINE Implant, Promote® plus incl. Guide System Insertion post and cover screw, sterile</p> <p>Material Titanium Grade 4</p>	K1053.3311	3.3 mm	11 mm	2.7 mm		
		K1053.3313		13 mm			
		K1053.3316		16 mm			
		K1053.3809	3.8 mm	9 mm	3.5 mm		
		K1053.3811		11 mm			
		K1053.3813		13 mm			
		K1053.3816	16 mm				
		K1053.4309	4.3 mm	9 mm	3.9 mm		
		K1053.4311		11 mm			
		K1053.4313		13 mm			
		K1053.4316		16 mm			
			<p>Guide System Pilot drill set internal irrigation, sterile (for pilot drilling Ø 2.0 mm)</p> <p>Material Stainless steel</p>	J5043.3311	3.3 mm	11 mm (incl. 5 and 9 mm)**	
				J5043.3313		13 mm (incl. 5, 9 and 11 mm)**	
J5044.3316*	16 mm						
J5043.4309	3.8 mm			9 mm (incl. 5 mm)**			
	4.3 mm						
J5043.4311	3.8 mm			11 mm (incl. 5 and 9 mm)**			
	4.3 mm						
J5043.4313	3.8 mm			13 mm (incl. 5, 9 and 11 mm)**			
	4.3 mm						
J5044.4316*	3.8 mm			16 mm			
	4.3 mm						

* Necessary Guide System pilot drill for implant length 16 mm, following obligatory prior use of the pilot drill set length 13 mm.

** All Guide System pilot drill sets include a 5 mm long pilot drill, as well as all pilot drills necessary for the selected implant length.

All Guide System drills and gingiva punches are intended for single use only.






	Article	Art.-No.	Ø	L
	Guide System Surgery set, SCREW-LINE internal irrigation, sterile Material Stainless steel	J5045.3311	3.3 mm	11 mm (incl. 5 and 9 mm)**
		J5045.3313		13 mm (incl. 5, 9 and 11 mm)**
		J5046.3316*		16 mm
		J5045.3809	3.8 mm	9 mm (incl. 5 mm)**
		J5045.3811		11 mm (incl. 5 and 9 mm)**
		J5045.3813		13 mm (incl. 5, 9 and 11 mm)**
		J5046.3816*		16 mm
		J5045.4309	4.3 mm	9 mm (incl. 5 mm)**
		J5045.4311		11 mm (incl. 5 and 9 mm)**
		J5045.4313		13 mm (incl. 5, 9 and 11 mm)**
		J5046.4316*		16 mm
	Guide System Form drill, SCREW-LINE, Cortical Bone internal irrigation, sterile Material Stainless steel	J5048.3311	3.3 mm	11 mm
		J5048.3313		13 mm
		J5048.3316		16 mm
		J5048.3809	3.8 mm	9 mm
		J5048.3811		11 mm
		J5048.3813		13 mm
		J5048.3816		16 mm
		J5048.4309	4.3 mm	9 mm
		J5048.4311		11 mm
		J5048.4313		13 mm
		J5048.4316		16 mm
	Guide System Gingiva punch sterile Material Stainless steel	J5041.3300	3.3 mm	-
		J5041.3800	3.8 mm	
		J5041.4300	4.3 mm	
	Guide System Guiding sleeve height 3.0 mm (2 units) Material Titanium alloy	J3714.3303	3.3 mm	-
		J3714.3803	3.8 mm	
		J3714.4303	4.3 mm	





* Necessary Guide System form drill for implant length 16 mm, following obligatory prior use of the Guide System surgery set length 13 mm.


** All Guide System surgery sets include a 5 mm long pre-drill, as well as all form drills necessary for the selected implant length.

All Guide System drills and gingiva punches are intended for single use only.


SCREW-LINE – GUIDE SYSTEM

	Article	Art.-No.	Ø	L
	Guide System CAMLOG® Insertion post for CAMLOG® Lab analogs, incl. fixing screw (2 units) Material Titanium alloy	K2026.3300	3.3 mm	-
		K2026.3800	3.8 mm	-
		K2026.4300	4.3 mm	-
	Guide System Template drill for Guide System Guiding sleeve Material Stainless steel	J3713.3300	3.3 mm	-
		J3713.4300	3.8 mm	
			4.3 mm	
	Guide System Seating tool for Guide System Guiding sleeve Material Stainless steel	J3716.3300	3.3 mm	-
		J3716.4300	3.8 mm	
			4.3 mm	

	Article	Art.-No.	Ø	L
	Guide System Check-up pin for Guide System Guiding sleeve Material Stainless steel	J5301.3300	3.3 mm	-
		J5301.4300	3.8 mm	
			4.3 mm	
	Guide System Driver for Guide System Implant Ø 3.3/3.8/4.3 mm, manual/wrench Material Stainless steel	J5303.4300	3.3 mm 3.8 mm 4.3 mm	-
	Guide System Driver for Guide System Implant Ø 3.3/3.8/4.3 mm, with ISO shaft for angled hand piece Material Stainless steel	J5304.4300	3.3 mm 3.8 mm 4.3 mm	-
	Drill extension ISO shaft, for drills with internal irrigation Material Stainless steel	J5002.0005	-	26.6 mm

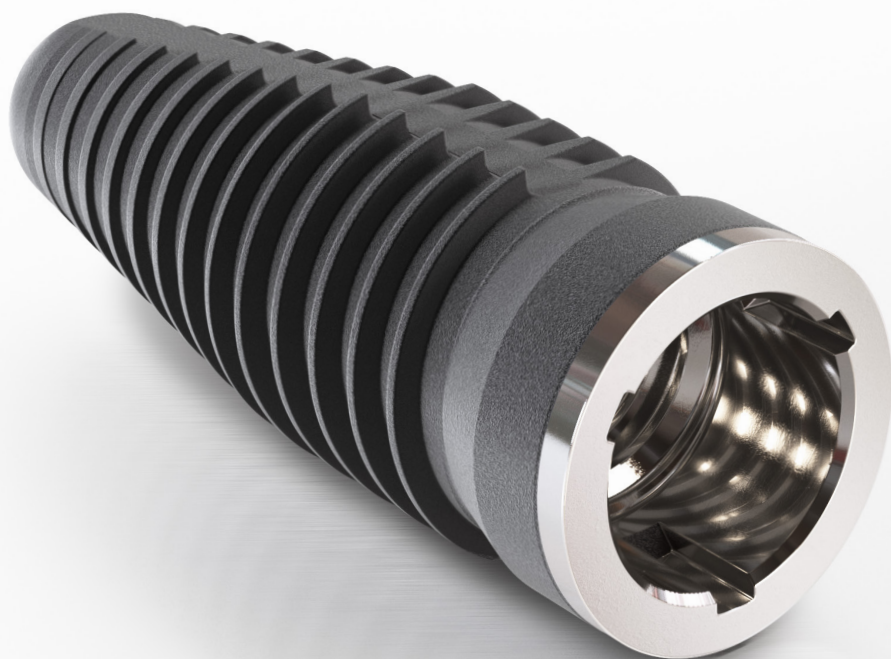


ROOT-LINE 2 – IMPLANTS


	Article	Art.-No.	Ø	L	A Ø
	CAMLOG® ROOT-LINE 2 Implant, Promote® plus incl. insertion post and cover screw, sterile Material Titanium Grade 4	K1032.3311	3.3 mm	11 mm	2.2 mm
		K1032.3313		13 mm	
		K1032.3316		16 mm	
		K1032.3809	3.8 mm	9 mm	2.3 mm
		K1032.3811		11 mm	
		K1032.3813		13 mm	
		K1032.3816		16 mm	
		K1032.4309	4.3 mm	9 mm	2.55 mm
		K1032.4311		11 mm	
		K1032.4313		13 mm	
		K1032.4316		16 mm	
		K1032.5009	5.0 mm	9 mm	2.9 mm
		K1032.5011		11 mm	
		K1032.5013		13 mm	
		K1032.5016		16 mm	
		K1032.6009	6.0 mm	9 mm	3.8 mm
		K1032.6011		11 mm	
		K1032.6013		13 mm	
		K1032.6016		16 mm	

SURGERY




With CAMLOG® ROOT-LINE 2 Implants with the Ø 3.8/4.3/5.0/6.0 mm, the option of Platform Switching is possible.

ROOT-LINE 2 – SURGERY SET CAMLOG®

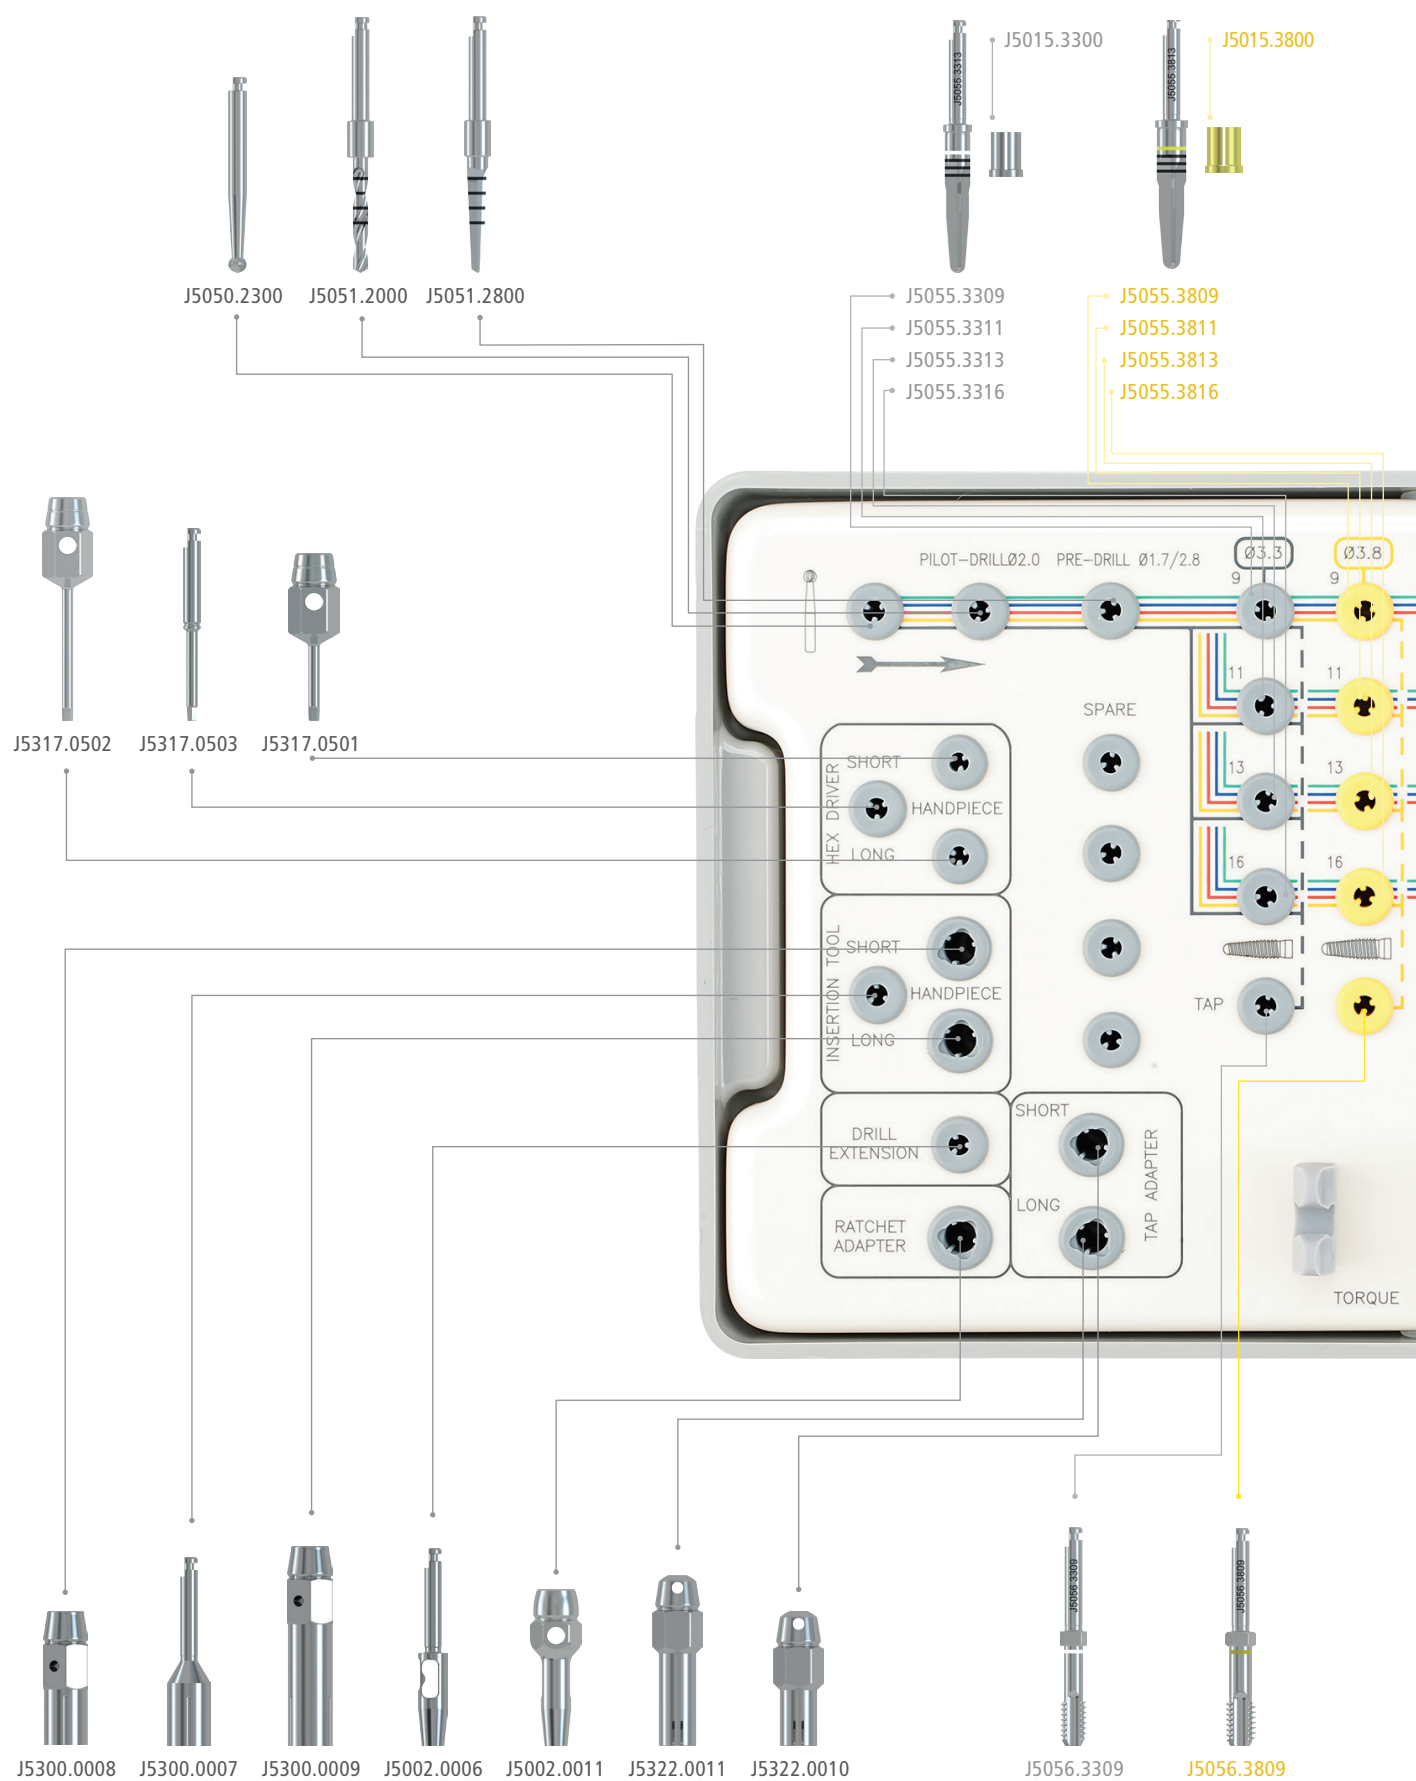

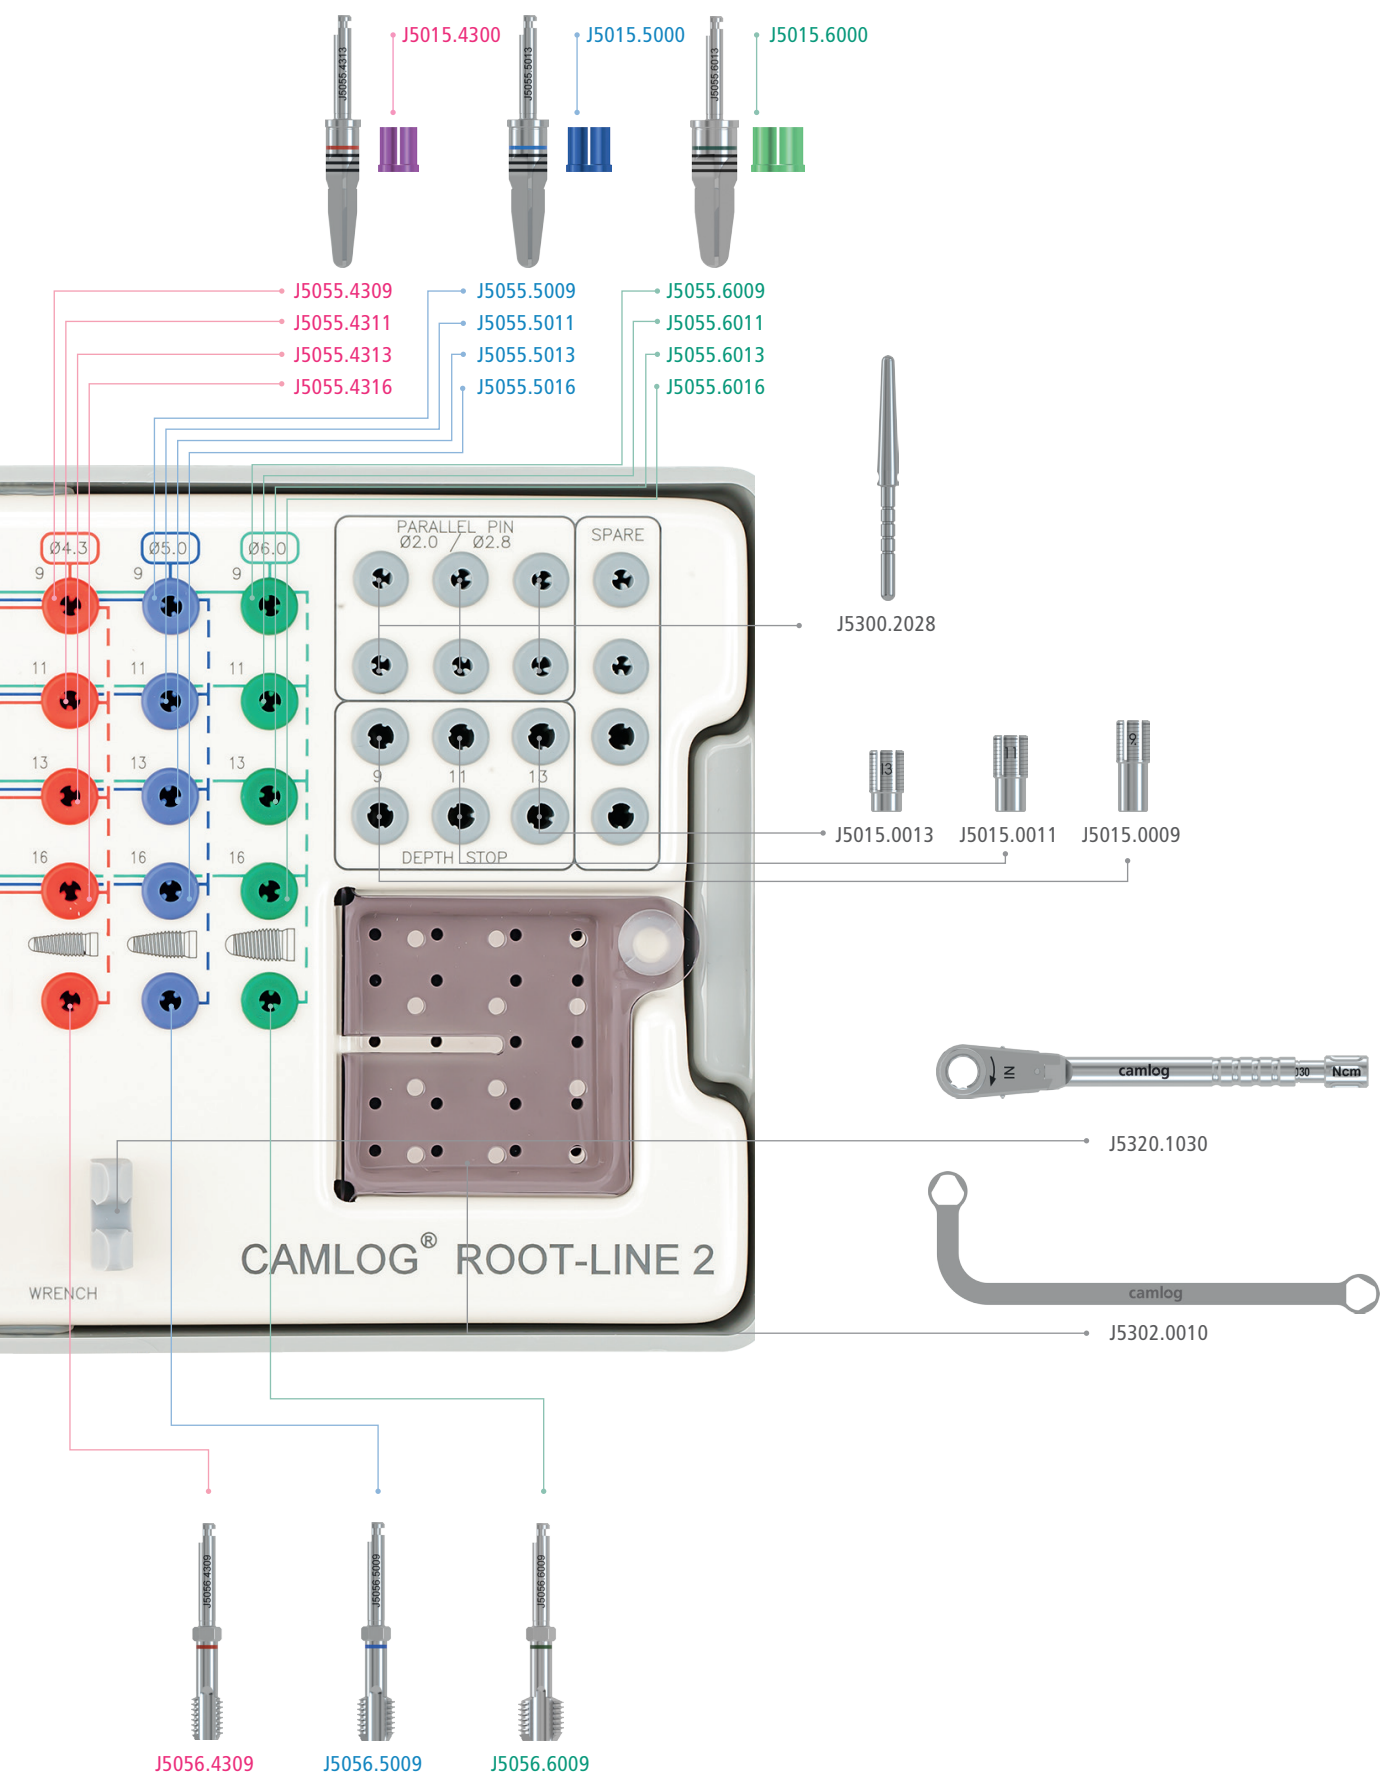



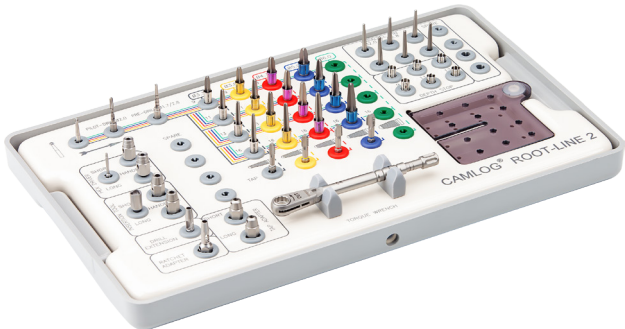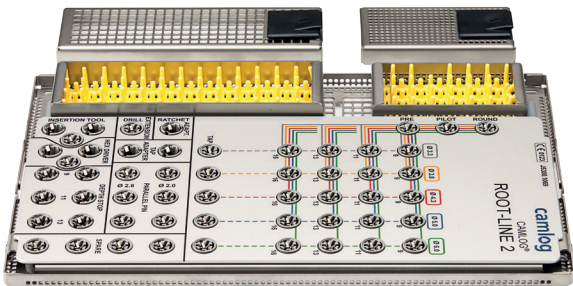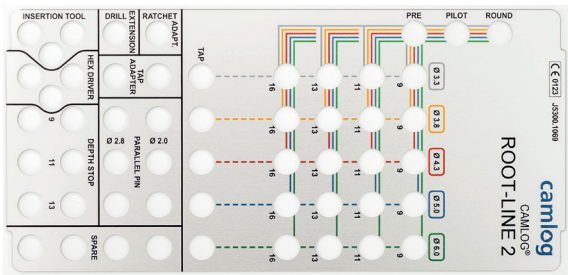




ROOT-LINE 2 – SURGERY SET

	Article	Art.-No.
 <p>A white plastic tray containing various surgical instruments. The instruments are organized into compartments and color-coded: red, yellow, green, blue, and silver. A torque wrench and a holding key are also visible. The tray is labeled 'CAMLOG® ROOT-LINE 2'.</p>	<p>Surgery set CAMLOG® ROOT-LINE 2 Contains all necessary color-code ordered surgical instruments, incl. torque wrench and holding key for insertion post (drills and taps for Ø 6.0 mm are not included)</p>	J5300.0059
 <p>A white plastic tray with a grid of circular holes. The holes are color-coded: red, yellow, green, blue, and silver. The tray is labeled 'CAMLOG® ROOT-LINE 2'.</p>	<p>Surgery wash tray CAMLOG® ROOT-LINE 2 incl. pattern, without content</p>	J5300.8969
 <p>A white plastic tray with a grid of circular holes. The holes are color-coded: red, yellow, green, blue, and silver. The tray is labeled 'CAMLOG® ROOT-LINE 2'.</p>	<p>Pattern for surgery wash tray CAMLOG® ROOT-LINE 2</p>	J5300.1069






ROOT-LINE 2 – SURGICAL INSTRUMENTS

	Article	Art.-No.	Ø	L
	Form drill ROOT-LINE 2 resterilizable Material Stainless steel	J5055.3309	3.3 mm	9 mm
		J5055.3311		11 mm
		J5055.3313		13 mm
		J5055.3316		16 mm
		J5055.3809	3.8 mm	9 mm
		J5055.3811		11 mm
		J5055.3813		13 mm
		J5055.3816		16 mm
		J5055.4309	4.3 mm	9 mm
		J5055.4311		11 mm
		J5055.4313		13 mm
		J5055.4316		16 mm
		J5055.5009	5.0 mm	9 mm
		J5055.5011		11 mm
		J5055.5013		13 mm
		J5055.5016		16 mm
		J5055.6009	6.0 mm	9 mm
		J5055.6011		11 mm
		J5055.6013		13 mm
		J5055.6016		16 mm
	Depth stop for form drill SCREW-LINE und ROOT-LINE 2 resterilizable Material Titanium alloy	J5015.3300	3.3 mm	-
		J5015.3800	3.8 mm	
		J5015.4300	4.3 mm	
		J5015.5000	5.0 mm	
		J5015.6000	6.0 mm	
	Tap ROOT-LINE 2 with hexagon, resterilizable Material Stainless steel	J5056.3309	3.3 mm	-
		J5056.3809	3.8 mm	
		J5056.4309	4.3 mm	
		J5056.5009	5.0 mm	
		J5056.6009	6.0 mm	

GENERAL SURGICAL INSTRUMENTS

	Article	Art.-No.	Ø	L
	Round bur resterilizable Material Stainless steel	J5050.2300	2.3 mm	-
	Pilot drill without coil, resterilizable Material Stainless steel	J5051.2003	2.0 mm	-
	Pilot drill SCREW-LINE* resterilizable Material Stainless steel	J5051.2000	2.0 mm	-
	Pre-drill SCREW-LINE* resterilizable Material Stainless steel	J5051.2800	1.7 – 2.8 mm	-

* Can also be used for the preparation of the implant bed for CAMLOG® ROOT-LINE 2 implants

	Article	Art.-No.	Ø	L
	Depth stop SCREW-LINE* for pilot drill (J5051.2000) and pre-drill (J5051.2800), sterilizable Material Stainless steel	J5015.0009	-	9 mm
		J5015.0011		11 mm
		J5015.0013		13 mm
	Bone profiler Ø 5.0 mm Material Stainless steel	J5003.3350	3.3 mm	-
	Bone profiler Ø 6.0 mm Material Stainless steel	J5003.4360	3.8 mm 4.3 mm	-
	Bone profiler Ø 7.0 mm Material Stainless steel	J5003.5070	5.0 mm	-
	CAMLOG® Guiding pin for bone profiler Material Titanium alloy	J5002.3300	3.3 mm	-
		J5002.3800	3.8 mm	
		J5002.4300	4.3 mm	
		J5002.5000	5.0 mm	








* Can also be used for the preparation of the implant bed for CAMLOG® ROOT-LINE 2 implants

GENERAL SURGICAL INSTRUMENTS

	Article	Art.-No.	Dimension
	Paralleling pin SCREW-LINE* with depth marks Material Titanium alloy	J5300.2028	Ø 1.7 – 2.8 mm/ 2.0 mm
	Drill extension ISO shaft (not for drills with internal irrigation) Material Stainless steel	J5002.0006	26.5 mm
	Tap adapter, short for tap SCREW-LINE* Material Stainless steel	J5322.0010	18.0 mm
	Tap adapter, long for tap SCREW-LINE* Material Stainless steel	J5322.0011	23.0 mm
	Driver for screw implants, with ISO shaft for angled hand piece Material Stainless steel	J5300.0007**	27.5 mm

* Can also be used for the preparation of the implant bed for CAMLOG® ROOT-LINE 2 implants





** only for use with CAMLOG® SCREW-LINE implants with Art. No. K1042.xxxx and K1052.xxxx, as well as with CAMLOG® ROOT-LINE 2 implants with Art. No. K1032.xxxx.

	Article	Art.-No.	Dimension
	Driver, short for screw implants, manual/wrench, with borehole for screwdriver, hex, long Material Stainless steel	J5300.0008*	18.0 mm
	Driver, long for screw implants, manual/wrench Material Stainless steel	J5300.0009*	27.0 mm
	Driver, extra short for screw implants, manual/wrench Material Stainless steel	J5300.0031**	13.7 mm
	Driver, short for screw implants, manual/wrench Material Stainless steel	J5300.0032**	19.2 mm
	Driver, long for screw implants, manual/wrench Material Stainless steel	J5300.0033**	24.8 mm
	Driver, short for screw implants, with ISO-shaft for angled hand piece Material Stainless steel	J5300.0034**	19.1 mm
	Driver, long for screw implants, with ISO-shaft for angled hand piece Material Stainless steel	J5300.0035**	28.2 mm






* only for use with CAMLOG® SCREW-LINE implants with Art. No. K1042.xxxx and K1052.xxxx, as well as with CAMLOG® ROOT-LINE 2 implants with Art. No. K1032.xxxx.

** only for use with CAMLOG® SCREW-LINE implants with Art. No. K1044.xxxx and K1054.xxxx.






GENERAL SURGICAL INSTRUMENTS

	Article	Art.-No.	Dimension
	Cardanic driver (30°) for screw implants, adjustable length Material Stainless steel	J5300.0010*	-
	PickUp instrument holder for carrying implants Material Stainless steel	J5300.0030	-
	Adapter ISO shaft for angled hand piece Material Stainless steel	J5002.0011	21.0 mm
	Holding key for insertion post Material Stainless steel	J5302.0010	-




* only for use with CAMLOG® SCREW-LINE implants with Art. No. K1042.xxxx and K1052.xxxx, as well as with CAMLOG® ROOT-LINE 2 implants with Art. No. K1032.xxxx.

	Article	Art.-No.	Dimension
	Adapter for screw implants, long for CAMLOG® SCREW-LINE and ROOT-LINE 2 Implants Material Stainless steel	K5302.3310	3.3 mm
		K5302.3810	3.8 mm
		K5302.4310	4.3 mm
	Holding sleeve for screw implants color-coded Material titanium alloy	J5302.3300	3.3 mm
		J5302.3800	3.8 mm
		J5302.4300	4.3 mm
	Screwdriver hex, extra short, manual/wrench Material Stainless steel	J5317.0510	14.5 mm
	Screwdriver hex, short, manual/wrench Material Stainless steel	J5317.0501	22.5 mm
	Screwdriver hex, long, manual/wrench Material Stainless steel	J5317.0502	30.3 mm

GENERAL SURGICAL INSTRUMENTS




	Article	Art.-No.	Dimension
	Screwdriver hex, short, ISO shaft Material Stainless steel	J5317.0504	18.0 mm
	Screwdriver hex, long, ISO shaft Material Stainless steel	J5317.0503	26.0 mm
	Manual screwdriver, hex without wrench head connection Material Stainless steel	J5317.0511	23.0 mm
	Cleaning needle for drills with internal irrigation Material Stainless steel	J5002.0012	-
	Cleaning cannula for drills with internal irrigation Material Stainless steel	J5002.0020	-

SCREW-LINE – OSTEOTOMY SET

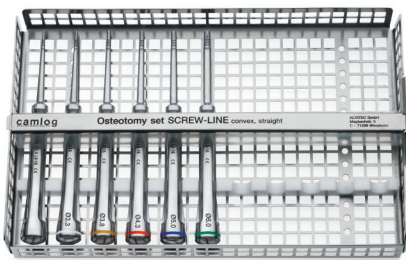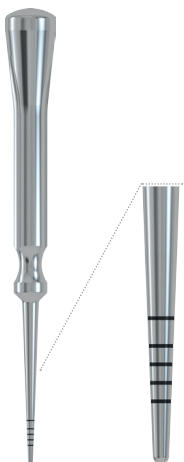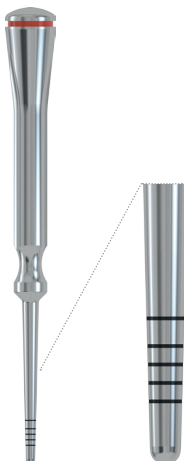
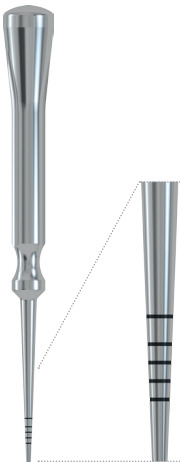
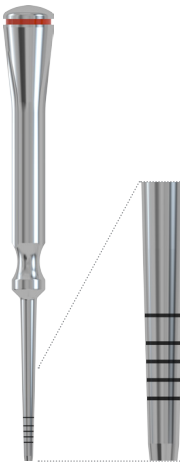
	Article	Art.-No.	Ø
	Osteotomy set CAMLOG®/ CONELOG® SCREW-LINE straight convex Material Stainless steel	J5418.0020	-
	Pre-Osteotome SCREW-LINE straight convex Material Stainless steel	J5417.2800*	1.7 – 2.8 mm
	Osteotome SCREW-LINE straight convex Material Stainless steel	J5418.3300*	3.3 mm
		J5418.3800*	3.8 mm
		J5418.4300*	4.3 mm
		J5418.5000*	5.0 mm
		J5418.6000*	6.0 mm

* These products are also included in the osteotomy set CAMLOG®/CONELOG® SCREW-LINE straight convex.

SCREW-LINE – OSTEOTOMY SET

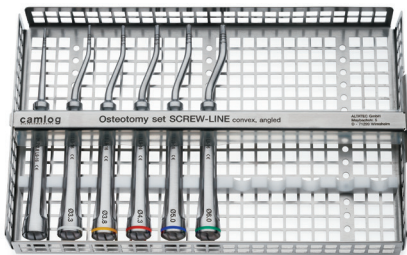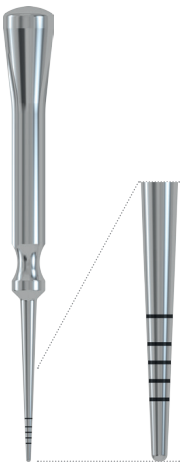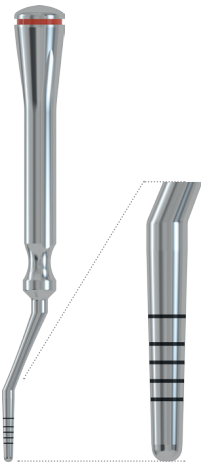
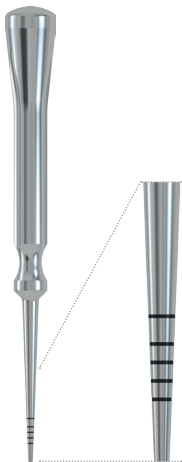
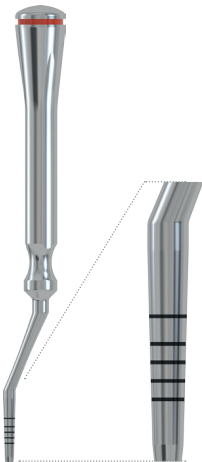
	Article	Art.-No.	Ø
	Osteotomy set CAMLOG®/CONELOG® SCREW-LINE angled convex Material Stainless steel	J5418.0030	-
	Pre-Osteotome SCREW-LINE straight convex Material Stainless steel	J5417.2800*	1.7 – 2.8 mm
	Osteotome SCREW-LINE angled convex Material Stainless steel	J5418.3310*	3.3 mm
		J5418.3810*	3.8 mm
		J5418.4310*	4.3 mm
		J5418.5010*	5.0 mm
		J5418.6010*	6.0 mm

* These products are also included in the osteotomy set CAMLOG®/CONELOG® SCREW-LINE angled convex.

	Article	Art.-No.	Ø
	Osteotomy set CAMLOG®/ CONELOG® SCREW-LINE straight concave Material Stainless steel	J5420.0020	-
	Pre-Osteotome SCREW-LINE straight concave Material Stainless steel	J5419.2800*	1.7 – 2.8 mm
	Osteotome SCREW-LINE straight concave Material Stainless steel	J5420.3300*	3.3 mm
		J5420.3800*	3.8 mm
		J5420.4300*	4.3 mm
		J5420.5000*	5.0 mm
		J5420.6000*	6.0 mm





* These products are also included in the osteotomy set CAMLOG®/CONELOG® SCREW-LINE straight concave.

SCREW-LINE – OSTEOTOMY SET

	Article	Art.-No.	Ø
	Osteotomy set CAMLOG®/ CONELOG® SCREW-LINE angled concave Material Stainless steel	J5420.0030	-
	Pre-Osteotome SCREW-LINE straight concave Material Stainless steel	J5419.2800*	1.7 – 2.8 mm
	Osteotome SCREW-LINE angled concave Material Stainless steel	J5420.3310*	3.3 mm
		J5420.3810*	3.8 mm
		J5420.4310*	4.3 mm
		J5420.5010*	5.0 mm
		J5420.6010*	6.0 mm




* These products are also included in the osteotomy set CAMLOG®/CONELOG® SCREW-LINE angled concave.

ALTAPIN SET



	Article	Art.-No.
	ALTApin set Membrane fixation system, resterilizable Material Plastic/titanium alloy/ stainless steel	M5600.0110
	ALTApin Tray (without content) Material Plastic	M5600.0210
	ALTApin applicator, straight incl. activator Material Stainless steel	M5100.0010*
	ALTApin applicator, angled 90° incl. activator Material Stainless steel	M5100.0030

* These products are included in the ALTApin set.

ALTAPIN SET




	Article	Art.-No.
	ALTApin applicator, straight, work element incl. activator Material Stainless steel	M5200.0010
	ALTApin pricker Material Stainless steel	M5100.0050*
	ALTApin membrane fixator Material Stainless steel	M5100.0070*

* These products are included in the ALTApin set.

	Article	Art.-No.
	ALTApin surgery mallet Material Stainless steel	M5100.0100
	ALTApin single patient drill, ISO shaft Material Stainless steel	M5500.0050
	ALTApin pricker, insert Material Stainless steel	M5200.0055*
	ALTApin magazine 7 titanium pins, sterile, 1 unit Material Titanium alloy	M1000.0050*
	ALTApin magazine 7 titanium pins, sterile, 3 unit Material Titanium alloy	M1000.0100


* These products are included in the ALTApin set.

HEALING CAPS

	Article	Art.-No.	Ø	GH	G Ø
	CAMLOG® Healing cap, cylindrical sterile Material Titanium alloy	J2015.3320	3.3 mm	2.0 mm	3.3 mm
		J2015.3340		4.0 mm	3.3 mm
		J2015.3820	3.8 mm	2.0 mm	3.8 mm
		J2015.3840		4.0 mm	3.8 mm
		J2015.3860*		6.0 mm	3.8 mm
		J2015.4320	4.3 mm	2.0 mm	4.3 mm
		J2015.4340		4.0 mm	4.3 mm
		J2015.4360*		6.0 mm	4.3 mm
		J2015.5020	5.0 mm	2.0 mm	5.0 mm
		J2015.5040		4.0 mm	5.0 mm
		J2015.5060*		6.0 mm	5.0 mm
		J2015.6020	6.0 mm	2.0 mm	6.0 mm
		J2015.6040		4.0 mm	6.0 mm
		J2015.6060*		6.0 mm	6.0 mm
	CAMLOG® Healing cap, wide body sterile Material Titanium alloy	J2014.3320	3.3 mm	2.0 mm	4.5 mm
		J2014.3340		4.0 mm	4.5 mm
		J2014.3820	3.8 mm	2.0 mm	4.9 mm
		J2014.3840		4.0 mm	5.0 mm
		J2014.3860		6.0 mm	5.0 mm
		J2014.4320	4.3 mm	2.0 mm	5.4 mm
		J2014.4340		4.0 mm	5.5 mm
		J2014.4360		6.0 mm	5.5 mm
		J2014.5020	5.0 mm	2.0 mm	6.1 mm
		J2014.5040		4.0 mm	6.2 mm
		J2014.5060		6.0 mm	6.2 mm
		J2014.6020	6.0 mm	2.0 mm	7.1 mm
		J2014.6040		4.0 mm	7.2 mm
		J2014.6060		6.0 mm	7.2 mm
	CAMLOG® Healing cap, bottleneck sterile Material Titanium alloy	J2011.3340	3.3 mm	4.0 mm	3.5 mm
		J2011.3840	3.8 mm	4.0 mm	4.0 mm
		J2011.3860		6.0 mm	4.0 mm
		J2011.4340	4.3 mm	4.0 mm	4.5 mm
		J2011.4360		6.0 mm	4.5 mm
		J2011.5040	5.0 mm	4.0 mm	5.2 mm
		J2011.5060		6.0 mm	5.2 mm
		J2011.6040	6.0 mm	4.0 mm	6.2 mm
		J2011.6060		6.0 mm	6.2 mm

* suitable for bite registration

HEALING CAPS PLATFORM SWITCHING






	Article	Art.-No.	Ø	GH	G Ø
PS 	CAMLOG® Healing cap PS, cylindrical sterile, for Platform Switching with CAMLOG® Implants with K article number Material titanium alloy	K2005.3820	3.8 mm	2.0 mm	3.3 mm
		K2005.3840		4.0 mm	3.3 mm
		K2005.3860*		6.0 mm	3.3 mm
		K2005.4320	4.3 mm	2.0 mm	3.8 mm
		K2005.4340		4.0 mm	3.8 mm
		K2005.4360*		6.0 mm	3.8 mm
		K2005.5020	5.0 mm	2.0 mm	4.4 mm
		K2005.5040		4.0 mm	4.4 mm
		K2005.5060*		6.0 mm	4.4 mm
		K2005.6020	6.0 mm	2.0 mm	5.1 mm
		K2005.6040		4.0 mm	5.1 mm
		K2005.6060*		6.0 mm	5.1 mm
PS 	CAMLOG® Healing cap PS, wide body sterile, for Platform Switching with CAMLOG® Implants with K article number Material titanium alloy	K2004.3840	3.8 mm	4.0 mm	5.0 mm
		K2004.3860		6.0 mm	5.0 mm
		K2004.4340	4.3 mm	4.0 mm	5.5 mm
		K2004.4360		6.0 mm	5.5 mm
		K2004.5040	5.0 mm	4.0 mm	6.2 mm
		K2004.5060		6.0 mm	6.2 mm
		K2004.6040	6.0 mm	4.0 mm	7.2 mm
		K2004.6060		6.0 mm	7.2 mm
PS 	CAMLOG® Healing cap PS, bottleneck sterile, for Platform Switching with CAMLOG® Implants with K article number Material titanium alloy	K2001.3840	3.8 mm	4.0 mm	4.0 mm
		K2001.3860		6.0 mm	4.0 mm
		K2001.4340	4.3 mm	4.0 mm	4.5 mm
		K2001.4360		6.0 mm	4.5 mm
		K2001.5040	5.0 mm	4.0 mm	5.2 mm
		K2001.5060		6.0 mm	5.2 mm

* suitable for bite registration








IMPRESSION TAKING

	Article	Art.-No.	Ø
	CAMLOG® Impression posts, open tray incl. fixing screw (The fixing screw can be shortened extra-oral by 3 mm with a screwdriver, hex.) Material Titanium alloy	K2121.3300	3.3 mm
		K2121.3800	3.8 mm
		K2121.4300	4.3 mm
		K2121.5000	5.0 mm
		K2121.6000	6.0 mm
	CAMLOG® Impression posts, closed tray incl. impression cap, bite registration cap and fixing screw Material Titanium alloy/POM	K2110.3300	3.3 mm
		K2110.3800	3.8 mm
		K2110.4300	4.3 mm
		K2110.5000	5.0 mm
		K2110.6000	6.0 mm
	CAMLOG® Impression posts PS, open tray, for Platform Switching incl. fixing screw (The fixing screw can be shortened extra-oral by 3 mm with a screwdriver, hex) Material Titanium alloy	K2119.3800	3.8 mm
		K2119.4300	4.3 mm
		K2119.5000	5.0 mm
		K2119.6000	6.0 mm
	CAMLOG® Impression posts PS, closed tray, for Platform Switching incl. impression cap, bite registration cap and fixing screw Material Titanium alloy/POM	K2109.3800	3.8 mm
		K2109.4300	4.3 mm
		K2109.5000	5.0 mm
		K2109.6000	6.0 mm
	Impression caps for impression post, closed tray (5 units) Material POM	J2111.3300	3.3 mm
		J2111.3800	3.8 mm
		J2111.4300	4.3 mm
		J2111.5000	5.0 mm
		J2111.6000	6.0 mm



BITE REGISTRATION

	Article	Art.-No.	Ø
	CAMLOG® Bite registration posts incl. fixing screw and bite registration cap (also for Platform Switching) Material Titanium alloy/POM	J2140.3300	3.3 mm
		J2140.3800	3.8 mm
		J2140.4300	4.3 mm
		J2140.5000	5.0 mm
		J2140.6000	6.0 mm
	Bite registration caps (5 units) Material POM	J2112.3300	3.3 mm
		J2112.3800	3.8 mm
		J2112.4300	4.3 mm
		J2112.5000	5.0 mm
		J2112.6000	6.0 mm

FABRICATION OF THE PLASTER MODEL



	Article	Art.-No.	Ø
	CAMLOG® Lab analogs Material Titanium alloy	K3010.3300	3.3 mm
		K3010.3800	3.8 mm
		K3010.4300	4.3 mm
		K3010.5000	5.0 mm
		K3010.6000	6.0 mm

TEMPORARY RESTORATION

	Article	Art.-No.	Ø	GH
	CAMLOG® Temporary abutments, PEEK preparable, incl. abutment screw Material PEEK	K2241.3800	3.8 mm	-
		K2241.4300	4.3 mm	
		K2241.5000	5.0 mm	
		K2241.6000	6.0 mm	
	CAMLOG® Temporary abutments PS, PEEK, for Platform Switching preparable, incl. abutment screw Material PEEK	K2208.3800	3.8 mm	-
		K2208.4300	4.3 mm	
		K2208.5000	5.0 mm	
		K2208.6000	6.0 mm	
	CAMLOG® Temporary abutment, crown, titanium alloy incl. abutment screw Material Titanium alloy	K2239.3300	3.3 mm	-
		K2239.3800	3.8 mm	
		K2239.4300	4.3 mm	
		K2239.5000	5.0 mm	
		K2239.6000	6.0 mm	
	CAMLOG® Temporary abutment, bridge, titanium alloy incl. abutment screw Material Titanium alloy	J2339.3300	3.3 mm	-
		J2339.3800	3.8 mm	
		J2339.4300	4.3 mm	
		J2339.5000	5.0 mm	
		J2339.6000	6.0 mm	

ESTHOMIC® ABUTMENTS








Cemented crown and bridge restorations

	Article	Art.-No.	Ø	GH
	CAMLOG® Esthomic® Abutments, straight preparable, incl. abutment screw Material Titanium alloy	K2226.3810	3.8 mm	1.0 – 1.8 mm
		K2226.3830		3.0 – 4.5 mm
		K2226.4310	4.3 mm	1.0 – 1.8 mm
		K2226.4330		3.0 – 4.5 mm
		K2226.5010	5.0 mm	1.0 – 1.8 mm
		K2226.5030		3.0 – 4.5 mm
		K2226.6010	6.0 mm	1.0 – 1.8 mm
		K2226.6030		3.0 – 4.5 mm
	CAMLOG® Esthomic® Abutments, 15° angled, type A preparable, incl. abutment screw Material Titanium alloy	K2227.3810	3.8 mm	1.0 – 1.8 mm
		K2227.3830		3.0 – 4.5 mm
		K2227.4310	4.3 mm	1.0 – 1.8 mm
		K2227.4330		3.0 – 4.5 mm
		K2227.5010	5.0 mm	1.0 – 1.8 mm
		K2227.5030		3.0 – 4.5 mm
		K2227.6010	6.0 mm	1.0 – 1.8 mm
		K2227.6030		3.0 – 4.5 mm

CAMLOG® Abutments PS may only be used on CAMLOG® Implants with a K article number.

ESTHOMIC® ABUTMENTS



Cemented crown and bridge restorations

	Article	Art.-No.	Ø	GH
	CAMLOG® Esthomic® Abutments, 15° angled, type B preparable, incl. abutment screw Material Titanium alloy	K2228.3810	3.8 mm	1.0 – 1.8 mm
		K2228.3830		3.0 – 4.5 mm
		K2228.4310	4.3 mm	1.0 – 1.8 mm
		K2228.4330		3.0 – 4.5 mm
		K2228.5010	5.0 mm	1.0 – 1.8 mm
		K2228.5030		3.0 – 4.5 mm
		K2228.6010	6.0 mm	1.0 – 1.8 mm
		K2228.6030		3.0 – 4.5 mm
	CAMLOG® Esthomic® Abutments, 20° angled, type A preparable, incl. abutment screw Material Titanium alloy	K2231.3810	3.8 mm	1.0 – 1.8 mm
		K2231.3830		3.0 – 4.5 mm
		K2231.4310	4.3 mm	1.0 – 1.8 mm
		K2231.4330		3.0 – 4.5 mm
		K2231.5010	5.0 mm	1.0 – 1.8 mm
		K2231.5030		3.0 – 4.5 mm
		K2231.6010	6.0 mm	1.0 – 1.8 mm
		K2231.6030		3.0 – 4.5 mm
	CAMLOG® Esthomic® Abutments, 20° angled, type B preparable, incl. abutment screw Material Titanium alloy	K2232.3810	3.8 mm	1.0 – 1.8 mm
		K2232.3830		3.0 – 4.5 mm
		K2232.4310	4.3 mm	1.0 – 1.8 mm
		K2232.4330		3.0 – 4.5 mm
		K2232.5010	5.0 mm	1.0 – 1.8 mm
		K2232.5030		3.0 – 4.5 mm
		K2232.6010	6.0 mm	1.0 – 1.8 mm
		K2232.6030		3.0 – 4.5 mm
	CAMLOG® Esthomic® Abutments, Inset preparable, incl. abutment screw Material Titanium alloy	K2235.3315	3.3 mm	1.5 – 2.8 mm
		K2235.3815	3.8 mm	
		K2235.4315	4.3 mm	
		K2235.5015	5.0 mm	
		K2235.6015	6.0 mm	
	CAMLOG® Esthomic® Abutments PS, straight, for Platform Switching preparable, incl. abutment screw Material Titanium alloy	K2202.3815	3.8 mm	1.5 – 2.5
		K2202.4315	4.3 mm	
		K2202.5015	5.0 mm	
		K2202.6015	6.0 mm	
	CAMLOG® Esthomic® Abutments PS, 15° angled, type A, for Platform Switching preparable, incl. abutment screw Material Titanium alloy	K2203.3815	3.8 mm	1.5 – 2.5
		K2203.4315	4.3 mm	
		K2203.5015	5.0 mm	
		K2203.6015	6.0 mm	
	CAMLOG® Esthomic® Abutments PS, 15° angled, type B, for Platform Switching preparable, incl. abutment screw Material Titanium alloy	K2204.3815	3.8 mm	1.5 – 2.5
		K2204.4315	4.3 mm	
		K2204.5015	5.0 mm	
		K2204.6015	6.0 mm	

CAMLOG® Abutments PS may only be used on CAMLOG® Implants with a K article number.


UNIVERSAL ABUTMENTS

Cemented crown and bridge restorations

	Article	Art.-No.	Ø	Dimension
	CAMLOG® Universal abutments preparable, incl. abutment screw Material Titanium alloy	K2211.3300	3.3 mm*	-
		K2211.3800	3.8 mm	
		K2211.4300	4.3 mm	
		K2211.5000	5.0 mm	
		K2211.6000	6.0 mm	
	CAMLOG® Universal abutments PS for Platform Switching preparable, incl. abutment screw Material Titanium alloy	K2201.3800	3.8 mm	-
		K2201.4300	4.3 mm	
		K2201.5000	5.0 mm	
		K2201.6000	6.0 mm	


GOLD-PLASTIC ABUTMENT

Cemented crown and bridge restorations

	Article	Art.-No.	Ø	Noble metal weight
	CAMLOG® Gold-plastic abutment cast-on, incl. abutment screw Material Cast-on gold alloy/POM	K2246.3300	3.3 mm*	ca. 0.42 g
		K2246.3800	3.8 mm	ca. 0.46 g
		K2246.4300	4.3 mm	ca. 0.65 g
		K2246.5000	5.0 mm	ca. 0.81 g
		K2246.6000	6.0 mm	ca. 0.89 g

CERAMIC ABUTMENT

Crown restorations



	Article	Art.-No.	Ø	Dimension
	CAMLOG® Ceramic abutments, 2-parts, for bonded/cemented full ceramic crowns preparable, incl. titanium base, zirkonium oxide sleeve and abutment screw Material Titanium alloy/Zirkonium oxide	K2242.3340	3.3 mm*	-
		K2242.3840	3.8 mm	
		K2242.4340	4.3 mm	
		K2242.5040	5.0 mm	
		K2242.6040	6.0 mm	

CAMLOG® Abutments PS may only be used on CAMLOG® Implants with a K article number.

*only for crown restorations in the region of the upper lateral and lower lateral and central incisors (Ø 3.3 mm not for double crown restorations)




CERAMIC ABUTMENT

Crown restorations

	Article	Art.-No.	Ø	Dimension
	Zirkonium oxide sleeves for CAMLOG® Ceramic abutment, preparable Material Zirkonium oxide	J2242.3341	3.3 mm*	-
		J2242.3841	3.8 mm	
		J2242.4341	4.3 mm	
		J2242.5041	5.0 mm	
		J2242.6041	6.0 mm	
	CAMLOG® Titanium bases for CAMLOG® Ceramic abutment Material Titanium alloy	K2242.3342	3.3 mm*	-
		K2242.3842	3.8 mm	
		K2242.4342	4.3 mm	
		K2242.5042	5.0 mm	
		K2242.6042	6.0 mm	

LOGFIT® PROSTHETIC SYSTEM

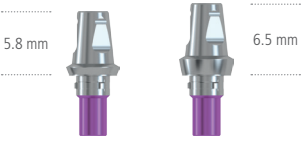

Cemented crown and bridge restorations

	Article	Art.-No.	Ø	GH
	CAMLOG® Logfit® Abutments incl. abutment screw Material Titanium alloy	K2550.3808	3.8 mm	0.8 mm
		K2550.3815		1.5 mm
		K2550.4308	4.3 mm	0.8 mm
		K2550.4315		1.5 mm
		K2550.5008	5.0 mm	0.8 mm
		K2550.5015		1.5 mm
		K2550.6008	6.0 mm	0.8 mm
		K2550.6015		1.5 mm
	Logfit® Impression caps Material POM	J2551.4300	3.8 mm	-
		J2551.4300	4.3 mm	
		J2551.6000	5.0 mm	
		J2551.6000	6.0 mm	
	Logfit® Analog Material Titanium alloy	J2552.4300	3.8 mm	-
		J2552.4300	4.3 mm	
		J2552.6000	5.0 mm	
		J2552.6000	6.0 mm	

*only for crown restorations in the region of the upper lateral and lower lateral and central incisors (Ø 3.3 mm not for double crown restorations)



LOGFIT® PROSTHETIC SYSTEM

Cemented crown and bridge restorations

	Article	Art.-No.	Ø
	Logfit® Plastic copings, for crowns (with rotation securing device) burn-out Material POM	J2553.4302	3.8 mm
		J2553.4302	4.3 mm
		J2553.6002	5.0 mm
		J2553.6002	6.0 mm
	Logfit® Plastic copings, for bridges (without rotation securing device) burn-out Material POM	J2553.4301	3.8 mm
		J2553.4301	4.3 mm
		J2553.6001	5.0 mm
		J2553.6001	6.0 mm




CAD/CAM PROSTHETICS

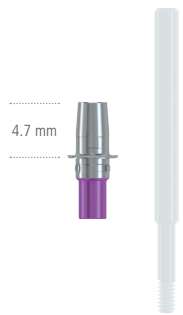Crown, bridge and hybrid restorations

	Article	Art.-No.	Ø
	CAMLOG® Titanium bases CAD/CAM, crown bonding base for individual CAD/CAM fabricated dental prosthesis, incl. abutment screw and Bonding aid (POM) Material Titanium alloy/POM	K2244.3348	3.3 mm*
		K2244.3848	3.8 mm
		K2244.4348	4.3 mm
		K2244.5048	5.0 mm
		K2244.6048	6.0 mm
	CAMLOG® Titanium bases CAD/CAM, bridge bonding base for individual CAD/CAM fabricated dental prosthesis, incl. abutment screw and Bonding aid (POM) Material Titanium alloy/POM	J2344.3348	3.3 mm
		J2344.3848	3.8 mm
		J2344.4348	4.3 mm
		J2344.5048	5.0 mm
		J2344.6048	6.0 mm

In order to achieve a high level of user friendliness and a high precision fit of the CAD/CAM fabricated abutments, the geometries of the CAMLOG® Titanium bases CAD/CAM are available as a CAD library for leading dental CAD systems. For more information see www.camlog.com/en/implant-systems/camlog/digital-technology.

*only for crown restorations in the region of the upper lateral and lower lateral and central incisors

	Article	Art.-No.	Ø
	CAMLOG® Modeling aids for CAMLOG® Titanium bases CAD/CAM burn-out, for fabricating mesostructures and crowns Material POM	J2244.3302	3.3 mm
		J2244.3802	3.8 mm
		J2244.4302	4.3 mm
		J2244.5002	5.0 mm
		J2244.6002	6.0 mm
	CAMLOG® Scanbodies for optical, 3-dimensional localization of CAMLOG® Implants in the mouth or CAMLOG® Lab analogs in the working model, incl. abutment screw, sterile Not compatible with the CEREC and inLab systems from Sirona Material PEEK	K2610.3310	3.3 mm
		K2610.3810*	3.8 mm
		K2610.4310*	4.3 mm
		K2610.6010*	5.0 mm
			6.0 mm
	CAMLOG® ScanPosts for Sirona Scanbody for digital recording of the CAMLOG® Implant or lab analog position, incl. abutment screw Material Titanium alloy	K2620.3306	3.3 mm
		K2620.3806*	3.8 mm
		K2620.4306*	4.3 mm
		K2620.5006*	5.0 mm
		K2620.6006*	6.0 mm

Matching Sirona Scanbodies size S for CAMLOG® ScanPosts and CAMLOG® Titanium base CAD/CAM crown with Ø 3.3/3.8/4.3 mm:

For Omnicam: Article number 6431311 For Bluecam: Article number 6431295

Matching Sirona Scanbodies size L for CAMLOG® ScanPosts and CAMLOG® Titanium base CAD/CAM crown with Ø 5.0/6.0 mm:

For Omnicam: Article number 6431329 For Bluecam: Article number 6431303

Sirona Scanbodies are available from Dentsply Sirona.

Information on the compatibility of the CAMLOG® Scanbody with suitable dental CAD systems is available at www.camlog.com/en/implant-systems/camlog/digital-technology.

* can also be used for Platform Switching

CAM TITANIUM BLANK

Milling production process of individualized one-piece abutments and healing caps by CAD/CAM technology

	Article	Art.-No.	Ø
	CAMLOG® CAM Titanium Blank, type IAC* Ø 12 mm, length 12.5 mm (2 units), sent with 2 separate packed abutment screws Material Titanium alloy	K2411.3313	3.3 mm
		K2411.3813	3.8 mm
		K2411.4313	4.3 mm
		K2411.6013	5.0 mm
			6.0 mm
	CAMLOG® CAM Titanium Blank, type ME** Ø 12 mm, length 20 mm (2 units), sent with 2 separate packed abutment screws Material Titanium alloy	K2421.3320	3.3 mm
		K2421.3820	3.8 mm
		K2421.4320	4.3 mm
		K2421.5020	5.0 mm
		K2421.6020	6.0 mm

ACCESSORIES FOR CAM-TITANIUM BLANKS, TYPE IAC

	Article	Art.-No.	Ø
	CAMLOG® Collet for CAM Blank, type IAC* Ø 6 mm, length 17 mm, incl. 2 fixing screws for CAM Blank, type IAC Material Stainless steel	K3720.3300	3.3 mm
		K3720.3800	3.8 mm
		K3720.4300	4.3 mm
		K3720.6000	5.0 mm
			6.0 mm

Type IAC*



For the milling process, the CAM titanium blank type IAC is fixated to the implant-abutment connection via the CAMLOG® Collet for CAM blanks. The machine-specific holders and adapters for the collet as well as the milling strategies are to be provided by the user.

Type ME**

For the milling process, the CAM titanium blank type ME is fixated with the front-facing groove of its cylindrical section via a milling holder for PreFace® Abutments from Medentika®. The machine-specific holders as well as the milling strategies are to be provided by the user.


Medentika® and Preface® are registered trademarks of Medentika GmbH, D-Hügelshheim.

ACCESSORIES FOR ABUTMENTS

	Article	Art.-No.	Ø	Thread
	CAMLOG® Abutment screw, hex for definitive screw retention of abutments into the implant Material Titanium alloy	J4005.1601	3.3 mm	M 1.6
			3.8 mm	
			4.3 mm	
		J4005.2001	5.0 mm	M 2.0
			6.0 mm	
	CAMLOG® Lab screw, hex for the fixation of abutments on the working model, brown anodized Material Titanium alloy	J4006.1601	3.3 mm	M 1.6
			3.8 mm	
			4.3 mm	
		J4006.2001	5.0 mm	M 2.0
			6.0 mm	

Lab screws may not be used on patients.








COMFOUR™ – OCCLUSALLY SCREW-RETAINED RESTORATIONS

	Article	Art.-No.	Type	Ø	GH	PP Ø
	CAMLOG® Bar abutment, straight sterile Material Titanium alloy	J2254.3305	-	3.3 mm	0.5 mm	4.3 mm
		J2254.3320			2.0 mm	
		J2254.3805		3.8 mm	0.5 mm	4.3 mm
		J2254.3820			2.0 mm	
		J2254.3840			4.0 mm	
		J2254.4305		4.3 mm	0.5 mm	4.3 mm
		J2254.4320			2.0 mm	
		J2254.4340			4.0 mm	
		J2254.5005		5.0 mm	0.5 mm	6.0 mm
		J2254.5020			2.0 mm	
		J2254.5040			4.0 mm	
	CAMLOG® Bar abutment, 17° angled incl. light blue anodized abutment screw with reduced head, sterile Material Titanium alloy	K2256.3325	A	3.3 mm	2.5 mm	4.3 mm
		K2256.3340			4.0 mm	
		K2257.3325	B		2.5 mm	
		K2257.3340			4.0 mm	
		K2256.3825	A	3.8 mm	2.5 mm	4.3 mm
		K2256.3840			4.0 mm	
		K2257.3825	B		2.5 mm	
		K2257.3840			4.0 mm	
		K2256.4325	A	4.3 mm	2.5 mm	4.3 mm
		K2256.4340			4.0 mm	
		K2257.4325	B		2.5 mm	
		K2257.4340			4.0 mm	
		K2256.5025	A	5.0 mm	2.5 mm	6.0 mm
		K2256.5040			4.0 mm	
		K2257.5025	B		2.5 mm	
		K2257.5040			4.0 mm	
	CAMLOG® Bar abutment, 30° angled incl. light blue anodized abutment screw with reduced head, sterile Material Titanium alloy	K2258.3325	A	3.3 mm	2.5 mm	4.3 mm
		K2258.3340			4.0 mm	
		K2259.3325	B		2.5 mm	
		K2259.3340			4.0 mm	
		K2258.3825	A	3.8 mm	2.5 mm	4.3 mm
		K2258.3840			4.0 mm	
		K2259.3825	B		2.5 mm	
		K2259.3840			4.0 mm	
		K2258.4325	A	4.3 mm	2.5 mm	4.3 mm
		K2258.4340			4.0 mm	
		K2259.4325	B		2.5 mm	
		K2259.4340			4.0 mm	
		K2258.5035	A	5.0 mm	3.5 mm	6.0 mm
		K2258.5050			5.0 mm	
		K2259.5035	B		3.5 mm	
		K2259.5050			5.0 mm	

	Article	Art.-No.	Ø			Dimension
	Healing cap for bar abutment partial light blue anodized, sterile	J2029.4300	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy	J2029.6000	5.0 mm			
	Impression cap for bar abutment, closed tray (bridge/bar) partial light blue anodized, sterile	J2129.4300	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy	J2129.6000	5.0 mm			
	Driver for impression caps and healing caps for bar abutments	J5300.0027	3.3 mm	3.8 mm	4.3 mm	19.1 mm
	Material Stainless steel	J5300.0028	5.0 mm			19.1 mm
	Bar lab analog for bar abutments	J3020.4300	3.3 mm	3.8 mm	4.3 mm	-
	Material Stainless steel	J3020.6000	5.0 mm			
	Scanning cap for bar abutments incl. prosthetic screw, light blue anodized, sterile	J2610.4300	3.3 mm	3.8 mm	4.3 mm	-
	Material PEEK	J2610.6000	5.0 mm			
	Aligning tool 17° for angled bar abutments, for insertion post	J2269.0003	-			-
	Material Stainless steel					
	Aligning tool 30° for angled bar abutments, for insertion post	J2269.0004	-			-
	Material Stainless steel					
	Titanium cap for bar abutment, for crown incl. prosthetic screw light blue anodized, sterile	J2259.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy	J2259.6001	5.0 mm			


COMFOUR™ – OCCLUSALLY SCREW-RETAINED RESTORATIONS

	Article	Art.-No.	Ø			Noble metal weight
	Titanium cap for bar abutment, for bridge incl. prosthetic screw light blue anodized, sterile	J2259.4302	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy	J2259.6002	5.0 mm			
	Crown base for bar abutment burn-out	J2256.4306	3.3 mm	3.8 mm	4.3 mm	-
	Material POM	J2256.6006	5.0 mm			
	Base for bar abutment burn-out	J2257.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material POM	J2257.6001	5.0 mm			
	Base for bar abutment cast-on	J2263.4300	3.3 mm	3.8 mm	4.3 mm	ca. 0.48 g
	Material Cast-on gold alloy/POM	J2263.6000	5.0 mm			ca. 0.70 g
	Base for bar abutment solderable	J2258.4300	3.3 mm	3.8 mm	4.3 mm	-
	Material Solderable gold alloy	J2258.6000	5.0 mm			
	Base for bar abutment, titanium laser-weldable	J2262.4300	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium Grade 4	J2262.6000	5.0 mm			
	Titanium bonding base for bar abutment Passive-Fit	J2260.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy	J2260.6001	5.0 mm			
	Bar sleeve for titanium bonding base burn-out, Passive-Fit, incl. Prosthetic screw for bar abutments, hex (only for fabrication of the cast framework in conjunction with bar sleeves for titanium bonding base Passive-Fit)	J2261.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material POM	J2261.6001	5.0 mm			
	Locator® Fixture for bar abutment	J2253.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy/TiN	J2253.6001	5.0 mm			




	Article	Art.-No.	Ø			Thread
	CAMLOG® Abutment screw with reduced head, hex, light blue anodized	J4004.1601	3.3 mm	3.8 mm	4.3 mm	M 1.6
	Material Titanium alloy	J4004.2001	5.0 mm			M 2.0
	CAMLOG® Lab screw with reduced head, hex, partial light blue anodized	J4004.1600	3.3 mm	3.8 mm	4.3 mm	M 1.6
	Material Titanium alloy	J4004.2000	5.0 mm			M 2.0
	Prosthetic screw for bar abutments hex, light blue anodized (for final fixation of the bar bases)	J4012.1601	3.3 mm	3.8 mm	4.3 mm	M 1.6
	Material Titanium alloy	J4012.2001	5.0 mm			M 2.0
	Lab prosthetic screw for bar abutment hex, brown anodized	J4013.1601	3.3 mm	3.8 mm	4.3 mm	M 1.6
	Material Titanium alloy	J4013.2001	5.0 mm			M 2.0
	Screw, hex, length 10 mm can be shortened by 2.5 mm, light blue anodized, sterile	J4012.1610	-			M 1.6
	Material Titanium alloy	J4012.2010				M 2.0
	Screw, hex, length 15 mm can be shortened by 2.5 mm, light blue anodized, sterile	J4012.1615	-			M 1.6
	Material Titanium alloy	J4012.2015				M 2.0
	Screw, hex, length 20 mm can be shortened by 2.5 mm, light blue anodized, sterile	J4012.1620	-			M 1.6
	Material Titanium alloy	J4012.2020				M 2.0

Lab screws may not be used on patients.

COMFOUR™ – OCCLUSALLY SCREW-RETAINED RESTORATIONS



	Article	Art.-No.	Ø	Thread
	Plastic screw for bar abutment hex, length 27 mm, sterile Material PEEK	J4009.1627	-	M 1.6
		J4009.2027		M 2.0

BALL ABUTMENT ANCHORING SYSTEM




	Article	Art.-No.	Ø	GH
	CAMLOG® Ball abutment sets, incl. male part and matrix CM Dalbo®-Plus red duplication aid/spacer, stabilizing ring and ball abutment analog Material Titanium alloy/Titanium Grade 4/ Gold alloy/Brass/Plastic	J2250.3315	3.3 mm	1.5 mm
		J2250.3330		3.0 mm
		J2250.3815	3.8 mm	1.5 mm
		J2250.3830		3.0 mm
		J2250.3845	4.3 mm	4.5 mm
		J2250.4315		1.5 mm
		J2250.4330		3.0 mm
		J2250.4345	5.0 mm	4.5 mm
		J2250.5015		1.5 mm
		J2250.5030	5.0 mm	3.0 mm
		J2250.5045		4.5 mm
	CAMLOG® Ball abutments, male part incl. stabilizing ring Material Titanium alloy/Plastic	J2249.3315	3.3 mm	1.5 mm
		J2249.3330		3.0 mm
		J2249.3815	3.8 mm	1.5 mm
		J2249.3830		3.0 mm
		J2249.3845	4.3 mm	4.5 mm
		J2249.4315		1.5 mm
		J2249.4330		3.0 mm
		J2249.4345	5.0 mm	4.5 mm
		J2249.5015		1.5 mm
		J2249.5030	5.0 mm	3.0 mm
		J2249.5045		4.5 mm
	Matrix CM Dalbo®-Plus for ball abutment, incl. lamella retention insert Material Titanium Grade 4/Gold alloy	J2250.0005	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	

Dalbo®-Plus is a registered trademark of Cendres + Métaux SA, Biel, Switzerland.






BALL ABUTMENT ANCHORING SYSTEM





	Article	Art.-No.	Ø	GH
	Lamella retention insert for matrix CM Dalbo®-Plus Material Gold alloy	J2250.0007	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	
	Ball abutment analogs incl. stabilizing ring Material Brass/Plastic	J3015.3300	3.3 mm	-
		J3015.3800	3.8 mm	
		J3015.4300	4.3 mm	
		J3015.5000	5.0 mm	

LOCATOR® ANCHORING SYSTEM

	Article	Art.-No.	Ø	GH
	CAMLOG® Locator® Abutments Material Titanium alloy/TiN	J2253.3310	3.3 mm	1.0 mm
		J2253.3320		2.0 mm
		J2253.3330		3.0 mm
		J2253.3340		4.0 mm
		J2253.3810	3.8 mm	1.0 mm
		J2253.3820		2.0 mm
		J2253.3830		3.0 mm
		J2253.3840		4.0 mm
		J2253.3850		5.0 mm
		J2253.4310	4.3 mm	1.0 mm
		J2253.4320		2.0 mm
		J2253.4330		3.0 mm
		J2253.4340		4.0 mm
		J2253.4350		5.0 mm
		J2253.5010	5.0 mm	1.0 mm
		J2253.5020		2.0 mm
		J2253.5030		3.0 mm
		J2253.5040		4.0 mm
		J2253.5050		5.0 mm
	Locator® Impression cap (4 units) Material Aluminum/Polyethylene	J2253.0200	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	
	Locator® Analog (4 units) Material Aluminum	J2253.0340	3.3 mm	-
			3.8 mm	
			4.3 mm	
		J2253.0350	5.0 mm	

LOCATOR® ANCHORING SYSTEM



	Article	Art.-No.	Ø
	Locator® Male processing package (2 units) Content per package: 1 Titanium housing with processing replacement male 1 Block out spacer white 1 Replacement male clear 1 Replacement male pink 1 Replacement male blue Material Titanium alloy/Polyethylene/Teflon/Nylon	J2253.0102	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Male processing package for extended range (2 units) Content per package: 1 Titanium housing with processing replacement male 1 Block out spacer white 1 Replacement male green, 1 Replacement male orange, 1 Replacement male red Material Titanium alloy/Polyethylene/Teflon/Nylon	J2253.0112	3.8 mm
			4.3 mm
			5.0 mm
	Locator® Block out spacer (20 units) Material Teflon	J2253.0401	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Processing replacement male (4 units) Material Polyethylene	J2253.0402	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male clear, STRONG, Div.: 0°-10° (4 units) Material Nylon	J2253.1005	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm

	Article	Art.-No.	Ø
	Locator® Replacement male pink, MEDIUM, Div.: 0° – 10° (4 units) Material Nylon	J2253.1003	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male blue, LIGHT, Div.: 0° – 10° (4 units) Material Nylon	J2253.1002	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male for extended range* green, STRONG, Div.: 10° – 20° (4 units) Material Nylon	J2253.2004	3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male for extended range* orange, MEDIUM, Div.: 10° – 20° (4 units) Material Nylon	J2253.2003	3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male for extended range* red, LIGHT, Div.: 10° – 20° (4 units) Material Nylon	J2253.2002	3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male for extended range* gray, NO RETENTION, Div.: 0° – 20° (4 units) Material Nylon	J2253.2000	3.8 mm
			4.3 mm
			5.0 mm

* not permitted for implant Ø 3.3 mm



Manufacturer Locator®: Zest Anchors, 2875 Loker Avenue East, Carlsbad, California 92010, USA
Locator® is a registered trademark of Zest Anchors

DOUBLE CROWN RESTORATION

	Article	Art.-No.	Ø
 <p>11 mm</p>	CAMLOG® Universal abutments for double crown restorations preparable, incl. Abutment screw Material Titanium alloy	K2211.3800	3.8 mm
		K2211.4300	4.3 mm
		K2211.5000	5.0 mm
		K2211.6000	6.0 mm
 <p>PS</p> <p>11 mm</p>	CAMLOG® Universal abutments PS for double crown restorations for Platform Switching preparable, incl. Abutment screw Material Titanium alloy	K2201.3800	3.8 mm
		K2201.4300	4.3 mm
		K2201.5000	5.0 mm
		K2201.6000	6.0 mm
 <p>12 mm</p>	CAMLOG® Telescope abutments for double crown restorations preparable, incl. Abutment screw Material Titanium alloy	K2212.3800	3.8 mm
		K2212.4300	4.3 mm
		K2212.5000	5.0 mm
		K2212.6000	6.0 mm

CAMLOG® Abutments PS may only be used on CAMLOG® Implants with a K article number.

ACCESSORIES FOR CAMLOG® ABUTMENTS

	Article	Art.-No.	Ø	Thread
	CAMLOG® Abutment screw, hex for definitive screw retention of abutments into the implant Material Titanium alloy	J4005.1601	3.3 mm	M 1.6
			3.8 mm	
			4.3 mm	
		J4005.2001	5.0 mm	M 2.0
			6.0 mm	
	CAMLOG® Lab screw, hex for the fixation of abutments on the working model, brown anodized Material Titanium alloy	J4006.1601	3.3 mm	M 1.6
			3.8 mm	
			4.3 mm	
		J4006.2001	5.0 mm	M 2.0
			6.0 mm	

Lab screws may not be used on patients.




PROSTHETIC INSTRUMENTS

	Article	Art.-No.	L
	Torque wrench with continuous torque adjustment until maximal 30 Ncm Material Stainless steel	J5320.1030	-
	Driver for ball abutment, manual/wrench Material Stainless steel	J5300.0011	18.3 mm
	Screwdriver Activator for ball abutment matrix CM Dalbo®-Plus Material Stainless steel	J5315.0005	-
	Driver for straight bar abutment, short Ø 3.3/3.8/4.3 mm Material Stainless steel	J5300.0020	18.6 mm






	Article	Art.-No.	L
	Driver for straight bar abutment, short Ø 5.0/6.0 mm Material Stainless steel	J5300.0025	18.6 mm
	Driver for impression cap and healing cap for bar abutment Ø 3.3/3.8/4.3 mm Material Stainless steel	J5300.0027	19.1 mm
	Driver for impression cap and healing cap for bar abutment Ø 5.0/6.0 mm Material Stainless steel	J5300.0028	19.1 mm
	Driver for Locator®, manual/wrench Material Stainless steel	J2253.0001	24.3 mm
	Locator® Instrument threepart Material Stainless steel	J2253.0002	83.0 mm
	Locator® Angle measurement guide Material Stainless steel	J2253.0003	-
	Locator® Parallel post (4 units) Material Polyethylene	J2253.0004	-


PROSTHETIC INSTRUMENTS

	Article	Art.-No.	L
	Prosthetic tray (without content) Material Plastic	J5330.8500	-
	Prosthetic tray universal (without content), resterilizable Material Radel®, silicone	J5330.8700	-
	Screwdriver Hex, extra short, manual/wrench Material Stainless steel	J5317.0510	14.5 mm
	Screwdriver Hex, short, manual/wrench Material Stainless steel	J5317.0501	22.5 mm
	Screwdriver Hex, long, manual/wrench Material Stainless steel	J5317.0502	30.3 mm


	Article	Art.-No.	L
	Screwdriver Hex, short, ISO shaft Material Stainless steel	J5317.0504	18.0 mm
	Screwdriver Hex, long, ISO shaft Material Stainless steel	J5317.0503	26.0 mm
	Manual screwdriver Hex, without wrench head connection Material Stainless steel	J5317.0511	23.0 mm

INSTRUMENTS FOR DENTAL TECHNICIANS

	Article	Art.-No.	Ø
	Universal holder incl. 2 CAMLOG® Lab screws, hex, and 1 each CAMLOG® Abutment collet Ø 3.3/3.8/4.3/5.0/6.0 mm Material Stainless steel/Titanium alloy	J3709.0010	-
	Universal holder Material Stainless steel	J3709.0015	-
	CAMLOG® Abutment collets for universal holder, for grinding CAMLOG® Abutments Material Titanium alloy	J3709.3300	3.3 mm
		J3709.3800	3.8 mm
		J3709.4300	4.3 mm
		J3709.5000	5.0 mm
		J3709.6000	6.0 mm
	Collets for zirconium oxide sleeve for universal holder Material PEEK	J3712.4300	3.3 mm
			3.8 mm
			4.3 mm
		J3712.6000	5.0 mm
			6.0 mm
	Reamers for dilating the plaster model, for universal holder incl. color-coded guide pin Material Stainless steel/Titanium alloy	J3706.3300	3.3 mm
		J3706.3800	3.8 mm
		J3706.4300	4.3 mm
		J3706.5000	5.0 mm
		J3706.6000	6.0 mm
	Reworking reamer, for base for bar abutment plane surface/cone seat, burn-out Material Stainless steel	J3711.0010	3.3 mm
			3.8 mm
			4.3 mm
		J3711.0015	5.0 mm
			6.0 mm

	Article	Art.-No.	Ø
	Reworking reamer, for base for bar abutment screw seat, burn-out	J3711.0020	3.3 mm
			3.8 mm
			4.3 mm
	Material Stainless steel	J3711.0025	5.0 mm
			6.0 mm

SELECTION ABUTMENTS


	Article	Art.-No.	Ø
	CAMLOG® Selection abutment kit (Content: 2 units each, according table below)	K8011.1000	-


Content: CAMLOG® Selection abutment kit

Article	Material	Ø			GH
CAMLOG® Esthomic® Selection abutment, straight*	POM	3.8 mm	4.3 mm	5.0 mm	1.0 – 1.8
					3.0 – 4.5
CAMLOG® Esthomic® Selection abutment, 15° angled, type A*		3.8 mm	4.3 mm	5.0 mm	1.0 – 1.8
CAMLOG® Esthomic® Selection abutment, 15° angled, type B*		3.8 mm	4.3 mm	5.0 mm	1.0 – 1.8
CAMLOG® Esthomic® Selection abutment, 20° angled, type A*		3.8 mm	4.3 mm	5.0 mm	1.0 – 1.8
CAMLOG® Esthomic® Selection abutment, 20° angled, type B*		3.8 mm	4.3 mm	5.0 mm	1.0 – 1.8
CAMLOG® Vario SR selection abutment, straight*		3.8 mm	4.3 mm	5.0 mm	0.8
CAMLOG® Vario SR selection abutment, 20° angled*		3.8 mm			3.1 – 1.8
		4.3 mm			3.2 – 1.7
		5.0 mm			3.9 – 2.2
CAMLOG® Vario SR selection abutment, 30° angled*		3.8 mm			3.1 – 1.2
		4.3 mm			3.2 – 1.0
	5.0 mm			4.0 – 1.5	

Attention, do not use selection abutments on patients!

* These products are not available singly.



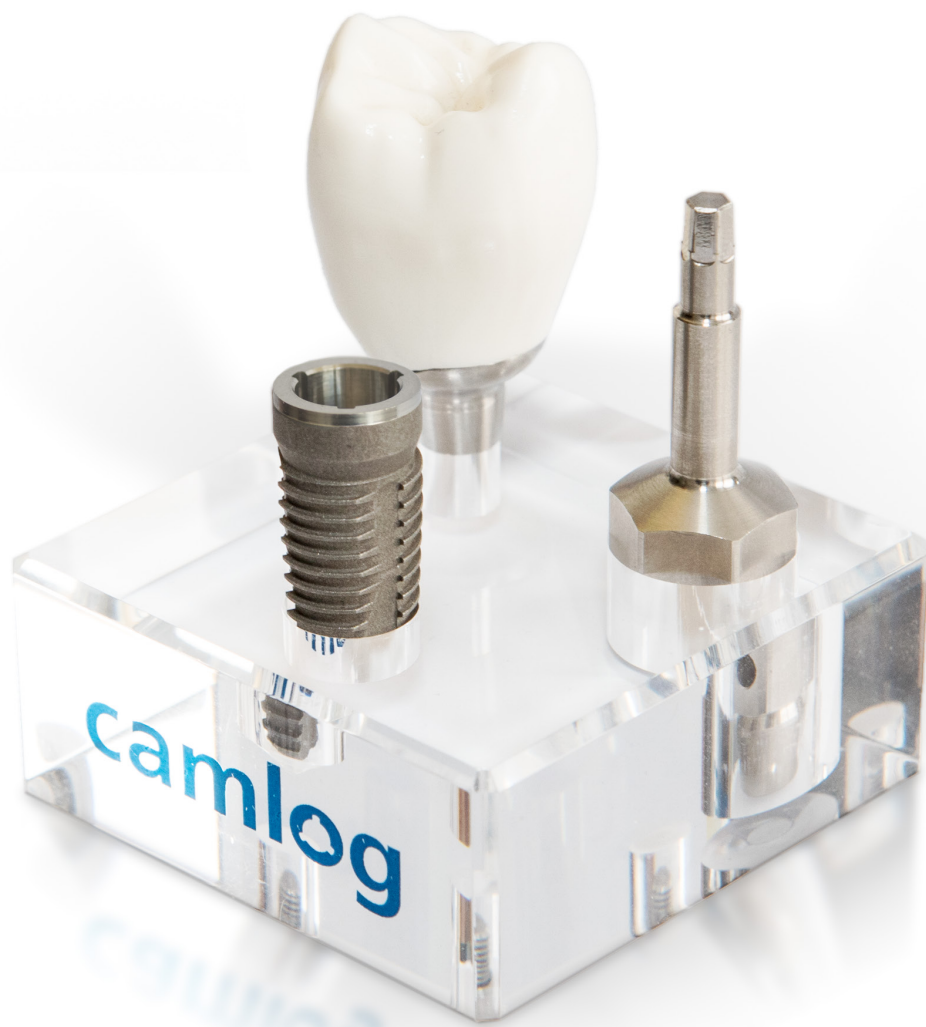

IMPLANTS FOR PRACTICE

	Article	Art.-No.	Ø	L
	CAMLOG® SCREW-LINE Implant for practice incl. insertion post and cover screw, yellow anodized Material Titanium alloy	K1049.3813	3.8 mm	13 mm
	CAMLOG® SCREW-LINE Implant for practice incl. insertion post and cover screw, red anodized Material Titanium alloy	K1049.4313	4.3 mm	13 mm
	CAMLOG® ROOT-LINE 2 Implant for practice incl. insertion post and cover screw, yellow anodized Material Titanium alloy	K1039.3813	3.8 mm	13 mm
	CAMLOG® ROOT-LINE 2 Implant for practice incl. insertion post and cover screw, red anodized Material Titanium alloy	K1039.4313	4.3 mm	13 mm

DEMONSTRATION MODELS

	Article	Art.-No.	Ø	L
	CAMLOG® Demonstration model, acrylic glass upper jaw, 4 CAMLOG® SCREW-LINE Implants, 4 x Ø 4.3 mm Material Acrylic glass/Titanium	K8070.1020	-	-
	CAMLOG® Demonstration model, acrylic glass lower jaw, 4 CAMLOG® SCREW-LINE Implants, 4 x Ø 4.3 mm Material Acrylic glass/Titanium	K8050.1040	-	-
	Edentulous mandible incl. mounting plate Material Plastic	J8070.2050	-	-

Attention, do not use implants for practice on patients!

MACRO MODELS





















	Article	Art.-No.
	<p>CAMLOG® SCREW-LINE Macro model Scale 3:1</p> <p>Content: 1 CAMLOG® SCREW-LINE Implant 1 CAMLOG® Esthomic® Abutment, straight 1 CAMLOG® Abutment screw, hex 1 Screwdriver, hex 1 Premolar, suitable for CAMLOG® Esthomic® Abutment, straight 1 Acrylic socket</p> <p>Material Plastic/Stainless steel</p>	K8010.1010
	<p>CAMLOG® ROOT-LINE 2 Macro model Scale 3:1</p> <p>Content: 1 CAMLOG® ROOT-LINE 2 Implant 1 CAMLOG® Esthomic® Abutment, straight 1 CAMLOG® Abutment screw, hex 1 Screwdriver, hex 1 Premolar, suitable for CAMLOG® Esthomic® Abutment, straight 1 Acrylic socket</p> <p>Material Plastic/Stainless steel</p>	K8010.1011











LITERATURE

	Article	Art.-No.
	Patient brochure Questions and answers to dental implants	-
	Implant pass Patient-specific documentation of implant restoration Packaging units: 10 units	-
	Patient advice sheets Set á 4 sheets, A4	-
	Presentation folder A4, laminated	-
	Poster Format: 50 x 70 cm	-

	Article	Art.-No.
	Appointment pad 50 sheets/pad, A7 Packaging units: 5 units	-
	Implant prosthetics DVD compendium Four teams – their concepts and solutions, Volume 1–4 A. Kirsch, K. L. Ackermann, G. Neuendorff, A. Happe, A. Nolte, S. Wolfart, V. Weber, F. Beuer, M. Stimmelmayer, J. Schweiger 2012 Quintessence Publishing Co, Ltd	B2012.0100





INDICATION OVERVIEW


Single tooth restoration		Bridge restoration
Cemented	Screwed	Cemented
 <p>Temporary abutments, PEEK, incl. PS</p>	 <p>Temporary abutments, PEEK, incl. PS</p>	 <p>Temporary abutments, PEEK, incl. PS</p>
	 <p>Temporary abutment, crown, titanium alloy</p>	
 <p>Esthomic® Abutments, incl. PS</p>		 <p>Esthomic® Abutments, incl. PS</p>
	 <p>Bar abutments</p>	
 <p>Titanium bases CAD/CAM, crown</p>	 <p>Titanium bases CAD/CAM, crown</p>	 <p>Titanium bases CAD/CAM, bridge</p>
 <p>Logfit® Abutment</p>		 <p>Logfit® Abutment</p>
 <p>Universal abutment, incl. PS</p>		 <p>Universal abutment, incl. PS</p>
 <p>Gold-plastic abutment</p>	 <p>Gold-plastic abutment</p>	 <p>Gold-plastic abutment</p>
 <p>Ceramic abutment</p>	 <p>Ceramic abutment</p>	 <p>Ceramic abutment</p>

Bridge restoration	Hybrid restoration
Screwed	Removable (full denture)
 <p>Temporary abutment, bridge, titanium alloy</p>	
 <p>Bar abutments</p>	 <p>Bar abutments</p>
 <p>Titanium bases CAD/CAM, bridge</p>	
	 <p>Locator® Anchoring system</p>
	 <p>Ball abutment</p>
Double crown restoration	 <p>Universal abutment, incl. PS</p>
	 <p>Telescope abutment</p>
	 <p>Gold-plastic abutment</p>
	 <p>Titanium bases CAD/CAM, crown</p>







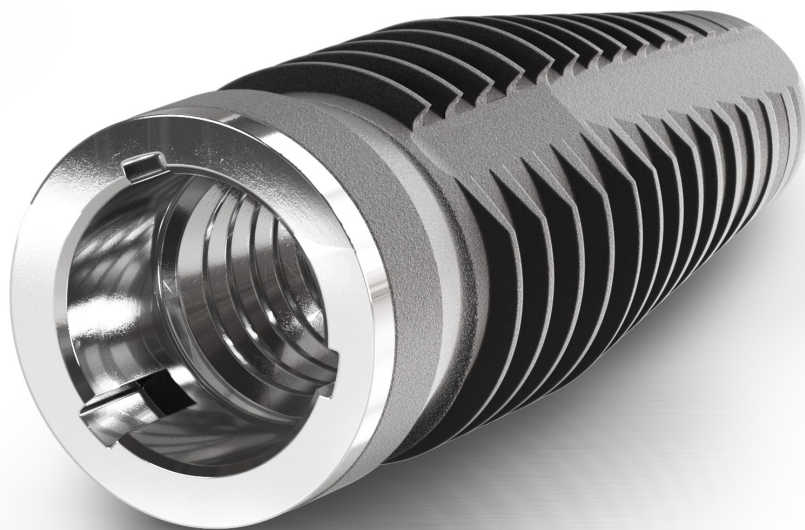


IMPLANT OVERVIEW

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm	L
		A Ø 2.7 mm	A Ø 3.5 mm	A Ø 3.9 mm	A Ø 4.6 mm	A Ø 5.5 mm	
Article		Art.-No.					
	CAMLOG® SCREW-LINE Implant, Promote®	-	K1044.3809	K1044.4309	K1044.5009	K1044.6009	9 mm
		K1044.3311	K1044.3811	K1044.4311	K1044.5011	K1044.6011	11 mm
		K1044.3313	K1044.3813	K1044.4313	K1044.5013	K1044.6013	13 mm
		K1044.3316	K1044.3816	K1044.4316	K1044.5016	K1044.6016	16 mm
	CAMLOG® SCREW-LINE Implant, Promote® plus	-	K1054.3809	K1054.4309	K1054.5009	K1054.6009	9 mm
		K1054.3311	K1054.3811	K1054.4311	K1054.5011	K1054.6011	11 mm
		K1054.3313	K1054.3813	K1054.4313	K1054.5013	K1054.6013	13 mm
		K1054.3316	K1054.3816	K1054.4316	K1054.5016	K1054.6016	16 mm
	CAMLOG® ROOT-LINE 2 Implant, Promote® plus	-	K1032.3809	K1032.4309	K1032.5009	K1032.6009	9 mm
		K1032.3311	K1032.3811	K1032.4311	K1032.5011	K1032.6011	11 mm
		K1032.3313	K1032.3813	K1032.4313	K1032.5013	K1032.6013	13 mm
		K1032.3316	K1032.3816	K1032.4316	K1032.5016	K1032.6016	16 mm
	Guide System CAMLOG® SCREW- LINE Implant, Promote® plus	-	K1053.3809	K1053.4309			9 mm
		K1053.3311	K1053.3811	K1053.4311			11 mm
		K1053.3313	K1053.3813	K1053.4313			13 mm
		K1053.3316	K1053.3816	K1053.4316			16 mm




PROSTHETICS OVERVIEW


Impression taking

	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm	
Article	Art.-No.					GH
 CAMLOG® Impression posts, open tray	K2121.3300	K2121.3800	K2121.4300	K2121.5000	K2121.6000	-
 CAMLOG® Impression posts, closed tray	K2110.3300	K2110.3800	K2110.4300	K2110.5000	K2110.6000	-
  CAMLOG® Impression posts PS, open tray, for Platform Switching with CAMLOG® Implants with K article number	-	K2119.3800	K2119.4300	K2119.5000	K2119.6000	-
  CAMLOG® Impression posts PS, closed tray, for Platform Switching with CAMLOG® Implants with K article number	-	K2109.3800	K2109.4300	K2109.5000	K2109.6000	-
 Impression caps for impression post, closed tray	J2111.3300	J2111.3800	J2111.4300	J2111.5000	J2111.6000	-










Bite registration

 CAMLOG® Bite registration posts incl. fixing screw and bite registration cap	J2140.3300	J2140.3800	J2140.4300	J2140.5000	J2140.6000	-
---	------------	------------	------------	------------	------------	---

Fabrication of the plaster model














		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm	
Article		Art.-No.					GH
 CAMLOG® Lab analogs		K3010.3300	K3010.3800	K3010.4300	K3010.5000	K3010.6000	-







Abutments for crown and bridge restorations

	CAMLOG® Temporary abutments, PEEK	-	K2241.3800	K2241.4300	K2241.5000	K2241.6000	-
	CAMLOG® Temporary abutments PS, PEEK, for Platform Switching with CAMLOG® Implants with K article number	-	K2208.3800	K2208.4300	K2208.5000	K2208.6000	-
	CAMLOG® Temporary abutment, crown, titanium alloy	K2239.3300	K2239.3800	K2239.4300	K2239.5000	K2239.6000	-
	CAMLOG® Temporary abutment, bridge, titanium alloy	J2339.3300	J2339.3800	J2339.4300	J2339.5000	J2339.6000	-
	CAMLOG® Esthomic® Abutments, straight	-	K2226.3810	K2226.4310	K2226.5010	K2226.6010	1.0-1.8 mm
			K2226.3830	K2226.4330	K2226.5030	K2226.6030	3.0-4.5 mm
	CAMLOG® Esthomic® Abutments, 15° angled, type A	-	K2227.3810	K2227.4310	K2227.5010	K2227.6010	1.0-1.8 mm
			K2227.3830	K2227.4330	K2227.5030	K2227.6030	3.0-4.5 mm
	CAMLOG® Esthomic® Abutments, 15° angled, type B	-	K2228.3810	K2228.4310	K2228.5010	K2228.6010	1.0-1.8 mm
			K2228.3830	K2228.4330	K2228.5030	K2228.6030	3.0-4.5 mm
	CAMLOG® Esthomic® Abutments, 20° angled, type A	-	K2231.3810	K2231.4310	K2231.5010	K2231.6010	1.0-1.8 mm
			K2231.3830	K2231.4330	K2231.5030	K2231.6030	3.0-4.5 mm
	CAMLOG® Esthomic® Abutments, 20° angled, type B	-	K2232.3810	K2232.4310	K2232.5010	K2232.6010	1.0-1.8 mm
			K2232.3830	K2232.4330	K2232.5030	K2232.6030	3.0-4.5 mm









PROSTHETICS OVERVIEW

Abutments for crown and bridge restorations

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm	
Article		Art.-No.					GH
 	CAMLOG® Esthomic® Abutments PS, straight, for Platform Switching with CAMLOG® Implants with K article number	-	K2202.3815	K2202.4315	K2202.5015	K2202.6015	1.5 – 2.5 mm
 	CAMLOG® Esthomic® Abutments PS, 15° angled, type A, for Platform Switching with CAMLOG® Implants with K article number	-	K2203.3815	K2203.4315	K2203.5015	K2203.6015	1.5 – 2.5 mm
 	CAMLOG® Esthomic® Abutments PS, 15° angled, type B, for Platform Switching with CAMLOG® Implants with K article number	-	K2204.3815	K2204.4315	K2204.5015	K2204.6015	1.5 – 2.5 mm
	CAMLOG® Esthomic® Abutments, Inset	K2235.3315	K2235.3815	K2235.4315	K2235.5015	K2235.6015	1.5 – 2.5 mm
	CAMLOG® Universal abutment	K2211.3300	K2211.3800	K2211.4300	K2211.5000	K2211.6000	-
 	CAMLOG® Universal abutments PS for Platform Switching with CAMLOG® Implants with K article number	-	K2201.3800	K2201.4300	K2201.5000	K2201.6000	-
	CAMLOG® Gold-plastic abutment	K2246.3300	K2246.3800	K2246.4300	K2246.5000	K2246.6000	-
	CAMLOG® Titanium bases CAD/CAM, crown	K2244.3348	K2244.3848	K2244.4348	K2244.5048	K2244.6048	-
	CAMLOG® Titanium bases CAD/CAM, bridge	J2344.3348	J2344.3848	J2344.4348	J2344.5048	J2344.6048	-




		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm	
Article		Art.-No.					GH
 CAMLOG® Ceramic abutments		K2242.3340	K2242.3840	K2242.4340	K2242.5040	K2242.6040	-
 CAMLOG® Logfit® Abutments		-	K2550.3808	K2550.4308	K2550.5008	K2550.6008	0.8 mm
		-	K2550.3815	K2550.4315	K2550.5015	K2550.6015	1.5 mm
 Logfit® Impression caps		-	J2551.4300	J2551.4300	J2551.6000	J2551.6000	-
 Logfit® Analog		-	J2552.4300	J2552.4300	J2552.6000	J2552.6000	-
 Logfit® Plastic copings, for crowns		-	J2553.4302	J2553.4302	J2553.6002	J2553.6002	-
 Logfit® Plastic copings, for bridges		-	J2553.4301	J2553.4301	J2553.6001	J2553.6001	-

COMFOUR™ – Abutments for crown, bridge and hybrid restorations



 CAMLOG® Bar abutment, straight	J2254.3305	J2254.3805	J2254.4305	J2254.5005	-	0.5 mm
	J2254.3320	J2254.3820	J2254.4320	J2254.5020		2.0 mm
	-	J2254.3840	J2254.4340	J2254.5040		4.0 mm
 CAMLOG® Bar abutment, 17° angled, type A	K2256.3325	K2256.3825	K2256.4325	K2256.5025	-	2.5 mm
	K2256.3340	K2256.3840	K2256.4340	K2256.5040		4.0 mm
 CAMLOG® Bar abutment, 17° angled, type B	K2257.3325	K2257.3825	K2257.4325	K2257.5025	-	2.5 mm
	K2257.3340	K2257.3840	K2257.4340	K2257.5040		4.0 mm
 CAMLOG® Bar abutment, 30° angled, Type A	K2258.3325	K2258.3825	K2258.4325	K2258.5035*	-	2.5/3.5* mm
	K2258.3340	K2258.3840	K2258.4340	K2258.5050*		4.0/5.0* mm
 CAMLOG® Bar abutment, 30° angled, Type B	K2259.3325	K2259.3825	K2259.4325	K2259.5035*	-	2.5/3.5* mm
	K2259.3340	K2259.3840	K2259.4340	K2259.5050*		4.0/5.0* mm
 Healing cap for bar abutment	J2029.4300	J2029.4300	J2029.4300	J2029.6000	-	-
 Impression cap for bar abutment, closed tray	J2129.4300	J2129.4300	J2129.4300	J2129.6000	-	-
 Scanning cap for bar abutments	J2610.4300	J2610.4300	J2610.4300	J2610.6000	-	-










PROSTHETICS OVERVIEW

COMFOUR™ – Abutments for crown, bridge and hybrid restorations



		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm	
Article		Art.-No.					GH
 Aligning tool 17°		J2269.0003	J2269.0003	J2269.0003	J2269.0003	-	-
 Aligning tool 30°		J2269.0004	J2269.0004	J2269.0004	J2269.0004	-	-
 Titanium cap for bar abutment, for crown		J2259.4301	J2259.4301	J2259.4301	J2259.6001	-	-
 Titanium cap for bar abutment, for bridge		J2259.4302	J2259.4302	J2259.4302	J2259.6002	-	-
 Crown base for bar abutment, burn-out		J2256.4306	J2256.4306	J2256.4306	J2256.6006	-	-
 Bases for bar abutment, burn-out		J2257.4301	J2257.4301	J2257.4301	J2257.6001	-	-
 Bases for bar abutment, cast-on		J2263.4300	J2263.4300	J2263.4300	J2263.6000	-	-
 Bases for bar abutment, solderable		J2258.4300	J2258.4300	J2258.4300	J2258.6000	-	-
 Bases for bar abutment, titanium, laser-weldable		J2262.4300	J2262.4300	J2262.4300	J2262.6000	-	-
 Titanium bonding bases for bar abutment, Passive-Fit		J2260.4301	J2260.4301	J2260.4301	J2260.6001	-	-
 Sleeves for titanium bonding base, burn-out, Passive-Fit		J2261.4301	J2261.4301	J2261.4301	J2261.6001	-	-
 Locator® Fixture for bar abutment		J2253.4301	J2253.4301	J2253.4301	J2253.6001	-	-

Hybrid restoration

	J2250.3315	J2250.3815	J2250.4315	J2250.5015	-	1.5 mm
	J2250.3330	J2250.3330	J2250.4330	J2250.5030		3.0 mm
	-	J2250.3845	J2250.4345	J2250.5045		4.5 mm
	J2249.3315	J2249.3815	J2249.4315	J2249.5015	-	1.5 mm
	J2249.3330	J2249.3830	J2249.4330	J2249.5030		3.0 mm
	-	J2249.3845	J2249.4345	J2249.5045		4.5 mm

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm	
Article		Art.-No.					GH
	Ball abutment analogs	J3015.3300	J3015.3800	J3015.4300	J3015.5000	-	-
	CAMLOG® Locator® Abutments	J2253.3310	J2253.3810	J2253.4310	J2253.5010	-	1.0 mm
		J2253.3320	J2253.3820	J2253.4320	J2253.5020	-	2.0 mm
		J2253.3330	J2253.3830	J2253.4330	J2253.5030	-	3.0 mm
		J2253.3340	J2253.3840	J2253.4340	J2253.5040	-	4.0 mm
		-	J2253.3850	J2253.4350	J2253.5050	-	5.0 mm
	Locator® Impression cap	J2253.0200	J2253.0200	J2253.0200	J2253.0200	-	-
	Locator® Analog	J2253.0340	J2253.0340	J2253.0340	J2253.0350	-	-
	Locator® Male processing package	J2253.0102	J2253.0102	J2253.0102	J2253.0102	-	-
	Locator® Male processing package for extended range	-	J2253.0112	J2253.0112	J2253.0112	-	-
	CAMLOG® Universal abutments	-	K2211.3800	K2211.4300	K2211.5000	K2211.6000	-
	CAMLOG® Universal abutments PS for Platform Switching with CAMLOG® Implants with K article number	-	K2201.3800	K2201.4300	K2201.5000	K2201.6000	-
	CAMLOG® Telescope abutments for double crown restorations	-	K2212.3800	K2212.4300	K2212.5000	K2212.6000	-

CAD/CAM Prosthetic
















	CAMLOG® Scanbodies	K2610.3310	K2610.3810	K2610.4310	K2610.6010	K2610.6010	-
	CAMLOG® ScanPost for Sirona Scanbody	K2620.3306	K2620.3806	K2620.4306	K2620.5006	K2620.6006	-

DEDICAM® CAD/CAM PROSTHETICS FROM CAMLOG

Find out more about DEDICAM® products at www.dedicam.com.

SCREW OVERVIEW – ABUTMENT AND PROSTHETIC SCREWS – INTRAORAL USE

Implant-Abutment connection






		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm	
		M 1.6			M 2.0		
Article		CAMLOG® Abutment screw					Tightening torque
	Temporary Abutments PEEK, incl. PS Scanbody ScanPost for Sirona Scanbody	 J4005.1601			 J4005.2001		tightened by hand**
	Temporary Abutments titanium, crown and bridge						
	Esthomic® Abutments, incl. PS						
	Universal Abutment, incl. PS Telescope Abutment Gold-plastic Abutment Logfit® Abutment						
	Ceramic Abutment						
	Titanium bases CAD/CAM, crown and bridge						
	Vario SR Abutments, 20° and 30° angled						
		CAMLOG® Vario SR Abutment screws					
	Vario SR Abutment, straight	 J4007.1600			 J4007.2000		20 Ncm*
		CAMLOG® Abutment screws with reduced head, light blue anodized					
	COMFOUR™ Bar Abutments, 17° and 30° angled	 J4004.1601			 J4004.2001		20 Ncm*

* with torque wrench J5320.1030

** Optional for temporary abutments titanium: Torque after completed healing phase 20 Ncm.













All screws must be retightened with the corresponding torque after at least 5 minutes!

Abutment-Prosthetic connection

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm	
		M 1.6			M 2.0		
Article		Prosthetic screws for bar abutments, light blue anodized					Tightening torque
 COMFOUR™ Bar Abutments, 17° and 30° angled		3.6 mm  J4012.1601			3.8 mm  J4012.2001		15 Ncm*
		Vario SR Prosthetic screw, yellow anodized					
 Vario SR Abutments, straight, 20° and 30° angled		4 mm  J4005.2004					15 Ncm*

AUXILIARY SCREWS INTRA- AND EXTRAORAL USE

Abutment-Prosthetic connection

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm	
		M 1.6			M 2.0		
Article		Prosthetic screws for bar abutments, light blue anodized					Tightening torque
	Scanning cap for bar abutments	3.6 mm  J4012.1601			3.8 mm  J4012.2001		tightened by hand
		Screws for bar abutments, for impression taking open tray and for soldering, light blue anodized					
	COMFOUR™ Bar abutments, straight, 17° and 30° angled	12 mm  J4012.1610			12.2 mm  J4012.2010		tightened by hand
		17 mm  J4012.1615			17.2 mm  J4012.2015		
		22 mm  J4012.1620			22.2 mm  J4012.2020		
		Plastic screws for bar abutment, as fixation and bonding aid, beige					
		29 mm  J4009.1627			29.2 mm  J4009.2027		tightened by hand

* with torque wrench J5320.1030

All screws must be retightened with the corresponding torque after at least 5 minutes!

SCREW OVERVIEW – LAB SCEWS

EXTRAORAL USE












Lab analog-Abutment connection

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm	
		M 1.6			M 2.0		
Article	CAMLOG® Lab screws*, brown anodized						Tightening torque
 Temporary Abutments PEEK, incl. PS Scanbody ScanPost for Sirona Scanbody	 10.5 mm J4006.1601			 10.5 mm J4006.2001		tightened by hand	
 Temporary Abutments titanium, crown and bridge							
 Esthomic® Abutments, incl. PS							
 Universal Abutment, incl. PS Telescope Abutment Gold-plastic Abutment							
 Ceramic Abutment							
 Titanium bases CAD/CAM, crown and bridge							
 Vario SR Abutments, 20° and 30° angled							
CAMLOG® Bonding aids**							
 Titanium bases CAD/CAM, crown and bridge	 27.5 mm			 27.5 mm		tightened by hand	
CAMLOG® Vario SR Lab screws*, brown anodized							
 Vario SR Abutment, straight	 11.9 mm J4008.1600			 11.9 mm J4008.2000		tightened by hand	
CAMLOG® Lab screws with reduced head*, light blue partially anodized							
 COMFOUR™ Bar Abutments, 17° and 30° angled	 9.5 mm J4004.1600			 9.5 mm J4004.2000		tightened by hand	

* Lab screws may not be used on patients.















**not available singly, are included in the packaging of the titanium base CAD/CAM.

Abutment-Prosthetic connection

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm		
		M 1.6			M 2.0			
Article	Lab prosthetic screws for bar abutments*, brown anodized						Tightening torque	
	Scanning cap for bar abutments	<div>3.6 mm</div> <div></div> <div>J4013.1601</div>			<div>3.8 mm</div> <div></div> <div>J4013.2001</div>		tightened by hand	
	COMFOUR™ Bar abutment, 17° and 30° angled							
	Bar lab analog for bar abutments							
		Vario SR Prosthetic screw, yellow anodized						
	Vario SR Abutments, straight, 20° and 30° angled	<div>4 mm</div> <div></div> <div>J4005.2004</div>					tightened by hand	
	Vario SR Analog							
		Prosthetic screw for bar abutments*, for fabrication of the wax up on the bar sleeve for titanium bonding base, Passive-Fit, on the bar lab analog						
	Titanium bonding base for bar abutments and bar sleeve for titanium bonding base, burn-out, Passive-Fit	<div>5.5 mm</div> <div></div> <div>J4005.1602</div>			<div>5.5 mm</div> <div></div> <div>J4005.2002</div>		tightened by hand	

* Lab screws may not be used on patients.



























OVERVIEW – TIGHTENING TORQUE

Article	Instrument	Tightening torque
 <p>CAMLOG® Implant cover screw</p>		
 <p>CAMLOG® Healing caps (incl. PS) cylindrical, wide body, bottleneck</p>		
 <p>CAMLOG® Impression posts (incl. PS)</p> <p>CAMLOG® Bite registration post</p>		tightened by hand**
 <p>CAMLOG® Lab screws</p> <p>CAMLOG® Labscrews with reduced head</p>		
 <p>CAMLOG® Temporary Abutments PEEK, incl. PS</p> <p>CAMLOG® Temporary Abutments titanium, crown and bridge</p>		
 <p>CAMLOG® Abutment screws</p> <p>CAMLOG® Abutment screws with reduced head</p>	     <p>J5317.0510 J5317.0501 J5317.0502 J5317.0504 J5317.0503</p>	
 <p>CAMLOG® Esthomic® Abutment, straight (incl. PS)</p> <p>CAMLOG® Esthomic® Abutment, angled 15°/20° (incl. PS)</p> <p>CAMLOG® Esthomic® Abutment, Inset</p>		
 <p>CAMLOG® Gold-plastic abutment</p> <p>CAMLOG® Universal abutment</p> <p>CAMLOG® Telescope abutment</p> <p>CAMLOG® Ceramic abutment</p>		20 Ncm*
 <p>CAMLOG® Logfit® Abutments</p> <p>CAMLOG® Titanium bases CAD/CAM, crown and bridge</p>		

* with torque wrench J5320.1030

** Optional for temporary abutments titanium: Torque after completed healing phase 20 Ncm.

All screws must be retightened with the corresponding torque after at least 5 minutes!

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	3.3	3.8	4.3	5.0	6.0
Article	Instrument					Tightening torque				
 CAMLOG® Bar abutment, straight	 J5300.0020	 J5300.0025				20 Ncm*	30 Ncm*			
 CAMLOG® Bar abutment, 17° and 30° angled	 J5317.0510  J5317.0501  J5317.0502  J5317.0504  J5317.0503					20 Ncm*				
 Scanning cap for bar abutments						tightened by hand				
 Titanium cap for bar abutment, for crown/bridge						15 Ncm*				
 Crown base for bar abutment, burn-out										
 Bases for bar abutments, burn-out, cast-on, solderable, laser-weldable										
 Titanium bonding bases for bar abutment, Passive-Fit	 J5300.0027  J5300.0028					tightened by hand				
 Healing cap for bar abutment										
 Impression cap for bar abutment, closed tray (bridge/bar)										
 CAMLOG® Ball abutments	 J5300.0011					20 Ncm*	30 Ncm*			
 CAMLOG® Locator® Abutments	 J2253.0001					20 Ncm*	30 Ncm*			
 CAMLOG® Scanbodies	 J5317.0501  J5317.0502					tightened by hand				
 CAMLOG® ScanPosts for Sirona Scanbody										

* with torque wrench J5320.1030

All screws must be retightened with the corresponding torque after at least 5 minutes!

MATERIALS

Titanium Grade 4			
Properties (ASTM F67)			
Chemical structure (in %)	O	≤	0.4
	Fe	≤	0.5
	C	≤	0.08
	N	≤	0.05
	H	≤	0.015
	Ti		Rest
Mechanical properties	Tensile strength	≥	550 MPa
	Elongation at break	≥	12 %

Titanium alloy Ti6Al4V ELI			
Properties (ASTM F136)			
Chemical structure (in %)	Al		5.5 – 6.5
	V		3.5 – 4.5
	Fe	≤	0.25
	C	≤	0.08
	N	≤	0.05
	O	≤	0.13
	H	≤	0.012
	Ti		Rest
Mechanical properties	Tensile strength	≥	860 MPa
	Elongation at break	≥	10 %

Cast-on gold alloy CAMLOG® Gold-plastic abutment			
Properties			
Chemical structure (in %)	Au		60
	Pd		20
	Pt		19
	Ir		1
Physical properties	Melting range		1400 – 1490 °C
	Density		17.5 g/cm³
	E-Modul		136 GPa
	Coefficient of thermal expansion (25-500°C)		11.9 µm/m· °C
	Coefficient of thermal expansion (25-600°C)		12.2 µm/m· °C
	Color		white
Mechanical properties			drawn
	Hardness HV5	>	215
	Tensile strength (Rm)	>	750 MPa
	0.2% Elongation limit (Rp 0.2%)	>	650 MPa
	Elongation at break	>	2 %

Cast-on gold alloy Base for bar abutment			
Properties			
Chemical structure (in %)	Au		60
	Pt		19
	Pd		20
	Ir		1
Physical properties	Density		17.5 g/cm³
	Color		white
	Liquidus		1490 °C
	Solidus		1400 °C
	Coefficient of thermal expansion (25-500°C)		12.5 µm/m· °C
	Coefficient of thermal expansion (25-600°C)		12.6 µm/m· °C
	E-Modul		136 GPa
Mechanical properties			hardened 700 °C/30 min.
	Hardness HV5		210
	0.2 % Elongation limit		450 – 570 MPa
	Elongation at break		min. 10 %
	Tensile strength MPa		530 – 650

Solderable gold alloy Base for bar abutment		
Properties		
Chemical structure (in %)	Au	70.00
	Pt	8.50
	Ag	13.40
	Pd	-
	Cu	7.50
	Zn	0.50
	Ir	0.10
	Rh	-
	Ru	-
Physical properties	Color	yellow
	Melting range	895 – 1010 °C
Mechanical properties	Hardness	
	annealed HV5	170
	hardened HV5	295
	self hardened HV5	280

Zirconium oxide		
Properties		
Chemical structure (in %)	ZrO ₂ + HfO ₂ + Y ₂ O ₃	> 99.0
	Y ₂ O ₃	4.5 – 5.4
	HfO ₂	< 5
	Al ₂ O ₃	< 0.5
	other oxides	< 0.5
Physical properties	Density	> 6.0 g/cm ³
	Porosity, open	0,00 %
	Microstructure	
Mechanical properties	Mean Linear intercept size	< 0.6 µm
	3 pt. transversal strength	≥ 800 MPa

INDEX – ALPHABETICAL

A

Abutment collets	74
Abutment screw, hex	59, 69
Abutment screw, with reduced head, hex	63
Adapter for screw implants, long	37
Adapter ISO shaft for angled hand piece	36
Aligning tool 17°	61
Aligning tool 30°	61
ALTApin applicator, angled 90°	43
ALTApin applicator, straight	43
ALTApin applicator, straight, work element	44
ALTApin magazine	45
ALTApin membrane fixator	44
ALTApin pricker	44
ALTApin pricker, insert	45
ALTApin set	43
ALTApin single patient drill, ISO shaft	45
ALTApin surgery mallet	45
ALTApin Tray	43
Appointment pad	81

B

Ball abutment analogs	65
Ball abutment sets, incl. male part and matrix CM Dalbo®-Plus	64
Ball abutments, male part	64
Bar abutment, 17° angled, type A and B	60
Bar abutment, 30° angled, type A and B	60
Bar abutment, straight	60
Bar lab analog for bar abutments	61

B

Bar sleeves for titanium bonding base	62
Base for bar abutment, burn-out	62
Base for bar abutment, cast-on	62
Base for bar abutment, solderable	62
Base for bar abutment, titanium	62
Bite registration caps	51
Bite registration posts	51
Bone profiler Ø 5.0 mm	33
Bone profiler Ø 6.0 mm	33
Bone profiler Ø 7.0 mm	33

C

CAM Titanium Blank, type IAC	58
CAM Titanium Blank, type ME	58
Cardanic driver (30°)	36
Ceramic abutments, 2-parts, for bonded/cemented full ceramic crowns	54
Cleaning cannula	38
Cleaning needle	38
Collet for CAM Blank, type IAC	58
Collets for zirconium oxide sleeve	74
Crown base for bar abutment	62
CT-tube	15

D

Demonstration model, acrylic glass	78
Depth stop for form drill SCREW-LINE und ROOT-LINE 2	21, 31
Depth stop SCREW-LINE	33
Drill extension ISO shaft, for drills with internal irrigation	25

D

Drill extension not for drills with internal irrigation	34
Drill for CT-tube	15
Driver for impression cap and healing cap for bar abutment	71
Driver for impression caps and healing caps for bar abutments	61
Driver for Locator®, manual/wrench	71
Driver for straight bar abutment, short	70, 71
Driver, extra short, for screw implants, manual/wrench	35
Driver, for ball abutment, manual/wrench	70
Driver, for screw implants, with ISO shaft for angled hand piece	34
Driver, long, for screw implants, manual/wrench	35
Driver, long, for screw implants, manual/wrench	35
Driver, long, for screw implants, with ISO-shaft for angled hand piece	35
Driver, short, for screw implants, manual/wrench	35
Driver, short, for screw implants, manual/wrench, with borehole for screwdriver, hex, long	35
Driver, short, for screw implants, with ISO-shaft for angled hand piece	35

E

Edentulous mandible	78
Esthomic® Abutments PS, 15° angled, type A, for Platform Switching	53
Esthomic® Abutments PS, 15° angled, type B, for Platform Switching	53
Esthomic® Abutments PS, straight, for Platform Switching	53
Esthomic® Abutments, 15° angled, type A	52
Esthomic® Abutments, 15° angled, type B	53

E

Esthomic® Abutments, 20° angled, type A	53
Esthomic® Abutments, 20° angled, type B	53
Esthomic® Abutments, Inset	53
Esthomic® Abutments, straight	52

F

Form drill ROOT-LINE 2	31
Form drill SCREW-LINE	21
Form drill SCREW-LINE Cortical bone	21

G

Gold-plastic abutment	54
Guide System CAMLOG® Insertion post	24
Guide System CAMLOG® SCREW-LINE Implant, Promote® plus	22
Guide System Check-up pin	25
Guide System Driver manual/wrench	25
Guide System Driver with ISO shaft	25
Guide System Form drill, SCREW-LINE, Cortical Bone	23
Guide System Gingiva punch	23
Guide System Guiding sleeve	23
Guide System Pilot drill set	22
Guide System Seating tool	24
Guide System Surgery set, SCREW-LINE	23
Guide System Template drill	24
Guiding pin for bone profiler	33

H

Healing cap for bar abutment	61
Healing cap PS, bottleneck	47

INDEX – ALPHABETICAL

H

Healing cap PS, cylindrical	47
Healing cap PS, wide body	47
Healing cap, bottleneck	46
Healing cap, cylindrical	46
Healing cap, wide body	46
Holding key for insertion post	36
Holding sleeve for screw implants	37

I

Implant pass	80
Implant prosthetics	81
Impression cap for bar abutment, closed tray (bridge/bar)	61
Impression caps for impression post, closed tray	50
Impression posts PS, closed tray, for Platform Switching	50
Impression posts PS, open tray, for Platform Switching	50
Impression posts, closed tray	50
Impression posts, open tray	50

L

Lab analogs	51
Lab prosthetic screw for bar abutment	63
Lab screw, hex	59, 69
Lab screw, with reduced head, hex	63
Lamella retention insert	65
Locator® Abutments	65
Locator® Analog	65
Locator® Angle measurement guide	71
Locator® Block out spacer	66

L

Locator® Fixture for bar abutment	62
Locator® Impression cap	65
Locator® Instrument	71
Locator® Male processing package	66
Locator® Male processing package for extended range	66
Locator® Parallel post	71
Locator® Processing replacement male	66
Locator® Replacement male	66, 67
Locator® Replacement male for extended range	67
Logfit® Abutments	55
Logfit® Analog	55
Logfit® Impression caps	55
Logfit® Plastic copings, for bridges (without rotation securing device)	56
Logfit® Plastic copings, for crowns (with rotation securing device)	56

M

Manual screwdriver, hex	38
Manual screwdriver, hex	73
Matrix CM Dalbo®-Plus	64
Modeling aids for CAMLOG® Titanium bases CAD/CAM	57

O

Osteotome SCREW-LINE	39, 40, 41, 44
Osteotomy set CAMLOG®/CONELOG® SCREW-LINE	39, 40, 41, 42

P

Paralleling pin SCREW-LINE	34
Patient advice sheets	80
Patient brochure	80
Pattern for surgery wash tray CAMLOG® ROOT-LINE 2	30
Pattern for surgery wash tray CAMLOG®/CONELOG® SCREW-LINE	20
PickUp instrument	36
Pilot drill	32
Pilot drill SCREW-LINE	32
Plastic screw for bar abutment	64
Poster	80
Pre-drill SCREW-LINE	32
Pre-Osteotome SCREW-LINE	39, 40, 41, 43
Presentation folder	80
Prosthetic screw for bar abutments	63
Prosthetic tray	72
Prosthetic tray universal	72

R

Reamers for dilating the plaster model, for universal holder	74
Reworking reamer, for base for bar abutment	74
Reworking reamer, for base for bar abutment	75
ROOT-LINE 2 Implant for practice	78
ROOT-LINE 2 Implant, Promote® plus	27
ROOT-LINE 2 Macro model	79
Round bur	32

S

Scanbodies	57
Scanning cap for bar abutments	61
ScanPosts for Sirona Scanbody	57
Screw, hex, length 10 mm	63
Screw, hex, length 15 mm	63
Screw, hex, length 20 mm	63
Screwdriver Activator	70
Screwdriver, hex, extra short, manual/wrench	37, 72
Screwdriver, hex, long, ISO shaft	38, 73
Screwdriver, hex, long, manual/wrench	37, 72
Screwdriver, hex, short, ISO shaft	38, 73
Screwdriver, hex, short, manual/wrench	37, 72
SCREW-LINE Implant for practice	78
SCREW-LINE Implant, Promote®	17
SCREW-LINE Implant, Promote® plus	17
SCREW-LINE Macro model	79
Selection abutment kit	75
Surgery set CAMLOG®/CONELOG® SCREW-LINE	20
Surgery set CAMLOG® ROOT-LINE 2	30
Surgery wash tray CAMLOG® ROOT-LINE 2	30
Surgery wash tray CAMLOG®/ CONELOG® SCREW-LINE	20

T

Tap adapter, long	34
Tap adapter, short	34
Tap ROOT-LINE 2	31
Tap SCREW-LINE	21

INDEX – ALPHABETICAL

T

Telescope abutments, for double crown restorations	68
Temporary abutment, bridge, titanium alloy	52
Temporary abutment, crown, titanium alloy	52
Temporary abutments PS, PEEK, for Platform Switching	52
Temporary abutments, PEEK	52
Titanium bases	55
Titanium bases CAD/CAM, bridge	56
Titanium bases CAD/CAM, crown	56
Titanium bonding base for bar abutment	62
Titanium cap for bar abutment, for bridge	62
Titanium cap for bar abutment, for crown	61
Torque wrench	70

U

Universal abutments	54
Universal abutments PS for Platform Switching	54
Universal abutments PS, for double crown restorations	68
Universal abutments, for double crown restorations	68
Universal holder	74

X

X-Ray Planning foil 1.25:1 CAMLOG® ROOT-LINE 2 Implants	14
X-Ray Planning foil 1.25:1 CAMLOG® SCREW-LINE Implants	14
X-Ray Planning foil 1.4:1 CAMLOG® ROOT-LINE 2 Implants	14
X-Ray Planning foil 1.4:1 CAMLOG® SCREW-LINE Implants	14

X

X-Ray Transfer pictures 1.25:1 CAMLOG® ROOT-LINE 2 Implants	14
X-Ray Transfer pictures 1.25:1 CAMLOG® SCREW-LINE Implants	14

Z

Zirkonium oxide sleeves	55
-------------------------	----

INDEX – ARTICLENUMBERS

A2002.2000	CT-tube	15		Impression caps for impression post, closed tray	
	Drill for CT-tube		J2111.3300	Ø 3.3 mm	50
A2050.2600	Ø 2.6 mm	15	J2111.3800	Ø 3.8 mm	50
A2050.2800	Ø 2.8 mm	15	J2111.4300	Ø 4.3 mm	50
			J2111.5000	Ø 5.0 mm	50
A2222.2200	CT-tube	15	J2111.6000	Ø 6.0 mm	50
B2012.0100	Implant prosthetics	81		Bite registration caps	
	Healing cap, bottleneck		J2112.3300	Ø 3.3 mm	51
J2011.3340	Ø 3.3 mm, GH 4.0 mm	46	J2112.3800	Ø 3.8 mm	51
J2011.3840	Ø 3.8 mm, GH 4.0 mm	46	J2112.4300	Ø 4.3 mm	51
J2011.3860	Ø 3.8 mm, GH 6.0 mm	46	J2112.5000	Ø 5.0 mm	51
J2011.4340	Ø 4.3 mm, GH 4.0 mm	46	J2112.6000	Ø 6.0 mm	51
J2011.4360	Ø 4.3 mm, GH 6.0 mm	46		Impression cap for bar abutment, closed tray (bridge/bar)	
J2011.5040	Ø 5.0 mm, GH 4.0 mm	46	J2129.4300	Ø 3.3/3.8/4.3 mm	61
J2011.5060	Ø 5.0 mm, GH 6.0 mm	46	J2129.6000	Ø 5.0/6.0 mm	61
J2011.6040	Ø 6.0 mm, GH 4.0 mm	46		Bite registration posts	
J2011.6060	Ø 6.0 mm, GH 6.0 mm	46	J2140.3300	Ø 3.3 mm	51
	Healing cap, wide body		J2140.3800	Ø 3.8 mm	51
J2014.3320	Ø 3.3 mm, GH 2.0 mm	46	J2140.4300	Ø 4.3 mm	51
J2014.3340	Ø 3.3 mm, GH 4.0 mm	46	J2140.5000	Ø 5.0 mm	51
J2014.3820	Ø 3.8 mm, GH 2.0 mm	46	J2140.6000	Ø 6.0 mm	51
J2014.3840	Ø 3.8 mm, GH 4.0 mm	46		Zirkonium oxide sleeves	
J2014.3860	Ø 3.8 mm, GH 6.0 mm	46	J2242.3341	Ø 3.3 mm	55
J2014.4320	Ø 4.3 mm, GH 2.0 mm	46	J2242.3841	Ø 3.8 mm	55
J2014.4340	Ø 4.3 mm, GH 4.0 mm	46	J2242.4341	Ø 4.3 mm	55
J2014.4360	Ø 4.3 mm, GH 6.0 mm	46	J2242.5041	Ø 5.0 mm	55
J2014.5020	Ø 5.0 mm, GH 2.0 mm	46	J2242.6041	Ø 6.0 mm	55
J2014.5040	Ø 5.0 mm, GH 4.0 mm	46		Modeling aids for CAMLOG®	
J2014.5060	Ø 5.0 mm, GH 6.0 mm	46		Titanium bases CAD/CAM	
J2014.6020	Ø 6.0 mm, GH 2.0 mm	46	J2244.3302	Ø 3.3 mm	57
J2014.6040	Ø 6.0 mm, GH 4.0 mm	46	J2244.3802	Ø 3.8 mm	57
J2014.6060	Ø 6.0 mm, GH 6.0 mm	46	J2244.4302	Ø 4.3 mm	57
	Healing cap, cylindrical		J2244.5002	Ø 5.0 mm	57
J2015.3320	Ø 3.3 mm, GH 2.0 mm	46	J2244.6002	Ø 6.0 mm	57
J2015.3340	Ø 3.3 mm, GH 4.0 mm	46		Ball abutment, male part	
J2015.3820	Ø 3.8 mm, GH 2.0 mm	46	J2249.3315	Ø 3.3 mm, GH 1.5 mm	64
J2015.3840	Ø 3.8 mm, GH 4.0 mm	46	J2249.3330	Ø 3.3 mm, GH 3.0 mm	64
J2015.3860	Ø 3.8 mm, GH 6.0 mm	46	J2249.3815	Ø 3.8 mm, GH 1.5 mm	64
J2015.4320	Ø 4.3 mm, GH 2.0 mm	46	J2249.3830	Ø 3.8 mm, GH 3.0 mm	64
J2015.4340	Ø 4.3 mm, GH 4.0 mm	46	J2249.3845	Ø 3.8 mm, GH 4.5 mm	64
J2015.4360	Ø 4.3 mm, GH 6.0 mm	46	J2249.4315	Ø 4.3 mm, GH 1.5 mm	64
J2015.5020	Ø 5.0 mm, GH 2.0 mm	46	J2249.4330	Ø 4.3 mm, GH 3.0 mm	64
J2015.5040	Ø 5.0 mm, GH 4.0 mm	46	J2249.4345	Ø 4.3 mm, GH 4.5 mm	64
J2015.5060	Ø 5.0 mm, GH 6.0 mm	46	J2249.5015	Ø 5.0 mm, GH 1.5 mm	64
J2015.6020	Ø 6.0 mm, GH 2.0 mm	46	J2249.5030	Ø 5.0 mm, GH 3.0 mm	64
J2015.6040	Ø 6.0 mm, GH 4.0 mm	46	J2249.5045	Ø 5.0 mm, GH 4.5 mm	64
J2015.6060	Ø 6.0 mm, GH 6.0 mm	46		Matrix CM Dalbo®-Plus	64
	Healing cap for bar abutment		J2250.0005		
J2029.4300	Ø 3.3/3.8/4.3 mm	61	J2250.0007	Lamella retention insert	65
J2029.6000	Ø 5.0/6.0 mm				

INDEX – ARTICLENUMBERS

Ball abutment sets, incl. male part and matrix CM Dalbo®-Plus			Locator® Abutments		
J2250.3315	Ø 3.3 mm, GH 1.5 mm	64	J2253.3850	Ø 3.8 mm, GH 5.0 mm	65
J2250.3330	Ø 3.3 mm, GH 3.0 mm	64	J2253.4310	Ø 4.3 mm, GH 1.0 mm	65
J2250.3815	Ø 3.8 mm, GH 1.5 mm	64	J2253.4320	Ø 4.3 mm, GH 2.0 mm	65
J2250.3830	Ø 3.8 mm, GH 3.0 mm	64	J2253.4330	Ø 4.3 mm, GH 3.0 mm	65
J2250.3845	Ø 3.8 mm, GH 4.5 mm	64	J2253.4340	Ø 4.3 mm, GH 4.0 mm	65
J2250.4315	Ø 4.3 mm, GH 1.5 mm	64	J2253.4350	Ø 4.3 mm, GH 5.0 mm	65
J2250.4330	Ø 4.3 mm, GH 3.0 mm	64	J2253.5010	Ø 5.0 mm, GH 1.0 mm	65
J2250.4345	Ø 4.3 mm, GH 4.5 mm	64	J2253.5020	Ø 5.0 mm, GH 2.0 mm	65
J2250.5015	Ø 5.0 mm, GH 1.5 mm	64	J2253.5030	Ø 5.0 mm, GH 3.0 mm	65
J2250.5030	Ø 5.0 mm, GH 3.0 mm	64	J2253.5040	Ø 5.0 mm, GH 4.0 mm	65
J2250.5045	Ø 5.0 mm, GH 4.5 mm	64	J2253.5050	Ø 5.0 mm, GH 5.0 mm	65
J2253.0001 Driver for Locator®			J2253.4301 Locator® Fixture for bar abutment		
J2253.0002 Locator® Instrument			J2253.6001 Ø 3.3/3.8/4.3 mm		
J2253.0003 Locator® Angle measurement guide			J2253.6001 Ø 5.0 mm		
J2253.0004 Locator® Parallel post			Bar abutments, straight		
J2253.0102 Locator® Male processing package			J2254.3305 Ø 3.3 mm, GH 0.5 mm		
J2253.0112 Locator® Male processing package for extended range			J2254.3320 Ø 3.3 mm, GH 2.0 mm		
J2253.0200 Locator® Impression cap			J2254.3805 Ø 3.8 mm, GH 0.5 mm		
Locator® Analog			J2254.3820 Ø 3.8 mm, GH 2.0 mm		
J2253.0340 Ø 3.3/3.8/4.3 mm			J2254.3840 Ø 3.8 mm, GH 4.0 mm		
J2253.0350 Ø 5.0/6.0 mm			J2254.4305 Ø 4.3 mm, GH 0.5 mm		
J2253.0401 Locator® Block out spacer			J2254.4320 Ø 4.3 mm, GH 2.0 mm		
J2253.0402 Locator® Processing replacement male			J2254.4340 Ø 4.3 mm, GH 4.0 mm		
Locator® Replacement male			J2254.5005 Ø 5.0 mm, GH 0.5 mm		
J2253.1002 Ø 3.3/3.8/4.3/5.0 mm, blue			J2254.5020 Ø 5.0 mm, GH 2.0 mm		
J2253.1003 Ø 3.3/3.8/4.3/5.0 mm, pink			J2254.5040 Ø 5.0 mm, GH 4.0 mm		
J2253.1005 Ø 3.3/3.8/4.3/5.0 mm, clear			Crown base for bar abutment		
Locator® Replacement male for extended range			J2256.4306 Ø 3.3/3.8/4.3 mm		
J2253.2000 Ø 3.8/4.3/5.0 mm, grey			J2256.6006 Ø 5.0 mm		
J2253.2002 Ø 3.8/4.3/5.0 mm, red			Bases for bar abutment, burn-out		
J2253.2003 Ø 3.8/4.3/5.0 mm, orange			J2257.4301 Ø 3.3/3.8/4.3 mm		
J2253.2004 Ø 3.8/4.3/5.0 mm, green			J2257.6001 Ø 5.0 mm		
Locator® Abutments			Bases for bar abutment, solderable		
J2253.3310 Ø 3.3 mm, GH 1.0 mm			J2258.4300 Ø 3.3/3.8/4.3 mm		
J2253.3320 Ø 3.3 mm, GH 2.0 mm			J2258.6000 Ø 5.0 mm		
J2253.3330 Ø 3.3 mm, GH 3.0 mm			Titanium cap for bar abutment		
J2253.3340 Ø 3.3 mm, GH 4.0 mm			J2259.4301 Ø 3.3/3.8/4.3 mm, for crown		
J2253.3810 Ø 3.8 mm, GH 1.0 mm			J2259.4302 Ø 3.3/3.8/4.3 mm, for bridge		
J2253.3820 Ø 3.8 mm, GH 2.0 mm			J2259.6001 Ø 3.3/3.8/4.3 mm, for crown		
J2253.3830 Ø 3.8 mm, GH 3.0 mm			J2259.6002 Ø 3.3/3.8/4.3 mm, for bridge		
J2253.3840 Ø 3.8 mm, GH 4.0 mm			Titanium bonding bases for bar abutment		
			J2260.4301 Ø 3.3/3.8/4.3 mm		
			J2260.6001 Ø 5.0 mm		

Bar sleeves for titanium bonding bases			Bar lab analog for bar abutments		
J2261.4301	Ø 3.3/3.8/4.3 mm	62	J3020.4300	Ø 3.3/3.8/4.3 mm	61
J2261.6001	Ø 5.0 mm	62	J3020.6000	Ø 5.0 mm	61
Bases for bar abutment, titanium			Reamers for dilating the plaster model, for universal holder		
J2262.4300	Ø 3.3/3.8/4.3 mm	62	J3706.3300	Ø 3.3 mm	74
J2262.6000	Ø 5.0 mm	62	J3706.3800	Ø 3.8 mm	74
Bases for bar abutment, cast-on			J3706.4300	Ø 4.3 mm	74
J2263.4300	Ø 3.3/3.8/4.3 mm	62	J3706.5000	Ø 5.0 mm	74
J2263.6000	Ø 5.0 mm	62	J3706.6000	Ø 6.0 mm	74
J2269.0003	Aligning tool 17°	61	J3709.0010	Universal holder, incl. Lab screw and Abutment collet	74
J2269.0004	Aligning tool 30°	61	J3709.0015	Universal holder	74
Temporary abutment bridge, titanium alloy			Abutment collets		
J2339.3300	Ø 3.3 mm	52	J3709.3300	Ø 3.3 mm	74
J2339.3800	Ø 3.8 mm	52	J3709.3800	Ø 3.8 mm	74
J2339.4300	Ø 4.3 mm	52	J3709.4300	Ø 4.3 mm	74
J2339.5000	Ø 5.0 mm	52	J3709.5000	Ø 5.0 mm	74
J2339.6000	Ø 6.0 mm	52	J3709.6000	Ø 6.0 mm	74
Titanium bases CAD/CAM, bridge			Reworking reamer, for base for bar abutment		
J2344.3348	Ø 3.3 mm	56	J3711.0010	Ø 3.3/3.8/4.3 mm, plane surface	74
J2344.3848	Ø 3.8 mm	56	J3711.0015	Ø 5.0/6.0 mm, plane surface	74
J2344.4348	Ø 4.3 mm	56	J3711.0020	Ø 3.3/3.8/4.3 mm, screw seat	75
J2344.5048	Ø 5.0 mm	56	J3711.0025	Ø 5.0/6.0 mm, screw seat	75
J2344.6048	Ø 6.0 mm	56	Collets for zirconium oxide sleeve		
Logfit® Impression caps			J3712.4300	Ø 3.3/3.8/4.3 mm	74
J2551.4300	Ø 3.8/4.3 mm	55	J3712.6000	Ø 5.0/6.0 mm	74
J2551.6000	Ø 5.0/6.0 mm	55	Guide System Template drill		
Logfit® analog			J3713.3300	Ø 3.3 mm	24
J2552.4300	Ø 3.8/4.3 mm	55	J3713.4300	Ø 3.8/4.3 mm	24
J2552.6000	Ø 5.0/6.0 mm	55	Guide System Guiding sleeves		
Logfit® Plastic copings			J3714.3303	Ø 3.3 mm	23
J2553.4301	Ø 3.8/4.3 mm, for bridges	56	J3714.3803	Ø 3.8 mm	23
J2553.4302	Ø 3.8/4.3 mm, for crowns	56	J3714.4303	Ø 4.3 mm	23
J2553.6001	Ø 5.0/6.0 mm, for bridges	56	Guide System Seating tool		
J2553.6002	Ø 5.0/6.0 mm, for crowns	56	J3716.3300	Ø 3.3 mm	24
Scanning cap for bar abutments			J3716.4300	Ø 3.8/4.3 mm	24
J2610.4300	Ø 3.3/3.8/4.3 mm	61	Lab screw with reduced head, hex		
J2610.6000	Ø 5.0 mm	61	J4004.1600	Ø 3.3/3.8/4.3 mm, M 1.6	63
Ball abutment analogs			J4004.2000	Ø 5.0/6.0 mm, M 2.0	63
J3015.3300	Ø 3.3 mm	65	Abutment screw with reduced head, hex		
J3015.3800	Ø 3.8 mm	65	J4004.1601	Ø 3.3/3.8/4.3 mm, M 1.6	63
J3015.4300	Ø 4.3 mm	65	J4004.2001	Ø 5.0/6.0 mm, M 2.0	63
J3015.5000	Ø 5.0 mm	65			

INDEX – ARTICLENUMBERS

J4005.1601	Abutment screw, hex				
	Ø 3.3/3.8/4.3 mm, M 1.6	59, 69			
J4005.2001	Ø 5.0/6.0 mm, M 2.0	59, 69			
J4006.1601	Lab screw, hex				
	Ø 3.3/3.8/4.3 mm, M 1.6	59, 69			
J4006.2001	Ø 5.0/6.0 mm, M 2.0	59, 69			
J4009.1627	Plastic screw for bar abutment				
	M 1.6	64			
J4009.2027	M 2.0	64			
J4012.1601	Prosthetic screw for bar abutments				
	Ø 3.3/3.8/4.3 mm	63			
J4012.2001	Ø 5.0 mm	63			
J4012.1610	Screw, hex				
	L 10 mm	63			
J4012.1615	L 15 mm	63			
J4012.1620	L 20 mm	63			
J4012.2010	L 10 mm	63			
J4012.2015	L 15 mm	63			
J4012.2020	L 20 mm	63			
J4013.1601	Lab prosthetic screw for bar abutment				
	Ø 3.3/3.8/4.3 mm	63			
J4013.2001	Ø 5.0 mm	63			
J5002.0005	Drill extension Iso shaft				
	for drills with internal irrigation	25			
J5002.0006	not for drills with internal irrigation	34			
J5002.0011	Adapter ISO-shaft	36			
J5002.0012	Cleaning needle	38			
J5002.0020	Cleaning cannula	38			
J5002.3300	Guiding pin for bone profiler				
	Ø 3.3 mm	33			
J5002.3800	Ø 3.8 mm	33			
J5002.4300	Ø 4.3 mm	33			
J5002.5000	Ø 5.0 mm	33			
J5003.3350	Bone profiler				
	Ø 5.0 mm	33			
J5003.4360	Ø 6.0 mm	33			
J5003.5070	Ø 7.0 mm	33			
J5015.0009	Depth stop SCREW-LINE for				
	pilot drill and pre-drill				
J5015.0011	L 9 mm	33			
J5015.0013	L 11 mm	33			
	L 13 mm	33			
J5015.3300	Depth stop for form drill				
	SCREW-LINE and ROOT-LINE 2				
J5015.3800	Ø 3.3 mm	21, 31			
J5015.4300	Ø 3.8 mm	21, 31			
J5015.5000	Ø 4.3 mm	21, 31			
J5015.6000	Ø 5.0 mm	21, 31			
	Ø 6.0 mm	21, 31			
J5041.3300	Guide System Gingiva punches				
	Ø 3.3 mm	23			
J5041.3800	Ø 3.8 mm	23			
J5041.4300	Ø 4.3 mm	23			
J5043.3311	Guide System Pilot drill set				
	Ø 3.3 mm, L 5/9/11 mm	22			
J5043.3313	Ø 3.3 mm, L 5/9/11/13 mm	22			
J5043.4309	Ø 3.8/4.3 mm, L 5/9 mm	22			
J5043.4311	Ø 3.8/4.3 mm, L 5/9/11 mm	22			
J5043.4313	Ø 3.8/4.3 mm, L 5/9/11/13 mm	22			
J5044.3316	Ø 3.3 mm, L 16 mm	22			
J5044.4316	Ø 3.8/4.3 mm, L 16 mm	22			
J5045.3311	Guide System Surgery set, SCREW-LINE				
	Ø 3.3 mm, L 5/9/11 mm	23			
J5045.3313	Ø 3.3 mm, L 5/9/11/13 mm	23			
J5045.3809	Ø 3.8 mm, L 5/9 mm	23			
J5045.3811	Ø 3.8 mm, L 5/9/11 mm	23			
J5045.3813	Ø 3.8 mm, L 5/9/11/13 mm	23			
J5045.4309	Ø 4.3 mm, L 5/9 mm	23			
J5045.4311	Ø 4.3 mm, L 5/9/11 mm	23			
J5045.4313	Ø 4.3 mm, L 5/9/11/13 mm	23			
J5046.3316	Ø 3.3 mm, L 16 mm	23			
J5046.3816	Ø 3.8 mm, L 16 mm	23			
J5046.4316	Ø 4.3 mm, L 16 mm	23			
J5048.3311	Guide System Form drill,				
	SCREW-LINE, Cortical Bone				
J5048.3313	Ø 3.3 mm, L 11 mm	23			
J5048.3316	Ø 3.3 mm, L 13 mm	23			
J5048.3316	Ø 3.3 mm, L 16 mm	23			
J5048.3809	Ø 3.8 mm, L 9 mm	23			
J5048.3811	Ø 3.8 mm, L 11 mm	23			
J5048.3813	Ø 3.8 mm, L 13 mm	23			
J5048.3816	Ø 3.8 mm, L 16 mm	23			
J5048.4309	Ø 4.3 mm, L 9 mm	23			
J5048.4311	Ø 4.3 mm, L 11 mm	23			
J5048.4313	Ø 4.3 mm, L 13 mm	23			
J5048.4316	Ø 4.3 mm, L 16 mm	23			
J5050.2300	Round bur	32			
J5051.2000	Pilot drill SCREW-LINE	32			
J5051.2003	Pilot drill	32			
J5051.2800	Pre-drill SCREW-LINE	32			

Form drill SCREW-LINE Cortical bone			Form drill SCREW-LINE		
J5053.3316	Ø 3.3 mm	21	J5062.5013	Ø 5.0 mm, L 13 mm	21
J5053.3816	Ø 3.8 mm	21	J5062.5016	Ø 5.0 mm, L 16 mm	21
J5053.4316	Ø 4.3 mm	21	J5062.6009	Ø 6.0 mm, L 9 mm	21
J5053.5016	Ø 5.0 mm	21	J5062.6011	Ø 6.0 mm, L 11 mm	21
J5053.6016	Ø 6.0 mm	21	J5062.6013	Ø 6.0 mm, L 13 mm	21
			J5062.6016	Ø 6.0 mm, L 16 mm	21
Tap SCREW-LINE					
J5054.3309	Ø 3.3 mm	21	J5300.0007	Driver for screw implants, with ISO shaft for angled hand piece	34
J5054.3809	Ø 3.8 mm	21			
J5054.4309	Ø 4.3 mm	21	J5300.0008	Driver, short, for screw implants, manuell/wrench	35
J5054.5009	Ø 5.0 mm	21			
J5054.6009	Ø 6.0 mm	21	J5300.0009	Driver, long, for screw implants, manuell/wrench	35
Form drill ROOT-LINE 2					
J5055.3309	Ø 3.3 mm, L 9 mm	31	J5300.0010	Cardanic driver (30°)	36
J5055.3311	Ø 3.3 mm, L 11 mm	31			
J5055.3313	Ø 3.3 mm, L 13 mm	31	J5300.0011	Driver, for ball abutment, manuell/wrench	70
J5055.3316	Ø 3.3 mm, L 16 mm	31			
J5055.3809	Ø 3.8 mm, L 9 mm	31	J5300.0020	Driver for straight bar abutment short, Ø 3.3/3.8/4.3 mm	70
J5055.3811	Ø 3.8 mm, L 11 mm	31			
J5055.3813	Ø 3.8 mm, L 13 mm	31	J5300.0025	Driver for straight bar abutment short, Ø 5.0/6.0 mm	71
J5055.3816	Ø 3.8 mm, L 16 mm	31			
J5055.4309	Ø 4.3 mm, L 9 mm	31	J5300.0027	Driver for impression cap and healing cap for bar abutment, Ø 3.3/3.8/4.3 mm	61, 71
J5055.4311	Ø 4.3 mm, L 11 mm	31			
J5055.4313	Ø 4.3 mm, L 13 mm	31	J5300.0028	Driver for impression cap and healing cap for bar abutment, Ø 5.0/6.0 mm	61, 71
J5055.4316	Ø 4.3 mm, L 16 mm	31			
J5055.5009	Ø 5.0 mm, L 9 mm	31	J5300.0030	PickUp instrument	36
J5055.5011	Ø 5.0 mm, L 11 mm	31			
J5055.5013	Ø 5.0 mm, L 13 mm	31	J5300.0031	Driver, extrashort for screw implants, manuell/wrench	35
J5055.5016	Ø 5.0 mm, L 16 mm	31			
J5055.6009	Ø 6.0 mm, L 9 mm	31	J5300.0032	Driver, short for screw implants, manuell/wrench	35
J5055.6011	Ø 6.0 mm, L 11 mm	31			
J5055.6013	Ø 6.0 mm, L 13 mm	31	J5300.0033	Driver, long for screw implants, manuell/wrench	35
J5055.6016	Ø 6.0 mm, L 16 mm	31			
Tap ROOT-LINE 2			J5300.0034	Driver, short for screw implants, with ISO shaft, manuell/wrench	35
J5056.3309	Ø 3.3 mm	31			
J5056.3809	Ø 3.8 mm	31	J5300.0035	Driver, long for screw implants, with ISO shaft, manuell/wrench	35
J5056.4309	Ø 4.3 mm	31			
J5056.5009	Ø 5.0 mm	31	J5300.0059	Surgery set CAMLOG® ROOT-LINE 2	30
J5056.6009	Ø 6.0 mm	31			
Form drill SCREW-LINE					
J5062.3309	Ø 3.3 mm, L 9 mm	21			
J5062.3311	Ø 3.3 mm, L 11 mm	21			
J5062.3313	Ø 3.3 mm, L 13 mm	21			
J5062.3316	Ø 3.3 mm, L 16 mm	21			
J5062.3809	Ø 3.8 mm, L 9 mm	21			
J5062.3811	Ø 3.8 mm, L 11 mm	21			
J5062.3813	Ø 3.8 mm, L 13 mm	21			
J5062.3816	Ø 3.8 mm, L 16 mm	21			
J5062.4309	Ø 4.3 mm, L 9 mm	21			
J5062.4311	Ø 4.3 mm, L 11 mm	21			
J5062.4313	Ø 4.3 mm, L 13 mm	21			
J5062.4316	Ø 4.3 mm, L 16 mm	21			
J5062.5009	Ø 5.0 mm, L 9 mm	21			
J5062.5011	Ø 5.0 mm, L 11 mm	21			

INDEX – ARTICLENUMBERS

J5300.0061	Surgery set CAMLOG®/ CONELOG® SCREW-LINE	20	J5418.0020	Osteotomy set CAMLOG®/ CONELOG® SCREW-LINE, straight convex	39
J5300.1067	Pattern for Surgery wash tray CAMLOG®/CONELOG® SCREW-LINE	20	J5418.0030	Osteotomy set CAMLOG®/ CONELOG® SCREW-LINE, angled convex	40
J5300.1069	Pattern for Surgery wash tray CAMLOG® ROOT-LINE 2	30		Osteotome SCREW-LINE	
J5300.2028	Paralleling pin SCREW-LINE	34	J5418.3300	Ø 3.3 mm, straight convex	39
J5300.8967	Surgery wash tray CAMLOG®/CONELOG® SCREW-LINE	20	J5418.3310	Ø 3.3 mm, angled convex	40
J5300.8969	Surgery wash tray CAMLOG® ROOT-LINE 2	30	J5418.3800	Ø 3.8 mm, straight convex	39
	Guide System Check-up pin		J5418.3810	Ø 3.8 mm, angled convex	40
J5301.3300	Ø 3.3 mm	25	J5418.4300	Ø 4.3 mm, straight convex	39
J5301.4300	Ø 3.8/4.3 mm	25	J5418.4310	Ø 4.3 mm, angled convex	40
J5302.0010	Holding key for insertion post	36	J5418.5000	Ø 5.0 mm, straight convex	39
	Holding sleeve for screw implants		J5418.5010	Ø 5.0 mm, angled convex	40
J5302.3300	Ø 3.3 mm	37	J5418.6000	Ø 6.0 mm, straight convex	39
J5302.3800	Ø 3.8 mm	37	J5418.6010	Ø 6.0 mm, angled convex	40
J5302.4300	Ø 4.3 mm	37		Pre-Osteotom SCREW-LINE	
	Guide System Driver		J5419.2800	1.7 – 2.8 mm, straight concave	41, 42
J5303.4300	Ø 3.3/3.8/4.3 mm, manuell/wrench	25	J5420.0020	Osteotomy set CAMLOG®/ CONELOG® SCREW-LINE, straight concave	41
J5304.4300	Ø 3.3/3.8/4.3 mm, mit ISO shaft	25	J5420.0030	Osteotomy set CAMLOG®/ CONELOG® SCREW-LINE, angled concave	42
J5315.0005	Screw driver Activator	70		Osteotome SCREW-LINE	
	Screw driver, hex		J5420.3300	Ø 3.3 mm, straight concave	41
J5317.0501	short, manuell/wrench	37, 72	J5420.3310	Ø 3.3 mm, angled concave	42
J5317.0502	long, manuell/wrench	37, 72	J5420.3800	Ø 3.8 mm, straight concave	41
J5317.0503	long, ISO shaft	38, 73	J5420.3810	Ø 3.8 mm, angled concave	42
J5317.0504	short, ISO shaft	38, 73	J5420.4300	Ø 4.3 mm, straight concave	41
J5317.0510	extrashort, manuell/wrench	37, 72	J5420.4310	Ø 4.3 mm, angled concave	42
J5317.0511	Manual screwdriver, hex	38, 73	J5420.5000	Ø 5.0 mm, straight concave	41
J5320.1030	Torque wrench	70	J5420.5010	Ø 5.0 mm, angled concave	42
	Tap Adapter		J5420.6000	Ø 6.0 mm, straight concave	41
J5322.0010	short	34	J5420.6010	Ø 6.0 mm, angled concave	42
J5322.0011	long	34	J8070.2050	Edentulous mandible	78
J5330.8500	Prosthetic tray	72		ROOT-LINE 2 Implant, Promote® plus	
J5330.8700	Prosthetic tray universal	72	K1032.3311	Ø 3.3 mm, L 11 mm	27
	Pre-Osteotom SCREW-LINE,		K1032.3313	Ø 3.3 mm, L 13 mm	27
J5417.2800	1.7 – 2.8 mm, straight convex	39, 40	K1032.3316	Ø 3.3 mm, L 16 mm	27
			K1032.3809	Ø 3.8 mm, L 9 mm	27
			K1032.3811	Ø 3.8 mm, L 11 mm	27
			K1032.3813	Ø 3.8 mm, L 13 mm	27
			K1032.3816	Ø 3.8 mm, L 16 mm	27
			K1032.4309	Ø 4.3 mm, L 9 mm	27
			K1032.4311	Ø 4.3 mm, L 11 mm	27
			K1032.4313	Ø 4.3 mm, L 13 mm	27
			K1032.4316	Ø 4.3 mm, L 16 mm	27
			K1032.5009	Ø 5.0 mm, L 9 mm	27

	ROOT-LINE 2 Implant, Promote® plus	
K1032.5011	Ø 5.0 mm, L 11 mm	27
K1032.5013	Ø 5.0 mm, L 13 mm	27
K1032.5016	Ø 5.0 mm, L 16 mm	27
K1032.6009	Ø 6.0 mm, L 9 mm	27
K1032.6011	Ø 6.0 mm, L 11 mm	27
K1032.6013	Ø 6.0 mm, L 13 mm	27
K1032.6016	Ø 6.0 mm, L 16 mm	27

	ROOT-LINE 2 Implant for practice	
K1039.3813	Ø 3.8 mm, L 13 mm	78
K1039.4313	Ø 4.3 mm, L 13 mm	78

	SCREW-LINE Implant, Promote®	
K1044.3311	Ø 3.3 mm, L 11 mm	17
K1044.3313	Ø 3.3 mm, L 13 mm	17
K1044.3316	Ø 3.3 mm, L 16 mm	17
K1044.3809	Ø 3.8 mm, L 9 mm	17
K1044.3811	Ø 3.8 mm, L 11 mm	17
K1044.3813	Ø 3.8 mm, L 13 mm	17
K1044.3816	Ø 3.8 mm, L 16 mm	17
K1044.4309	Ø 4.3 mm, L 9 mm	17
K1044.4311	Ø 4.3 mm, L 11 mm	17
K1044.4313	Ø 4.3 mm, L 13 mm	17
K1044.4316	Ø 4.3 mm, L 16 mm	17
K1044.5009	Ø 5.0 mm, L 9 mm	17
K1044.5011	Ø 5.0 mm, L 11 mm	17
K1044.5013	Ø 5.0 mm, L 13 mm	17
K1044.5016	Ø 5.0 mm, L 16 mm	17
K1044.6009	Ø 6.0 mm, L 9 mm	17
K1044.6011	Ø 6.0 mm, L 11 mm	17
K1044.6013	Ø 6.0 mm, L 13 mm	17
K1044.6016	Ø 6.0 mm, L 16 mm	17

	SCREW-LINE Implant for practice	
K1049.3813	Ø 3.8 mm, L 13 mm	78
K1049.4313	Ø 4.3 mm, L 13 mm	78

	Guide System CAMLOG®	
	SCREW-LINE Implant Promote® plus	
K1053.3311	Ø 3.3 mm, L 11 mm	22
K1053.3313	Ø 3.3 mm, L 13 mm	22
K1053.3316	Ø 3.3 mm, L 16 mm	22
K1053.3809	Ø 3.8 mm, L 9 mm	22
K1053.3811	Ø 3.8 mm, L 11 mm	22
K1053.3813	Ø 3.8 mm, L 13 mm	22
K1053.3816	Ø 3.8 mm, L 16 mm	22
K1053.4309	Ø 4.3 mm, L 9 mm	22
K1053.4311	Ø 4.3 mm, L 11 mm	22
K1053.4313	Ø 4.3 mm, L 13 mm	22
K1053.4316	Ø 4.3 mm, L 16 mm	22

	SCREW-LINE Implant, Promote® plus	
K1054.3311	Ø 3.3 mm, L 11 mm	17
K1054.3313	Ø 3.3 mm, L 13 mm	17
K1054.3316	Ø 3.3 mm, L 16 mm	17
K1054.3809	Ø 3.8 mm, L 9 mm	17
K1054.3811	Ø 3.8 mm, L 11 mm	17

	SCREW-LINE Implant, Promote® plus	
K1054.3813	Ø 3.8 mm, L 13 mm	17
K1054.3816	Ø 3.8 mm, L 16 mm	17
K1054.4309	Ø 4.3 mm, L 9 mm	17
K1054.4311	Ø 4.3 mm, L 11 mm	17
K1054.4313	Ø 4.3 mm, L 13 mm	17
K1054.4316	Ø 4.3 mm, L 16 mm	17
K1054.5009	Ø 5.0 mm, L 9 mm	17
K1054.5011	Ø 5.0 mm, L 11 mm	17
K1054.5013	Ø 5.0 mm, L 13 mm	17
K1054.5016	Ø 5.0 mm, L 16 mm	17
K1054.6009	Ø 6.0 mm, L 9 mm	17
K1054.6011	Ø 6.0 mm, L 11 mm	17
K1054.6013	Ø 6.0 mm, L 13 mm	17
K1054.6016	Ø 6.0 mm, L 16 mm	17

	Healing cap PS, bottleneck	
K2001.3840	Ø 3.8 mm, GH 4.0 mm	47
K2001.3860	Ø 3.8 mm, GH 6.0 mm	47
K2001.4340	Ø 4.3 mm, GH 4.0 mm	47
K2001.4360	Ø 4.3 mm, GH 6.0 mm	47
K2001.5040	Ø 5.0 mm, GH 4.0 mm	47
K2001.5060	Ø 5.0 mm, GH 6.0 mm	47

	Healing cap PS, wide body	
K2004.3840	Ø 3.8 mm, GH 4.0 mm	47
K2004.3860	Ø 3.8 mm, GH 6.0 mm	47
K2004.4340	Ø 4.3 mm, GH 4.0 mm	47
K2004.4360	Ø 4.3 mm, GH 6.0 mm	47
K2004.5040	Ø 5.0 mm, GH 4.0 mm	47
K2004.5060	Ø 5.0 mm, GH 6.0 mm	47
K2004.6040	Ø 6.0 mm, GH 4.0 mm	47
K2004.6060	Ø 6.0 mm, GH 6.0 mm	47

	Healing cap PS, cylindrical	
K2005.3820	Ø 3.8 mm, GH 2.0 mm	47
K2005.3840	Ø 3.8 mm, GH 4.0 mm	47
K2005.3860	Ø 3.8 mm, GH 6.0 mm	47
K2005.4320	Ø 4.3 mm, GH 2.0 mm	47
K2005.4340	Ø 4.3 mm, GH 4.0 mm	47
K2005.4360	Ø 4.3 mm, GH 6.0 mm	47
K2005.5020	Ø 5.0 mm, GH 2.0 mm	47
K2005.5040	Ø 5.0 mm, GH 4.0 mm	47
K2005.5060	Ø 5.0 mm, GH 6.0 mm	47
K2005.6020	Ø 6.0 mm, GH 2.0 mm	47
K2005.6040	Ø 6.0 mm, GH 4.0 mm	47
K2005.6060	Ø 6.0 mm, GH 6.0 mm	47

	Guide System CAMLOG® Insertion post	
K2026.3300	Ø 3.3 mm	24
K2026.3800	Ø 3.8 mm	24
K2026.4300	Ø 4.3 mm	24

INDEX – ARTICLENUMBERS

Impression posts PS, closed tray, for Platform Switching			Temporary abutments PS, PEEK, for Platform Switching		
K2109.3800	Ø 3.8 mm	50	K2208.3800	Ø 3.8 mm	52
K2109.4300	Ø 4.3 mm	50	K2208.4300	Ø 4.3 mm	52
K2109.5000	Ø 5.0 mm	50	K2208.5000	Ø 5.0 mm	52
K2109.6000	Ø 6.0 mm	50	K2208.6000	Ø 6.0 mm	52
Impression posts, closed tray			Universal abutment		
K2110.3300	Ø 3.3 mm	50	K2211.3300	Ø 3.3 mm	54, 68
K2110.3800	Ø 3.8 mm	50	K2211.3800	Ø 3.8 mm	54, 68
K2110.4300	Ø 4.3 mm	50	K2211.4300	Ø 4.3 mm	54, 68
K2110.5000	Ø 5.0 mm	50	K2211.5000	Ø 5.0 mm	54, 68
K2110.6000	Ø 6.0 mm	50	K2211.6000	Ø 6.0 mm	54, 68
Impression posts PS, open tray, for Platform Switching			Telescope abutments for double crown restorations		
K2119.3800	Ø 3.8 mm	50	K2212.3800	Ø 3.8 mm	68
K2119.4300	Ø 4.3 mm	50	K2212.4300	Ø 4.3 mm	68
K2119.5000	Ø 5.0 mm	50	K2212.5000	Ø 5.0 mm	68
K2119.6000	Ø 6.0 mm	50	K2212.6000	Ø 6.0 mm	68
Impression posts, open tray			Esthomic® Abutments, straight		
K2121.3300	Ø 3.3 mm	50	K2226.3810	Ø 3.8 mm, GH 1.0 – 1.8 mm	52
K2121.3800	Ø 3.8 mm	50	K2226.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm	52
K2121.4300	Ø 4.3 mm	50	K2226.4310	Ø 4.3 mm, GH 1.0 – 1.8 mm	52
K2121.5000	Ø 5.0 mm	50	K2226.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm	52
K2121.6000	Ø 6.0 mm	50	K2226.5010	Ø 5.0 mm, GH 1.0 – 1.8 mm	52
Universal abutment PS			K2226.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm	52
K2201.3800	Ø 3.8 mm	54, 68	K2226.6010	Ø 6.0 mm, GH 1.0 – 1.8 mm	52
K2201.4300	Ø 4.3 mm	54, 68	K2226.6030	Ø 6.0 mm, GH 3.0 – 4.5 mm	52
K2201.5000	Ø 5.0 mm	54, 68	Esthomic® Abutments, 15° angled, type A		
K2201.6000	Ø 6.0 mm	54, 68	K2227.3810	Ø 3.8 mm, GH 1.0 – 1.8 mm	52
Esthomic® Abutments PS, straight for Platform Switching			K2227.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm	52
K2202.3815	Ø 3.8 mm	53	K2227.4310	Ø 4.3 mm, GH 1.0 – 1.8 mm	52
K2202.4315	Ø 4.3 mm	53	K2227.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm	52
K2202.5015	Ø 5.0 mm	53	K2227.5010	Ø 5.0 mm, GH 1.0 – 1.8 mm	52
K2202.6015	Ø 6.0 mm	53	K2227.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm	52
Esthomic® Abutments PS, 15° angled, type A, for Platform Switching			K2227.6010	Ø 6.0 mm, GH 1.0 – 1.8 mm	52
K2203.3815	Ø 3.8 mm	53	K2227.6030	Ø 6.0 mm, GH 3.0 – 4.5 mm	52
K2203.4315	Ø 4.3 mm	53	Esthomic® Abutments, 15° angled, type B		
K2203.5015	Ø 5.0 mm	53	K2228.3810	Ø 3.8 mm, GH 1.0 – 1.8 mm	53
K2203.6015	Ø 6.0 mm	53	K2228.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm	53
Esthomic® Abutments PS, 15° angled, type B, for Platform Switching			K2228.4310	Ø 4.3 mm, GH 1.0 – 1.8 mm	53
K2204.3815	Ø 3.8 mm	53	K2228.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm	53
K2204.4315	Ø 4.3 mm	53	K2228.5010	Ø 5.0 mm, GH 1.0 – 1.8 mm	53
K2204.5015	Ø 5.0 mm	53	K2228.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm	53
K2204.6015	Ø 6.0 mm	53	K2228.6010	Ø 6.0 mm, GH 1.0 – 1.8 mm	53
			K2228.6030	Ø 6.0 mm, GH 3.0 – 4.5 mm	53

	Esthomic® Abutments, 20° angled, type A			Titanium bases CAD/CAM, crown	
K2231.3810	Ø 3.8 mm, GH 1.0 – 1.8 mm	53	K2244.3348	Ø 3.3 mm	56
K2231.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm	53	K2244.3848	Ø 3.8 mm	56
K2231.4310	Ø 4.3 mm, GH 1.0 – 1.8 mm	53	K2244.4348	Ø 4.3 mm	56
K2231.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm	53	K2244.5048	Ø 5.0 mm	56
K2231.5010	Ø 5.0 mm, GH 1.0 – 1.8 mm	53	K2244.6048	Ø 6.0 mm	56
K2231.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm	53		Gold-plastic abutment	
K2231.6010	Ø 6.0 mm, GH 1.0 – 1.8 mm	53	K2246.3300	Ø 3.3 mm	54
K2231.6030	Ø 6.0 mm, GH 3.0 – 4.5 mm	53	K2246.3800	Ø 3.8 mm	54
	Esthomic® Abutments, 20° angled, type B		K2246.4300	Ø 4.3 mm	54
K2232.3810	Ø 3.8 mm, GH 1.0 – 1.8 mm	53	K2246.5000	Ø 5.0 mm	54
K2232.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm	53	K2246.6000	Ø 6.0 mm	54
K2232.4310	Ø 4.3 mm, GH 1.0 – 1.8 mm	53		Bar abutment	
K2232.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm	53		17° angled, type A	
K2232.5010	Ø 5.0 mm, GH 1.0 – 1.8 mm	53	K2256.3325	Ø 3.3 mm, GH 2.5	60
K2232.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm	53	K2256.3340	Ø 3.3 mm, GH 4.0	60
K2232.6010	Ø 6.0 mm, GH 1.0 – 1.8 mm	53	K2256.3825	Ø 3.8 mm, GH 2.5	60
K2232.6030	Ø 6.0 mm, GH 3.0 – 4.5 mm	53	K2256.3840	Ø 3.8 mm, GH 4.0	60
	Esthomic® Abutments, Inset		K2256.4325	Ø 4.3 mm, GH 2.5	60
K2235.3315	Ø 3.3 mm, GH 1.5 – 2.8 mm	53	K2256.4340	Ø 4.3 mm, GH 4.0	60
K2235.3815	Ø 3.8 mm, GH 1.5 – 2.8 mm	53	K2256.5025	Ø 5.0 mm, GH 2.5	60
K2235.4315	Ø 4.3 mm, GH 1.5 – 2.8 mm	53	K2256.5040	Ø 5.0 mm, GH 4.0	60
K2235.5015	Ø 5.0 mm, GH 1.5 – 2.8 mm	53		Bar abutment,	
K2235.6015	Ø 6.0 mm, GH 1.5 – 2.8 mm	53		17° angled, type B	
	Temporary abutments, crown, titanium alloy		K2257.3325	Ø 3.3 mm, GH 2.5	60
K2239.3300	Ø 3.3 mm	52	K2257.3340	Ø 3.3 mm, GH 4.0	60
K2239.3800	Ø 3.8 mm	52	K2257.3825	Ø 3.8 mm, GH 2.5	60
K2239.4300	Ø 4.3 mm	52	K2257.3840	Ø 3.8 mm, GH 4.0	60
K2239.5000	Ø 5.0 mm	52	K2257.4325	Ø 4.3 mm, GH 2.5	60
K2239.6000	Ø 6.0 mm	52	K2257.4340	Ø 4.3 mm, GH 4.0	60
	Temporary abutments, PEEK		K2257.5025	Ø 5.0 mm, GH 2.5	60
K2241.3800	Ø 3.8 mm	52	K2257.5040	Ø 5.0 mm, GH 4.0	60
K2241.4300	Ø 4.3 mm	52		Bar abutment,	
K2241.5000	Ø 5.0 mm	52	K2258.3325	Ø 3.3 mm, GH 2.5	60
K2241.6000	Ø 6.0 mm	52	K2258.3340	Ø 3.3 mm, GH 4.0	60
	Ceramic abutments, 2-parts, for bonded/cemented full ceramic crowns		K2258.3825	Ø 3.8 mm, GH 2.5	60
K2242.3340	Ø 3.3 mm	54	K2258.3840	Ø 3.8 mm, GH 4.0	60
K2242.3840	Ø 3.8 mm	54	K2258.4325	Ø 4.3 mm, GH 2.5	60
K2242.4340	Ø 4.3 mm	54	K2258.4340	Ø 4.3 mm, GH 4.0	60
K2242.5040	Ø 5.0 mm	54	K2258.5035	Ø 5.0 mm, GH 3.5	60
K2242.6040	Ø 6.0 mm	54	K2258.5050	Ø 5.0 mm, GH 5.0	60
	Titanium bases for CAMLOG® Ceramic abutment			Bar abutment,	
K2242.3342	Ø 3.3 mm	55	K2259.3325	Ø 3.3 mm, GH 2.5	60
K2242.3842	Ø 3.8 mm	55	K2259.3340	Ø 3.3 mm, GH 4.0	60
K2242.4342	Ø 4.3 mm	55	K2259.3825	Ø 3.8 mm, GH 2.5	60
K2242.5042	Ø 5.0 mm	55	K2259.3840	Ø 3.8 mm, GH 4.0	60
K2242.6042	Ø 6.0 mm	55	K2259.4325	Ø 4.3 mm, GH 2.5	60
			K2259.4340	Ø 4.3 mm, GH 4.0	60
			K2259.5035	Ø 5.0 mm, GH 3.5	60
			K2259.5050	Ø 5.0 mm, GH 5.0	60

INDEX – ARTICLENUMBERS

CAM Titanium Blank, type IAC			K5300.9013 X-Ray Planning foil 1.4:1 CAMLOG® ROOT-LINE 2 Implants			14
K2411.3313	Ø 3.3 mm	58	X-Ray Transfer pictures 1.25:1 CAMLOG® ROOT-LINE 2 Implants			
K2411.3813	Ø 3.8 mm	58	K5300.9070	Ø 3.3 mm		14
K2411.4313	Ø 4.3 mm	58	K5300.9071	Ø 3.8 mm		14
K2411.6013	Ø 5.0/6.0 mm	58	K5300.9072	Ø 4.3 mm		14
CAM Titanium Blank, type ME			K5300.9073	Ø 5.0 mm		14
K2421.3320	Ø 3.3 mm	58	K5300.9074	Ø 6.0 mm		14
K2421.3820	Ø 3.8 mm	58	X-Ray Transfer pictures 1.25:1 CAMLOG® SCREW-LINE Implants			
K2421.4320	Ø 4.3 mm	58	K5300.9080	Ø 3.3 mm		14
K2421.5020	Ø 5.0 mm	58	K5300.9081	Ø 3.8 mm		14
K2421.6020	Ø 6.0 mm	58	K5300.9082	Ø 4.3 mm		14
Logfit® Abutments			K5300.9083	Ø 5.0 mm		14
K2550.3808	Ø 3.8 mm, GH 0.8 mm	55	K5300.9084	Ø 6.0 mm		14
K2550.3815	Ø 3.8 mm, GH 1.5 mm	55	Adapter for screw implants, long			
K2550.4308	Ø 4.3 mm, GH 0.8 mm	55	K5302.3310	Ø 3.3 mm		37
K2550.4315	Ø 4.3 mm, GH 1.5 mm	55	K5302.3810	Ø 3.8 mm		37
K2550.5008	Ø 5.0 mm, GH 0.8 mm	55	K5302.4310	Ø 4.3 mm		37
K2550.5015	Ø 5.0 mm, GH 1.5 mm	55	K8010.1010	SCREW-LINE Macro model		79
K2550.6008	Ø 6.0 mm, GH 0.8 mm	55	K8010.1011	ROOT-LINE 2 Macro model		79
K2550.6015	Ø 6.0 mm, GH 1.5 mm	55	K8011.1000	Selection abutment kit		75
Scanbodies			Demonstration model, acrylic glass			
K2610.3310	Ø 3.3 mm	57	K8050.1040	lower jaw		78
K2610.3810	Ø 3.8 mm	57	K8070.1020	upper jaw		78
K2610.4310	Ø 4.3 mm	57	M1000.0050	ALTApin magazine (1 units)		45
K2610.6010	Ø 5.0/6.0 mm	57	M1000.0100	ALTApin magazine (3 units)		45
ScanPosts for Sirona Scanbody			M5100.0010	ALTApin applicator, straight		43
K2620.3306	Ø 3.3 mm	57	M5100.0030	ALTApin applicator, angled 90°		43
K2620.3806	Ø 3.8 mm	57	M5100.0050	ALTApin pricker		44
K2620.4306	Ø 4.3 mm	57	M5100.0070	ALTApin membrane fixator		44
K2620.5006	Ø 5.0 mm	57	M5100.0100	ALTApin surgery mallet		45
K2620.6006	Ø 6.0 mm	57	M5200.0010	ALTApin applicator, straight, work element		44
Lab analogs			M5200.0055	ALTApin pricker, insert		45
K3010.3300	Ø 3.3 mm	51	M5500.0050	ALTApin single patient drill, ISO shaft		45
K3010.3800	Ø 3.8 mm	51	M5600.0110	ALTApin set		43
K3010.4300	Ø 4.3 mm	51	M5600.0210	ALTApin Tray		43
K3010.5000	Ø 5.0 mm	51				
K3010.6000	Ø 6.0 mm	51				
Collet for CAM Blank, type IAC						
K3720.3300	Ø 3.3 mm	58				
K3720.3800	Ø 3.8 mm	58				
K3720.4300	Ø 4.3 mm	58				
K3720.6000	Ø 5.0/6.0 mm	58				
K5300.9010	X-Ray Planning foil 1.25:1 CAMLOG® SCREW-LINE Implants	14				
K5300.9011	X-Ray Planning foil 1.4:1 CAMLOG® SCREW-LINE Implants	14				
K5300.9012	X-Ray Planning foil 1.25:1 CAMLOG® ROOT-LINE 2 Implants	14				

FURTHER DOCUMENTATION

FURTHER INFORMATION ON THE CAMLOG® PRODUCTS CAN BE FOUND IN THE FOLLOWING DOCUMENTS:

- CAMLOG® Product catalog
- CAMLOG® Working instructions
- CAMLOG® Instruction manuals
- Preparation instructions
- CAMLOG literature overview
- CAMLOG and science

The documents are available from the local CAMLOG representative.

See also:

<http://ifu.camlog.com>

www.camlog.com

TRADEMARKS AND COPYRIGHT

Protected brand names (trademarks) are not specially indicated. The absence of such indication does not mean that it is not a trademarked name. This publication with all its parts is protected by copyright. Any exploitation beyond the narrow limits of the copyright act is not permissible without the approval of CAMLOG Biotechnologies AG and is subject to legal sanctions.

CE0123

Art.-No. J8001.0003 Rev.4 03/2017



HEADQUARTERS

CAMLOG Biotechnologies AG | Margarethenstr. 38 | 4053 Basel | Switzerland
Phone +41 61 565 41 00 | Fax +41 61 565 41 01 | info@camlog.com | www.camlog.com

Manufacturer CAMLOG® and CONELOG® Products: ALTATEC GmbH | Maybachstr. 5 | 71299 Wimsheim | Germany

camlog